

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020030.D
 Acq On : 15 Jan 2021 17:44
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	78	rVB	184981	190274	13.17%	1.630%
2	1.569	142	149	159	rBV	180532	200931	13.91%	1.722%
3	2.110	307	317	344	rVB	363797	560021	38.76%	4.799%
4	2.727	507	509	512	rBV2	411	273	0.02%	0.002%
5	2.756	512	518	521	rBV6	1172	1128	0.08%	0.010%
6	2.913	564	567	569	rBV4	1015	581	0.04%	0.005%
7	2.946	575	577	582	rVB3	643	359	0.02%	0.003%
8	2.965	582	583	586	rBV2	473	219	0.02%	0.002%
9	3.029	598	603	604	rBV3	1360	941	0.07%	0.008%
10	3.167	643	646	648	rBV3	646	504	0.03%	0.004%
11	3.203	653	657	659	rBV4	524	420	0.03%	0.004%
12	3.267	675	677	679	rBV2	623	348	0.02%	0.003%
13	3.286	679	683	684	rVV2	791	493	0.03%	0.004%
14	3.402	715	719	722	rBV3	567	554	0.04%	0.005%
15	3.447	731	733	736	rBV3	643	376	0.03%	0.003%
16	3.502	747	750	753	rVB4	542	355	0.02%	0.003%
17	3.518	753	755	759	rBV2	495	280	0.02%	0.002%
18	3.605	779	782	783	rBV2	670	302	0.02%	0.003%
19	3.669	801	802	805	rVB2	866	301	0.02%	0.003%
20	3.688	805	808	813	rVB4	842	774	0.05%	0.007%
21	3.714	813	816	821	rVB3	540	343	0.02%	0.003%
22	3.756	825	829	830	rBV4	692	451	0.03%	0.004%
23	3.827	849	851	853	rVB	677	274	0.02%	0.002%
24	3.894	861	872	900	rBV	111879	334257	23.13%	2.864%
25	4.354	998	1015	1042	rBV	246251	606695	41.99%	5.199%
26	4.663	1109	1111	1114	rBV3	620	346	0.02%	0.003%
27	4.765	1140	1143	1146	rBV3	636	450	0.03%	0.004%
28	4.791	1148	1151	1153	rBV4	758	439	0.03%	0.004%
29	4.820	1158	1160	1164	rVB3	846	476	0.03%	0.004%
30	4.843	1164	1167	1170	rBV4	696	607	0.04%	0.005%
31	4.875	1173	1177	1178	rBV2	407	297	0.02%	0.003%
32	4.917	1186	1190	1192	rBV3	520	487	0.03%	0.004%
33	5.052	1214	1232	1256	rBV2	556706	1444877	100.00%	12.381%
34	5.351	1323	1325	1327	rBV4	713	384	0.03%	0.003%
35	5.396	1337	1339	1341	rBV3	715	296	0.02%	0.003%
36	5.521	1375	1378	1381	rBV5	733	493	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020030.D
 Acq On : 15 Jan 2021 17:44
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.621	1396	1409	1438	rBV	468359	954624	66.07%	8.180%
38	5.910	1490	1499	1514	rVB2	24565	48545	3.36%	0.416%
39	5.981	1519	1521	1525	rBV3	880	400	0.03%	0.003%
40	6.074	1537	1550	1575	rBV	335455	677645	46.90%	5.807%
41	6.322	1625	1627	1629	rBV2	540	266	0.02%	0.002%
42	6.386	1644	1647	1653	rVB6	1096	858	0.06%	0.007%
43	6.412	1653	1655	1658	rBV3	657	349	0.02%	0.003%
44	6.454	1666	1668	1671	rVB3	772	338	0.02%	0.003%
45	6.582	1706	1708	1711	rBV2	521	274	0.02%	0.002%
46	6.634	1717	1724	1725	rBV4	1518	1450	0.10%	0.012%
47	6.733	1752	1755	1757	rBV3	949	612	0.04%	0.005%
48	6.791	1768	1773	1775	rBV5	749	711	0.05%	0.006%
49	6.855	1789	1793	1796	rVB2	538	367	0.03%	0.003%
50	6.900	1804	1807	1811	rVB5	725	514	0.04%	0.004%
51	6.990	1824	1835	1854	rBV	174077	314248	21.75%	2.693%
52	7.322	1925	1938	1964	rBV	638057	1108935	76.75%	9.502%
53	7.627	2022	2033	2050	rBV	122453	214258	14.83%	1.836%
54	7.974	2139	2141	2144	rBV3	582	363	0.03%	0.003%
55	8.048	2162	2164	2167	rBV4	608	267	0.02%	0.002%
56	8.093	2167	2178	2212	rBV2	374864	743196	51.44%	6.368%
57	8.550	2318	2320	2324	rBV3	582	510	0.04%	0.004%
58	8.656	2351	2353	2356	rBV3	485	357	0.02%	0.003%
59	8.762	2384	2386	2388	rBV3	526	272	0.02%	0.002%
60	8.859	2404	2416	2442	rBV	738875	1205152	83.41%	10.327%
61	9.068	2478	2481	2484	rBV4	1179	717	0.05%	0.006%
62	9.100	2489	2491	2493	rVB2	744	319	0.02%	0.003%
63	9.196	2519	2521	2524	rBV3	542	312	0.02%	0.003%
64	9.248	2532	2537	2540	rBV3	956	935	0.06%	0.008%
65	9.280	2545	2547	2550	rBV2	517	341	0.02%	0.003%
66	9.595	2642	2645	2647	rVB3	800	401	0.03%	0.003%
67	9.662	2663	2666	2670	rBV4	794	529	0.04%	0.005%
68	9.756	2693	2695	2700	rVB2	780	571	0.04%	0.005%
69	9.785	2700	2704	2705	rBV3	500	343	0.02%	0.003%
70	9.801	2705	2709	2710	rBV2	408	279	0.02%	0.002%
71	9.855	2723	2726	2727	rBV2	530	295	0.02%	0.003%
72	9.887	2733	2736	2739	rBV4	841	640	0.04%	0.005%
73	10.032	2777	2781	2784	rBV4	971	791	0.05%	0.007%
74	10.116	2804	2807	2811	rVB5	833	608	0.04%	0.005%
75	10.148	2811	2817	2820	rBV5	1013	990	0.07%	0.008%
76	10.222	2828	2840	2856	rBV	437066	686856	47.54%	5.886%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020030.D
 Acq On : 15 Jan 2021 17:44
 Operator : SY/MD
 Sample : VIBLK81
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.505	2923	2928	2929	rBV4	626	549	0.04%	0.005%
78	10.543	2938	2940	2941	rBV2	513	254	0.02%	0.002%
79	10.740	2998	3001	3002	rBV	591	295	0.02%	0.003%
80	10.788	3014	3016	3019	rVB4	653	287	0.02%	0.002%
81	10.810	3019	3023	3024	rBV4	588	347	0.02%	0.003%
82	10.858	3036	3038	3044	rVB4	733	537	0.04%	0.005%
83	10.884	3044	3046	3049	rBV3	448	282	0.02%	0.002%
84	11.254	3149	3161	3184	rBV	786467	1223576	84.68%	10.485%
85	11.440	3215	3219	3224	rBV7	911	872	0.06%	0.007%
86	11.524	3241	3245	3247	rBV3	845	573	0.04%	0.005%
87	11.630	3266	3278	3298	rBV	706923	1116067	77.24%	9.563%
88	11.923	3366	3369	3370	rBV2	584	297	0.02%	0.003%
89	11.974	3383	3385	3392	rVB5	978	824	0.06%	0.007%
90	12.129	3431	3433	3435	rBV2	711	365	0.03%	0.003%
91	12.733	3619	3621	3626	rVB3	729	592	0.04%	0.005%
92	12.932	3681	3683	3686	rBV	741	510	0.04%	0.004%
93	13.064	3719	3724	3726	rBV4	748	554	0.04%	0.005%
94	13.141	3746	3748	3751	rVB4	783	470	0.03%	0.004%
95	13.161	3751	3754	3758	rVB3	748	530	0.04%	0.005%
96	13.183	3759	3761	3762	rBV	656	226	0.02%	0.002%
97	13.241	3775	3779	3780	rBV	786	476	0.03%	0.004%
98	13.273	3787	3789	3794	rVB5	936	642	0.04%	0.006%
99	13.556	3875	3877	3880	rBV3	713	530	0.04%	0.005%
100	13.977	4005	4008	4013	rBV3	605	559	0.04%	0.005%




Sum of corrected areas: 11670258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020030.D
Acq On : 15 Jan 2021 17:44
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

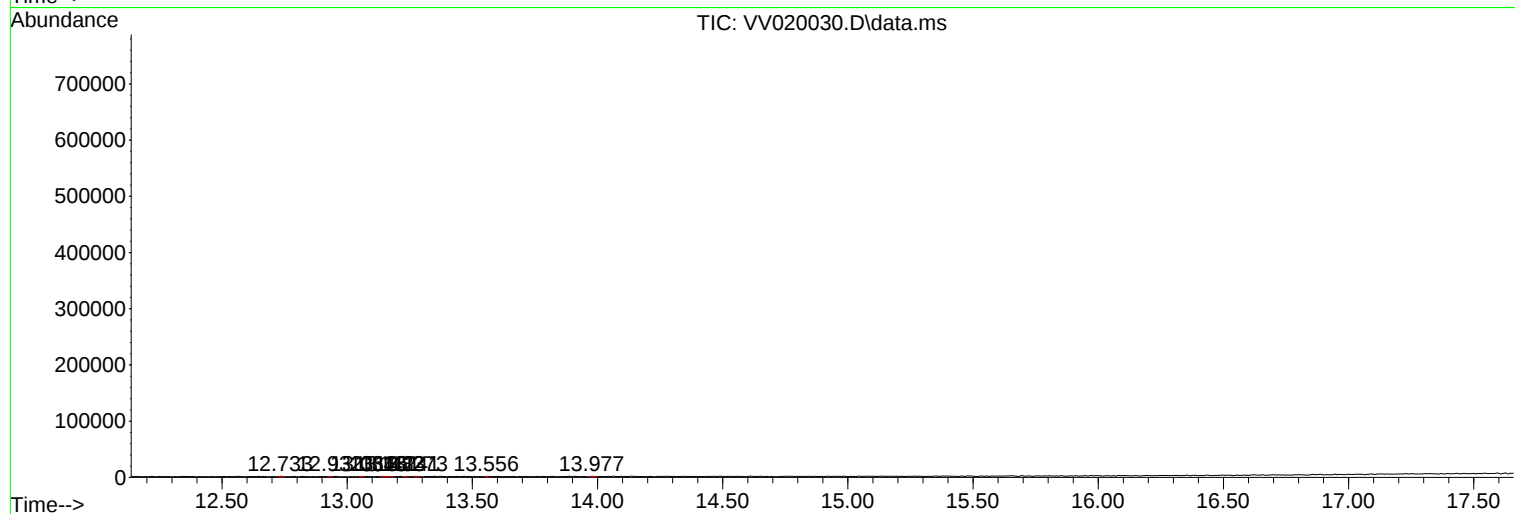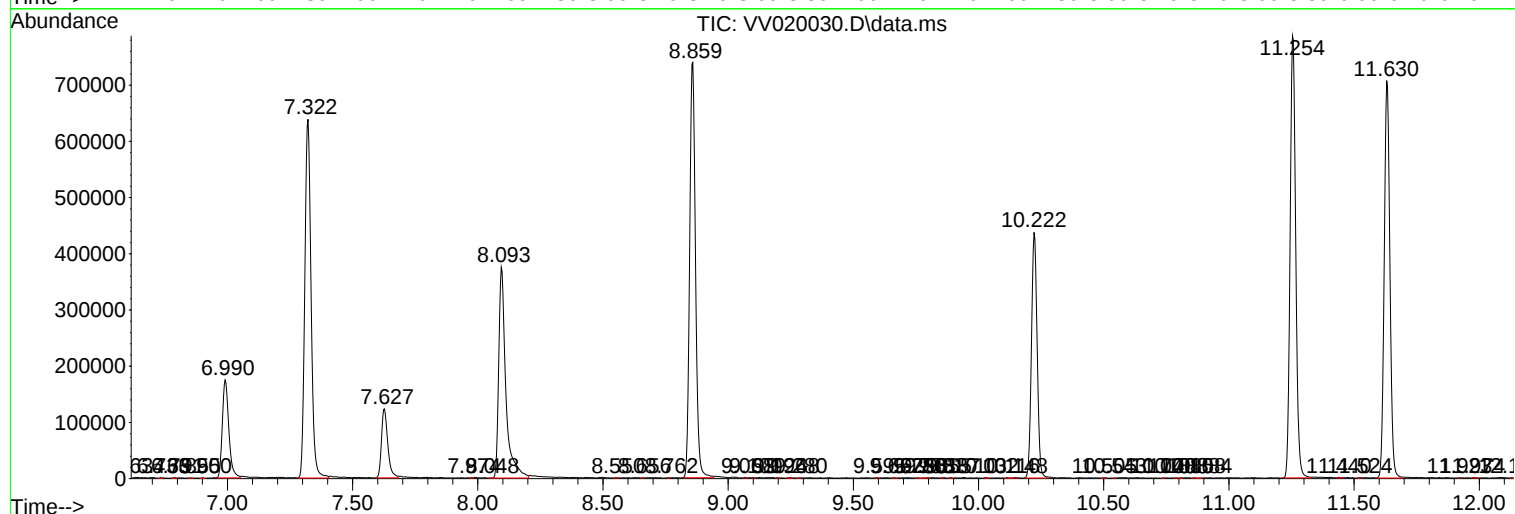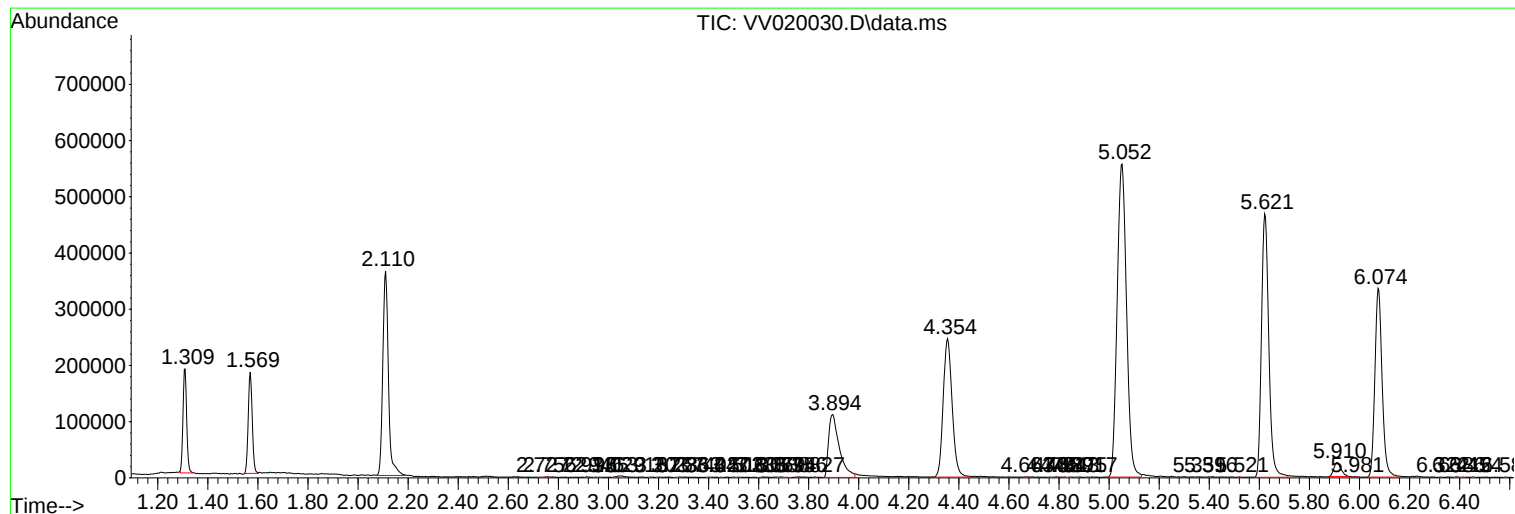

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020030.D
Acq On : 15 Jan 2021 17:44
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020030.D
Acq On : 15 Jan 2021 17:44
Operator : SY/MD
Sample : VIBLK81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
