

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020031.D
 Acq On : 15 Jan 2021 18:07
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	181337	184683	13.05%	1.603%
2	1.569	142	149	162	rBV	171360	193121	13.65%	1.676%
3	2.110	308	317	347	rVB	356081	547915	38.72%	4.755%
4	2.704	500	502	505	rBV3	679	357	0.03%	0.003%
5	2.733	508	511	512	rBV2	779	442	0.03%	0.004%
6	2.904	561	564	566	rVB3	541	330	0.02%	0.003%
7	3.103	623	626	629	rVB3	730	529	0.04%	0.005%
8	3.126	629	633	637	rBV5	927	811	0.06%	0.007%
9	3.177	644	649	650	rBV2	646	425	0.03%	0.004%
10	3.299	683	687	689	rVB2	676	492	0.03%	0.004%
11	3.322	689	694	698	rBV3	791	745	0.05%	0.006%
12	3.367	703	708	709	rBV4	538	354	0.03%	0.003%
13	3.595	778	779	784	rBV3	571	595	0.04%	0.005%
14	3.675	798	804	806	rBV3	793	876	0.06%	0.008%
15	3.746	823	826	827	rBV	525	343	0.02%	0.003%
16	3.801	841	843	845	rBV	753	364	0.03%	0.003%
17	3.855	856	860	861	rBV2	492	374	0.03%	0.003%
18	3.897	862	873	917	rBV	102376	333013	23.53%	2.890%
19	4.354	997	1015	1044	rBV	237879	594584	42.02%	5.160%
20	4.637	1102	1103	1107	rVB3	872	406	0.03%	0.004%
21	4.743	1134	1136	1139	rVB2	785	412	0.03%	0.004%
22	4.772	1141	1145	1149	rVB3	475	351	0.02%	0.003%
23	4.798	1152	1153	1157	rVB2	660	349	0.02%	0.003%
24	4.823	1157	1161	1162	rBV3	845	543	0.04%	0.005%
25	4.862	1170	1173	1175	rBV2	836	560	0.04%	0.005%
26	4.923	1189	1192	1195	rBV4	589	420	0.03%	0.004%
27	4.958	1200	1203	1209	rBV3	670	537	0.04%	0.005%
28	5.052	1214	1232	1255	rBV2	551462	1415149	100.00%	12.282%
29	5.392	1335	1338	1339	rBV2	904	459	0.03%	0.004%
30	5.457	1352	1358	1361	rBV6	1115	1011	0.07%	0.009%
31	5.473	1361	1363	1365	rBV3	556	328	0.02%	0.003%
32	5.550	1382	1387	1388	rBV4	754	596	0.04%	0.005%
33	5.621	1397	1409	1441	rVV	481108	967387	68.36%	8.396%
34	5.913	1488	1500	1511	rBV3	26327	54798	3.87%	0.476%
35	6.074	1536	1550	1576	rBV	325337	664628	46.97%	5.768%
36	6.354	1633	1637	1639	rBV3	622	514	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020031.D
 Acq On : 15 Jan 2021 18:07
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.479	1672	1676	1678	rBV3	529	454	0.03%	0.004%
38	6.537	1689	1694	1696	rBV3	612	423	0.03%	0.004%
39	6.621	1718	1720	1721	rBV2	787	346	0.02%	0.003%
40	6.695	1742	1743	1747	rBV3	777	553	0.04%	0.005%
41	6.765	1763	1765	1767	rBV2	765	427	0.03%	0.004%
42	6.849	1788	1791	1793	rBV2	784	496	0.04%	0.004%
43	6.990	1823	1835	1857	rVV	168879	311453	22.01%	2.703%
44	7.322	1923	1938	1960	rBV	617812	1078476	76.21%	9.360%
45	7.572	2013	2016	2019	rBV2	634	355	0.03%	0.003%
46	7.627	2023	2033	2058	rBV	116635	210858	14.90%	1.830%
47	7.904	2117	2119	2124	rVB4	566	310	0.02%	0.003%
48	7.929	2124	2127	2129	rBV3	785	429	0.03%	0.004%
49	7.977	2137	2142	2143	rBV3	927	681	0.05%	0.006%
50	8.003	2147	2150	2152	rBV3	825	617	0.04%	0.005%
51	8.093	2168	2178	2217	rBV2	348148	714105	50.46%	6.197%
52	8.383	2265	2268	2270	rBV3	1011	584	0.04%	0.005%
53	8.653	2350	2352	2357	rVB4	663	448	0.03%	0.004%
54	8.759	2383	2385	2387	rBV2	908	607	0.04%	0.005%
55	8.788	2392	2394	2399	rVB4	651	336	0.02%	0.003%
56	8.858	2400	2416	2440	rBV	743618	1223128	86.43%	10.615%
57	9.109	2491	2494	2495	rBV3	639	397	0.03%	0.003%
58	9.164	2507	2511	2512	rBV4	1054	776	0.05%	0.007%
59	9.421	2588	2591	2593	rBV3	810	541	0.04%	0.005%
60	9.662	2662	2666	2667	rBV	516	377	0.03%	0.003%
61	9.698	2675	2677	2680	rBV2	482	345	0.02%	0.003%
62	9.717	2680	2683	2685	rVV3	704	484	0.03%	0.004%
63	9.743	2688	2691	2693	rBV2	692	449	0.03%	0.004%
64	9.788	2702	2705	2709	rBV5	630	543	0.04%	0.005%
65	9.833	2717	2719	2724	rVB5	896	598	0.04%	0.005%
66	9.865	2724	2729	2732	rBV5	617	604	0.04%	0.005%
67	10.093	2797	2800	2805	rVB5	603	446	0.03%	0.004%
68	10.138	2812	2814	2819	rVB2	736	498	0.04%	0.004%
69	10.177	2823	2826	2827	rBV	601	322	0.02%	0.003%
70	10.222	2829	2840	2857	rBV	421382	658783	46.55%	5.717%
71	10.328	2870	2873	2874	rBV2	569	321	0.02%	0.003%
72	10.411	2894	2899	2902	rBV5	801	893	0.06%	0.008%
73	10.543	2937	2940	2944	rVB4	805	613	0.04%	0.005%
74	10.727	2994	2997	3002	rVV2	897	875	0.06%	0.008%
75	10.762	3006	3008	3013	rVB4	598	365	0.03%	0.003%
76	10.913	3053	3055	3058	rVB3	1042	464	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020031.D
 Acq On : 15 Jan 2021 18:07
 Operator : SY/MD
 Sample : VIBLK82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	11.112	3115	3117	3119	rBV2	667	319	0.02%	0.003%
78	11.125	3119	3121	3122	rBV	735	324	0.02%	0.003%
79	11.254	3150	3161	3181	rBV	795202	1242501	87.80%	10.783%
80	11.630	3264	3278	3300	rBV	684550	1083428	76.56%	9.403%
81	11.765	3318	3320	3325	rBV3	820	595	0.04%	0.005%
82	11.862	3346	3350	3352	rVB3	622	392	0.03%	0.003%
83	11.948	3375	3377	3378	rBV	715	331	0.02%	0.003%
84	11.958	3378	3380	3382	rVV3	746	378	0.03%	0.003%
85	12.000	3389	3393	3395	rBV2	788	589	0.04%	0.005%
86	12.296	3481	3485	3486	rBV2	605	421	0.03%	0.004%
87	12.389	3508	3514	3516	rBV3	541	510	0.04%	0.004%
88	12.469	3536	3539	3542	rBV5	715	450	0.03%	0.004%
89	12.836	3649	3653	3659	rBV4	1143	1281	0.09%	0.011%
90	13.048	3717	3719	3721	rBV	586	323	0.02%	0.003%
91	13.103	3733	3736	3740	rBV5	783	745	0.05%	0.006%
92	13.167	3755	3756	3759	rVB3	863	347	0.02%	0.003%
93	13.289	3790	3794	3798	rBV3	874	807	0.06%	0.007%
94	13.601	3886	3891	3894	rBV3	596	545	0.04%	0.005%
95	13.755	3936	3939	3940	rBV2	587	330	0.02%	0.003%
96	13.894	3973	3982	3985	rBV6	986	1808	0.13%	0.016%
97	14.196	4072	4076	4081	rBV6	795	822	0.06%	0.007%
98	14.254	4091	4094	4095	rBV2	862	502	0.04%	0.004%
99	14.472	4156	4162	4165	rBV3	1038	1158	0.08%	0.010%
100	14.598	4198	4201	4206	rBV6	1113	1077	0.08%	0.009%




Sum of corrected areas: 11522564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020031.D
Acq On : 15 Jan 2021 18:07
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

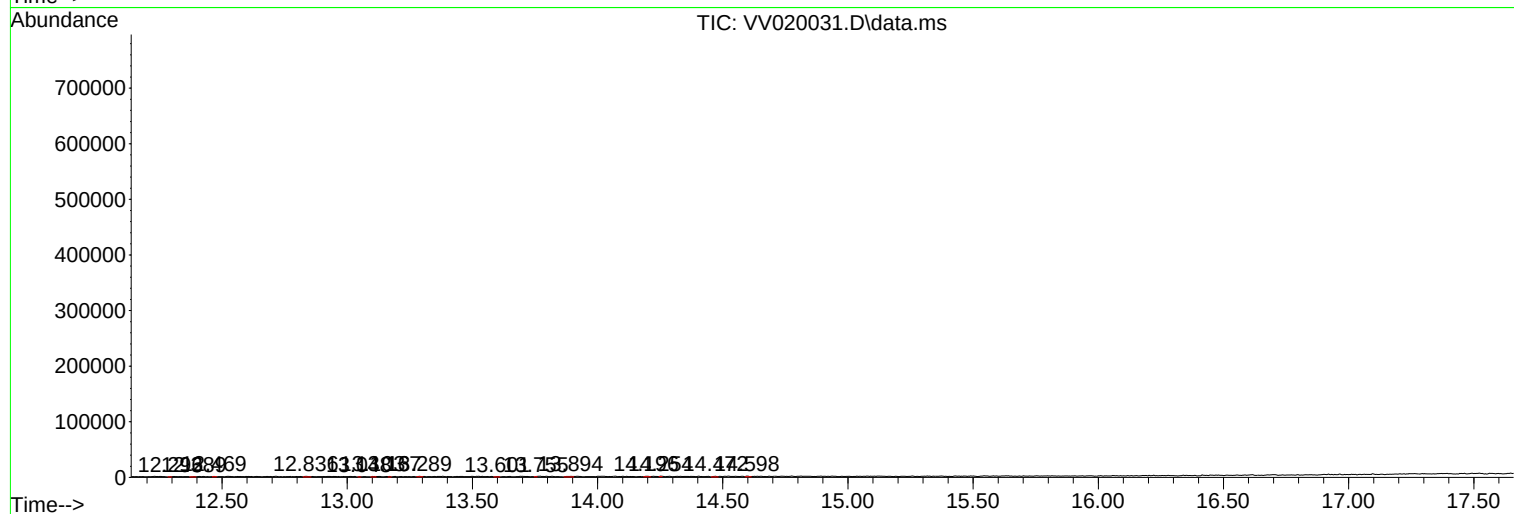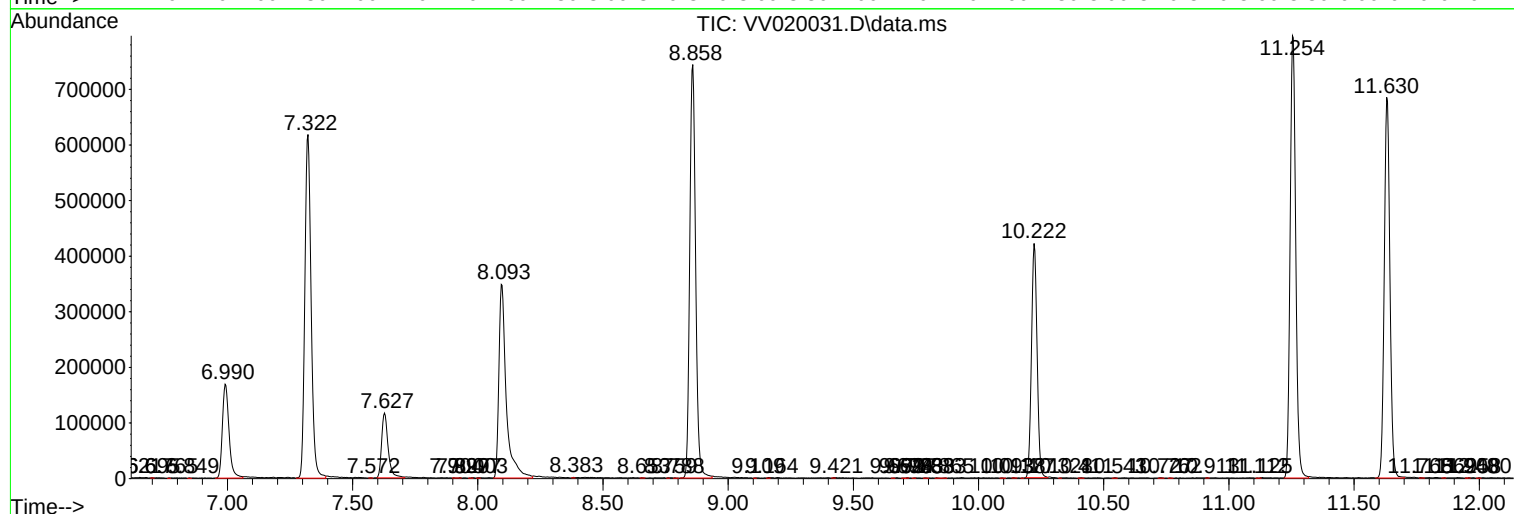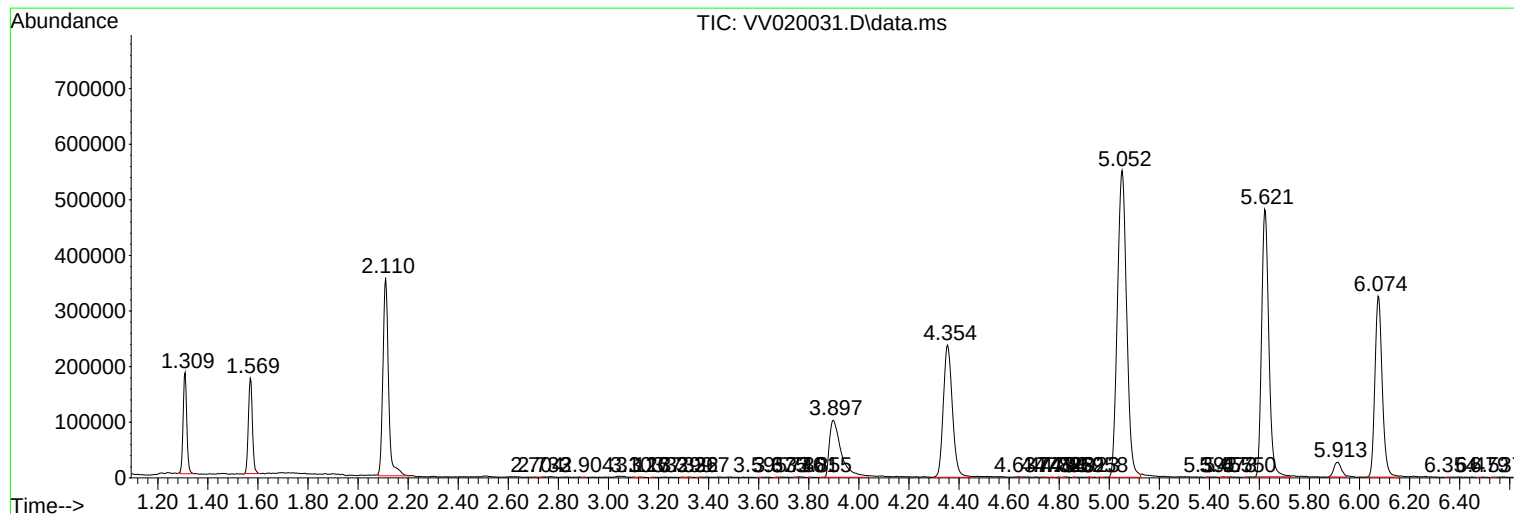

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020031.D
Acq On : 15 Jan 2021 18:07
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020031.D
Acq On : 15 Jan 2021 18:07
Operator : SY/MD
Sample : VIBLK82
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
