
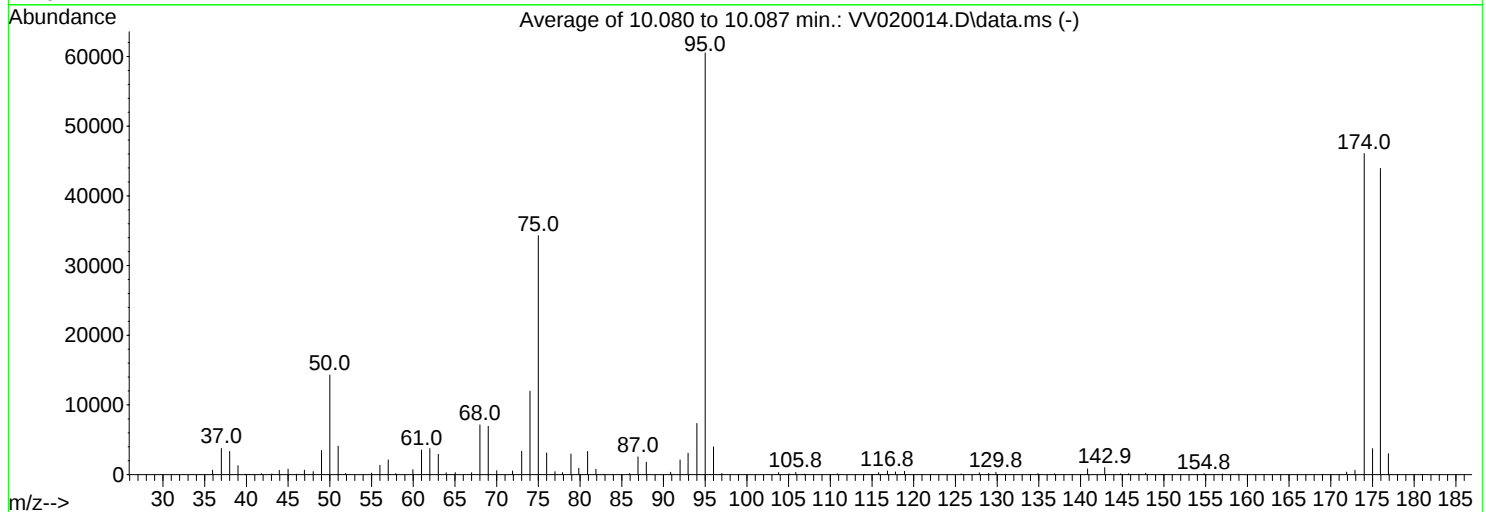


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020014.D
Acq On : 15 Jan 2021 09:28
Operator : SY/MD
Sample : BFB81
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Title : VOC Analysis
Last Update : Tue Jan 19 02:46:41 2021

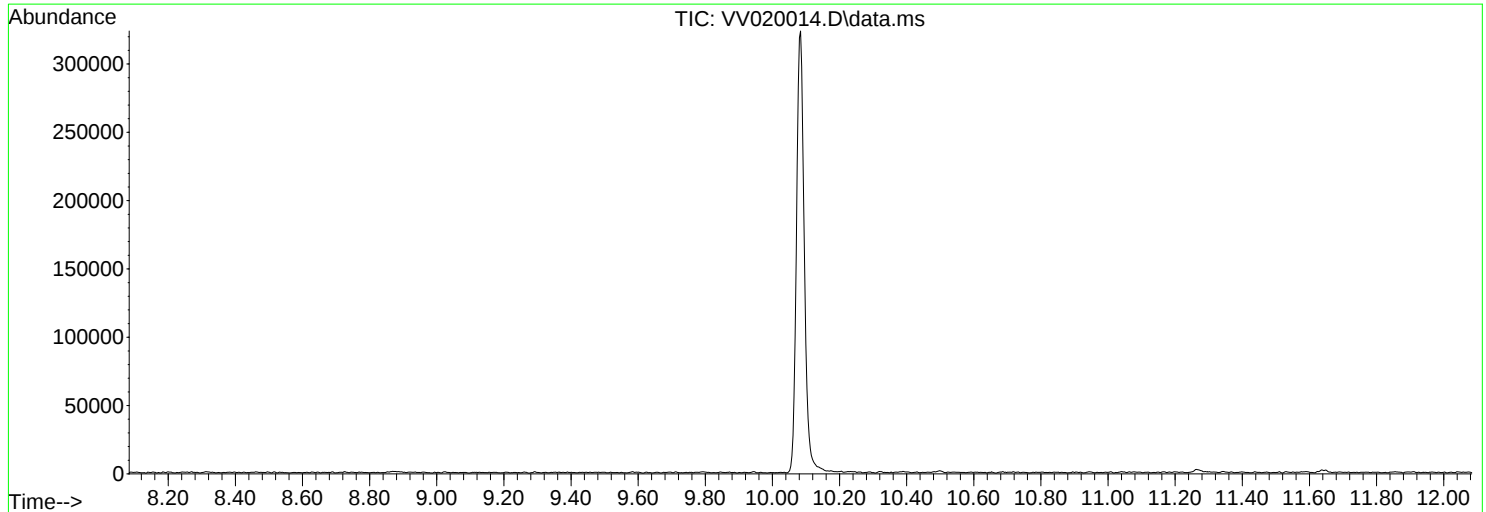

AutoFind: Scans 2796, 2797, 2798; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	14308	PASS
75	95	30	80	56.7	34291	PASS
95	95	100	100	100.0	60523	PASS
96	95	5	9	6.6	4002	PASS
173	174	0.00	2	1.4	655	PASS
174	95	50	120	76.1	46083	PASS
175	174	5	9	8.1	3752	PASS
176	174	95	101	95.3	43933	PASS
177	176	5	9	6.8	3004	PASS

Scan 2784 (10.042 min): VV020014.D\data.ms
BFB81

m/z	Abundance
36.00	117.0
39.00	102.0
39.80	189.0
44.00	402.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	728.0
37.00	3774.0
38.00	3657.0
39.00	1426.0
39.90	267.0
40.40	130.0
41.80	124.0
43.00	138.0
44.00	1029.0
45.00	745.0
47.00	632.0
48.00	449.0
49.00	3537.0
50.00	14963.0
51.00	4061.0
51.90	172.0
55.10	216.0
56.00	1478.0
57.00	2324.0
57.90	118.0
60.00	727.0
61.00	3646.0
62.00	3798.0
63.00	3096.0
64.00	261.0
65.00	324.0
67.00	245.0
68.00	7292.0
69.00	6949.0
70.00	545.0
71.90	527.0
73.00	3397.0
74.00	12359.0
75.00	35752.0
76.00	3294.0
77.00	434.0
77.90	284.0
78.90	3076.0
79.90	991.0
80.90	3316.0
81.90	765.0
86.00	122.0
86.90	2532.0
88.00	1932.0
90.90	386.0
92.00	2269.0
92.90	3053.0
94.00	7520.0
95.00	61728.0
96.00	4321.0
97.00	155.0
103.80	278.0
105.10	130.0
105.90	340.0
106.70	136.0
110.80	156.0
115.80	326.0
116.90	582.0
117.80	432.0
118.90	559.0
125.70	102.0
127.80	300.0
129.00	167.0
129.90	366.0
131.00	108.0
134.90	143.0
136.90	118.0
140.90	824.0
142.90	1072.0
144.80	180.0
145.80	133.0
147.00	104.0
147.70	200.0
154.80	151.0
160.90	138.0
171.90	402.0
172.90	652.0
174.00	45712.0
175.00	3701.0
175.90	43768.0
176.90	2885.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	768.0
37.00	3899.0
38.00	3365.0
39.00	1403.0
39.90	271.0
41.80	156.0
43.00	117.0
44.00	1024.0
45.00	860.0
46.00	122.0
46.90	684.0
48.00	419.0
49.00	3654.0
50.00	14930.0
51.00	4218.0
51.90	168.0
55.00	215.0
56.00	1325.0
57.00	2170.0
57.90	167.0
60.00	731.0
61.00	3635.0
62.00	3829.0
63.00	2981.0
64.00	278.0
65.10	308.0
67.00	293.0
68.00	7338.0
69.00	7167.0
70.00	587.0
71.90	573.0
73.00	3481.0
74.00	12330.0
75.00	35408.0
76.00	3263.0
77.00	453.0
77.90	324.0
78.90	3045.0
79.90	920.0
80.90	3467.0
81.90	804.0
82.90	101.0
85.90	162.0
87.00	2752.0
87.90	1798.0
90.90	353.0
92.00	2180.0
93.00	3114.0
94.00	7572.0
95.00	62512.0
96.00	4140.0
97.00	164.0
103.80	305.0
105.00	134.0
105.80	344.0
106.90	131.0
110.80	140.0
115.80	293.0
116.80	544.0
117.80	418.0
118.90	489.0
125.70	112.0
127.90	275.0
129.00	194.0
129.80	354.0
131.10	108.0
134.90	167.0
136.90	136.0
140.80	831.0
142.90	1067.0
144.80	169.0
145.80	142.0
147.00	111.0
147.80	179.0
154.80	160.0
157.00	133.0
158.90	118.0
171.90	387.0
172.90	677.0
174.00	47584.0
175.00	3967.0
176.00	45424.0
176.90	3074.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	764.0
37.00	3638.0
38.00	2970.0
39.00	1310.0
39.90	237.0
40.80	113.0
41.80	136.0
43.10	125.0
43.90	990.0
45.00	807.0
46.00	117.0
46.90	641.0
48.00	410.0
49.00	3191.0
50.00	13030.0
51.00	3963.0
51.90	151.0
54.90	272.0
56.00	1225.0
57.00	1817.0
57.90	171.0
59.90	656.0
61.00	3324.0
62.00	3583.0
63.00	2657.0
63.90	290.0
65.10	265.0
67.00	273.0
68.00	6760.0
69.00	6681.0
70.00	567.0
71.90	491.0
73.00	3202.0
74.00	11288.0
75.00	31712.0
76.00	2823.0
77.00	397.0
77.90	326.0
78.90	2781.0
79.80	815.0
80.90	3189.0
81.90	764.0
82.80	113.0
85.90	187.0
87.00	2367.0
87.90	1660.0
90.80	314.0
92.00	1921.0
93.00	3044.0
94.00	6976.0
95.00	57328.0
96.00	3544.0
97.00	169.0
103.80	297.0
105.00	118.0
105.80	309.0
106.90	129.0
110.90	133.0
114.10	117.0
115.80	267.0
116.80	460.0
117.80	324.0
118.90	424.0
125.70	105.0
127.90	237.0
129.00	163.0
129.80	289.0
134.90	192.0
136.90	168.0
140.80	824.0
142.90	923.0
145.70	142.0
147.90	211.0
149.70	126.0
154.80	151.0
157.00	145.0
158.90	134.0
171.90	344.0
172.90	637.0
174.00	44952.0
175.00	3589.0
176.00	42608.0
176.90	3052.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81