

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011524\
 Data File : VW033644.D
 Acq On : 15 Jan 2024 15:47
 Operator : SY/MD
 Sample : P1131-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B03

Quant Time: Jan 16 03:46:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 16 03:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	120121	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	111952	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	56531	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	27441	4.178	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.600%
7) Chloroethane-d5	1.535	69	26845	4.608	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.060	65	13347	4.509	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.200%
20) 2-Butanone-d5	3.822	46	76309	47.515	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.020%
24) Chloroform-d	4.252	84	65680	4.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	4.947	65	32303	5.072	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
32) Benzene-d6	4.963	84	127338	4.714	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
36) 1,2-Dichloropropane-d6	5.989	67	41268	4.582	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.600%
41) Toluene-d8	7.246	98	111600	4.628	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	7.561	79	13958	4.483	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.030	63	58277	47.674	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.340%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	25819	4.906	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	42268	4.870	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds						
					Qvalue	
25) Chloroform	4.278	83	11069	0.634	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033644.D
Acq On : 15 Jan 2024 15:47
Operator : SY/MD
Sample : P1131-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B03

Quant Time: Jan 16 03:46:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 16 03:40:53 2024
Response via : Initial Calibration

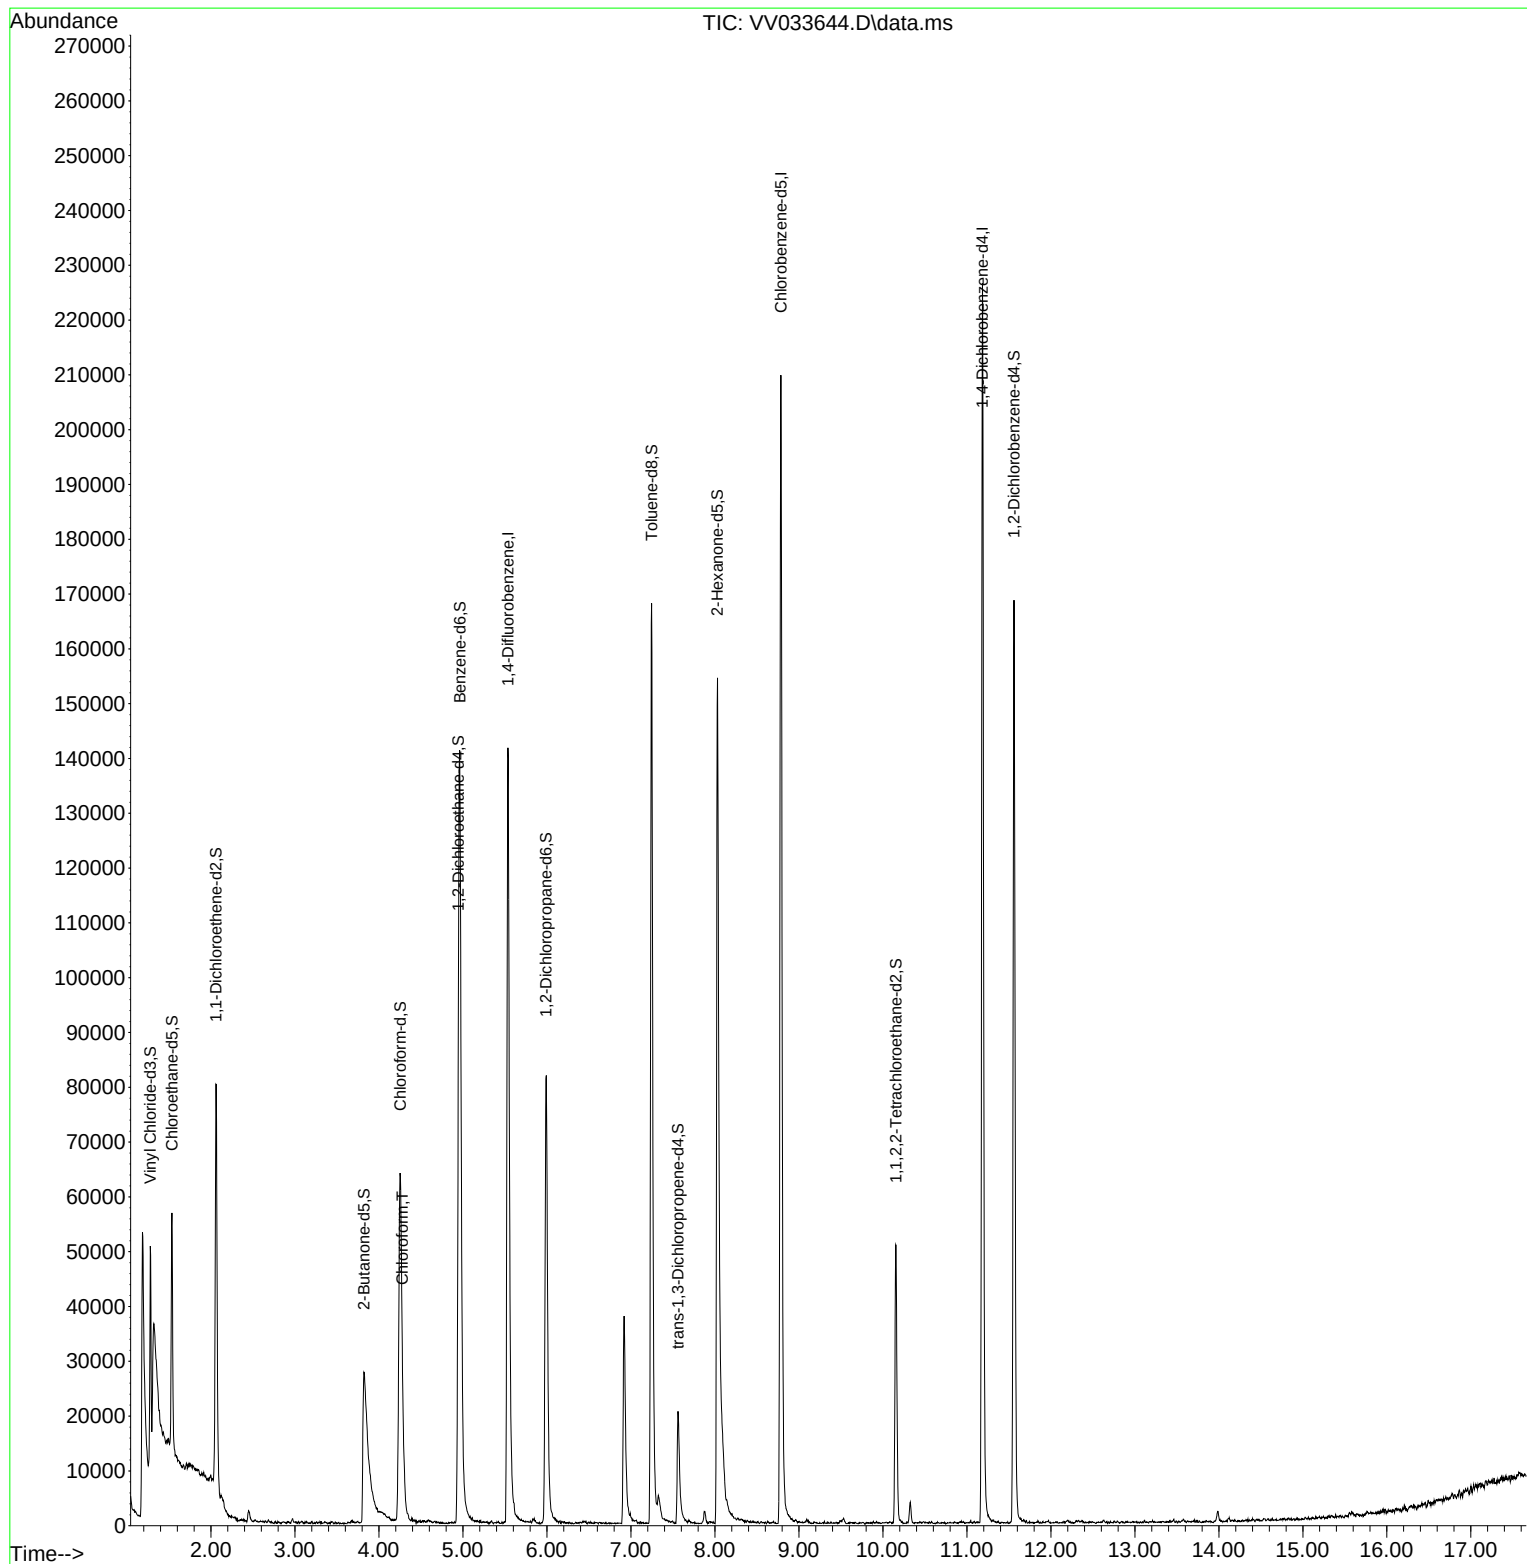

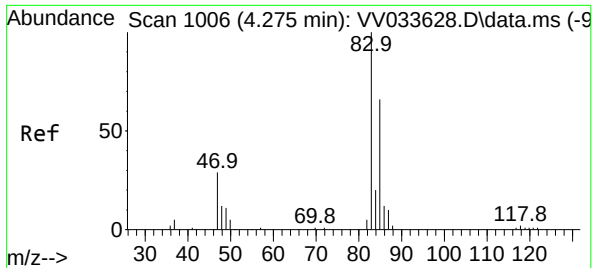

#25
 Chloroform
 Concen: 0.634 ug/L
 RT: 4.278 min Scan# 11
 Delta R.T. 0.003 min
 Lab File: VV033644.D
 Acq: 15 Jan 2024 15:47

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B03

Tgt Ion: 83 Resp: 11069
 Ion Ratio Lower Upper
 83 100
 85 61.8 45.1 83.9

