

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011524\
 Data File : VW033647.D
 Acq On : 15 Jan 2024 16:58
 Operator : SY/MD
 Sample : P1131-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAX0

Quant Time: Jan 16 03:47:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 16 03:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.548	114	110270	5.000	ug/L	0.01
28) Chlorobenzene-d5	8.796	117	98811	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	49746	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	23132	3.836	ug/L	0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.800%
7) Chloroethane-d5	1.555	69	23000	4.301	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.000%
11) 1,1-Dichloroethene-d2	2.072	65	11064	4.072	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.400%
20) 2-Butanone-d5	3.902	46	64524	43.766	ug/L	0.08
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.540%
24) Chloroform-d	4.265	84	54412	4.173	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.400%
26) 1,2-Dichloroethane-d4	4.960	65	27979	4.785	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
32) Benzene-d6	4.969	84	111307	4.669	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	6.014	67	37200	4.680	ug/L	0.03
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%
41) Toluene-d8	7.262	98	98489	4.627	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	7.577	79	11053	4.022	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.050	63	55347	51.299	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.600%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	22316	4.805	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	36523	4.782	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.304	62	25914	2.259	ug/L	95
18) trans-1,2-Dichloroethene	2.709	96	5873	0.669	ug/L	99
19) 1,1-Dichloroethane	3.130	63	54042	3.098	ug/L	97
22) cis-1,2-Dichloroethene	3.825	96	287370	31.256	ug/L	96
27) 1,2-Dichloroethane	5.066	62	10502	1.151	ug/L	99
30) Cyclohexane	4.577	56	4990	0.297	ug/L	93
33) Benzene	5.021	78	67740	1.931	ug/L	100
34) Trichloroethene	5.850	95	3088	0.331	ug/L	95
35) Methylcyclohexane	6.063	83	4541	0.287	ug/L	87
42) Toluene	7.346	91	5032	0.136	ug/L	100
51) Chlorobenzene	8.825	112	72775	3.202	ug/L	99
52) Ethylbenzene	8.963	91	3631	0.084	ug/L	99
53) m,p-Xylene	9.085	106	2071	0.131	ug/L	90
60) Isopropylbenzene	9.876	105	5178	0.132	ug/L #	84
64) 1,3-Dichlorobenzene	11.127	146	5270	0.303	ug/L	97
65) 1,4-Dichlorobenzene	11.214	146	17489	1.026	ug/L	95
67) 1,2-Dichlorobenzene	11.580	146	74793	4.944	ug/L	99
70) 1,2,4-trichlorobenzene	13.204	180	2779	0.247	ug/L #	83

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033647.D
Acq On : 15 Jan 2024 16:58
Operator : SY/MD
Sample : P1131-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Time: Jan 16 03:47:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 16 03:40:53 2024
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033647.D
Acq On : 15 Jan 2024 16:58
Operator : SY/MD
Sample : P1131-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Time: Jan 16 03:47:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 16 03:40:53 2024
Response via : Initial Calibration

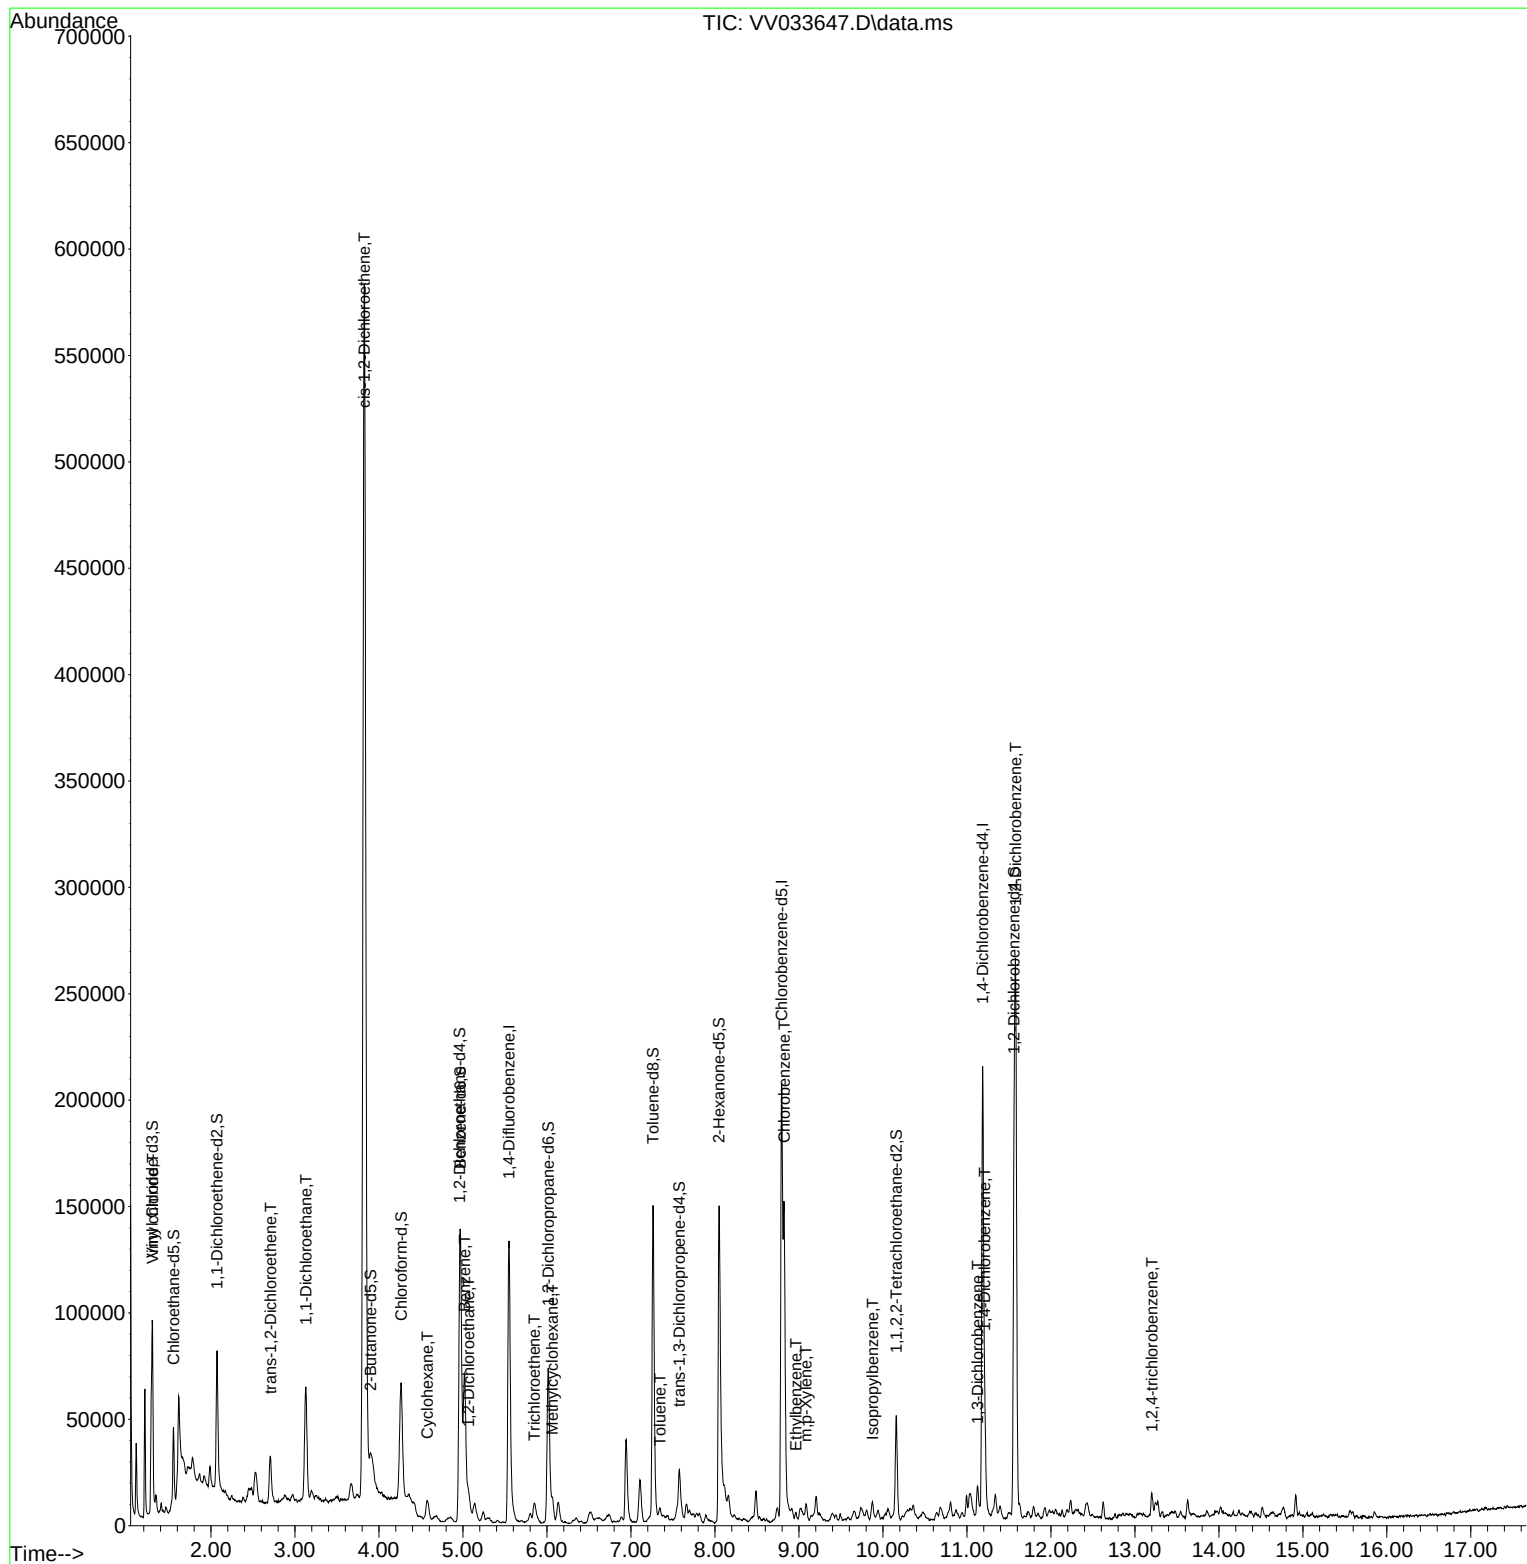

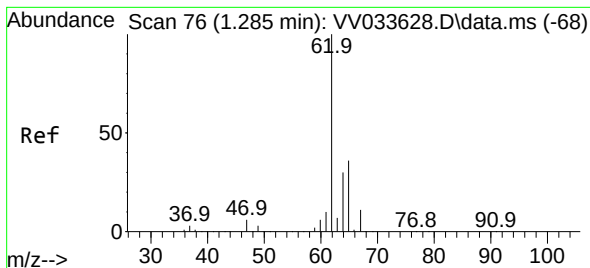

#5

Vinyl chloride

Concen: 2.259 ug/L

RT: 1.304 min Scan# 81

Delta R.T. 0.019 min

Lab File: VV033647.D

Acq: 15 Jan 2024 16:58

Instrument :

MSVOA_V

ClientSampleId :





COAX0

Tgt Ion: 62 Resp: 25914

Ion Ratio Lower Upper

62 100

64 29.8 23.0 42.8

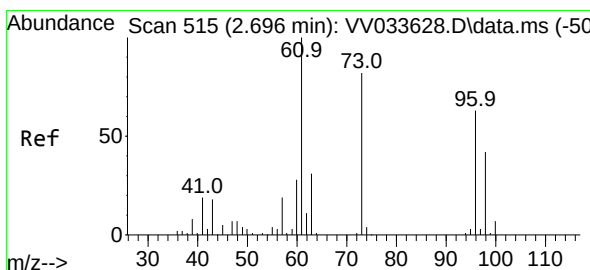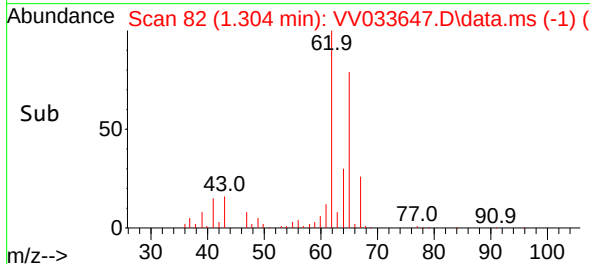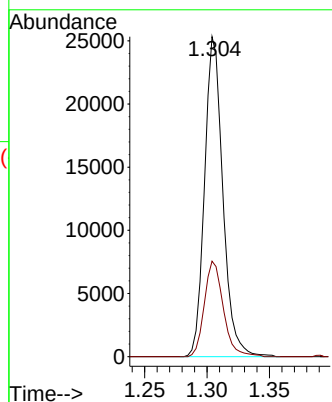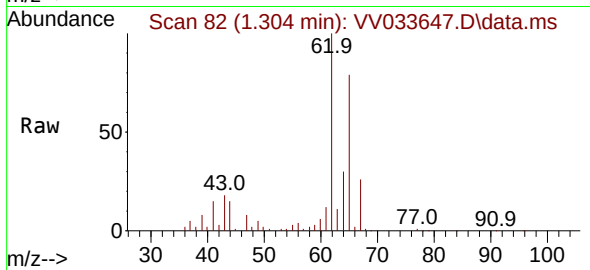

#18

trans-1,2-Dichloroethene

Concen: 0.669 ug/L

RT: 2.709 min Scan# 519

Delta R.T. 0.013 min

Lab File: VV033647.D

Acq: 15 Jan 2024 16:58




Tgt Ion: 96 Resp: 5873


Ion Ratio Lower Upper

96 100

61 158.4 110.4 205.0

98 65.9 44.1 81.9


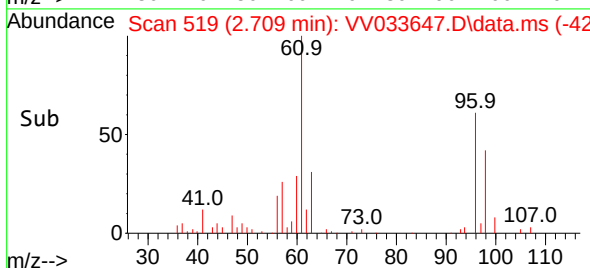
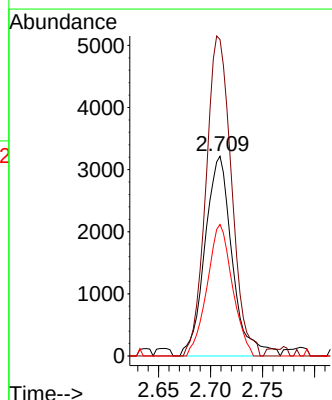
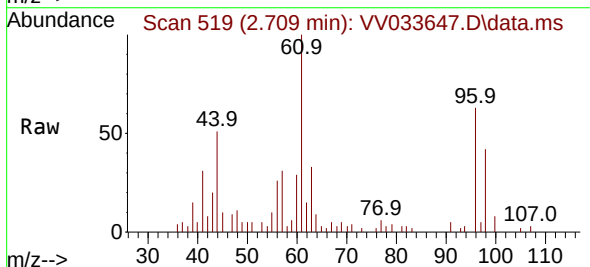




#19
1,1-Dichloroethane
Concen: 3.098 ug/L
RT: 3.130 min Scan# 61
Delta R.T. 0.019 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
COAX0


Tgt Ion: 63 Resp: 54042
Ion Ratio Lower Upper
63 100
65 32.7 21.6 40.2
83 13.4 9.1 16.9

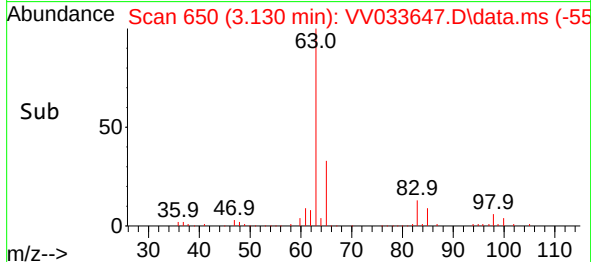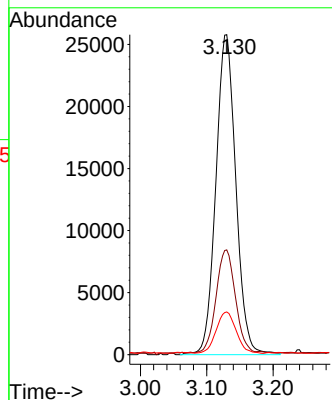

#22
cis-1,2-Dichloroethene
Concen: 31.256 ug/L
RT: 3.825 min Scan# 866
Delta R.T. 0.013 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion: 96 Resp: 287370
Ion Ratio Lower Upper
96 100
61 143.4 97.1 180.3
98 64.7 42.6 79.0


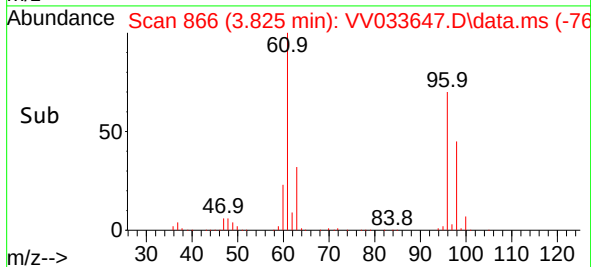
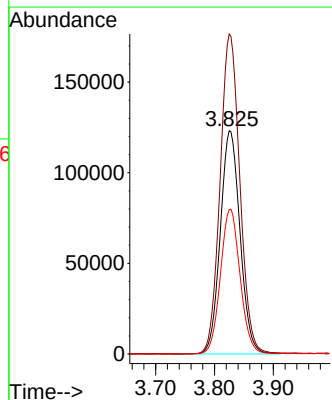
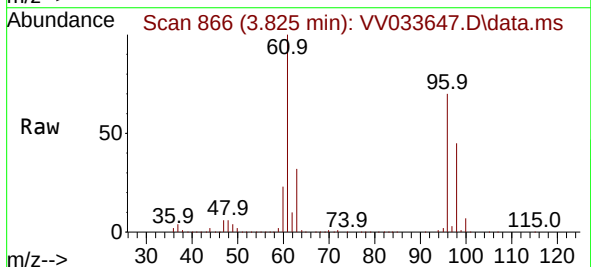




#27
1,2-Dichloroethane
Concen: 1.151 ug/L
RT: 5.066 min Scan# 1100
Delta R.T. 0.022 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
C0AX0


Tgt Ion: 62 Resp: 10502
Ion Ratio Lower Upper
62 100
98 8.4 7.0 10.6

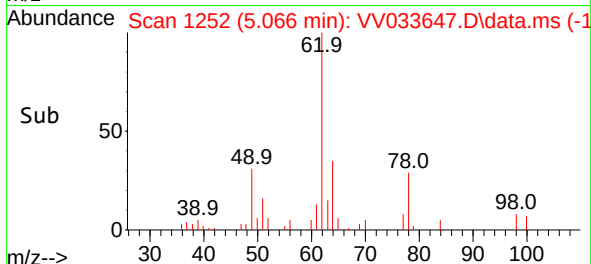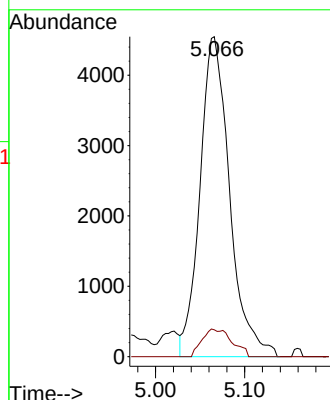

#30
Cyclohexane
Concen: 0.297 ug/L
RT: 4.577 min Scan# 1100
Delta R.T. -0.003 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion: 56 Resp: 4990
Ion Ratio Lower Upper
56 100
69 23.3 23.3 34.9
84 82.2 61.7 92.5


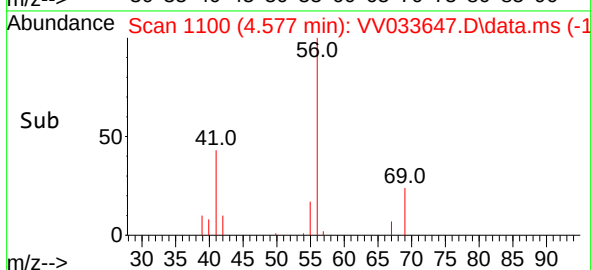
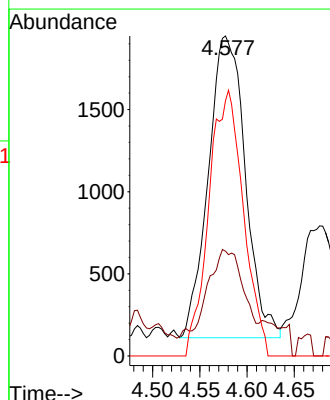





#33
Benzene
Concen: 1.931 ug/L
RT: 5.021 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Instrument :
MSVOA_V
ClientSampleId :
C0AX0




Tgt Ion: 78 Resp: 67740

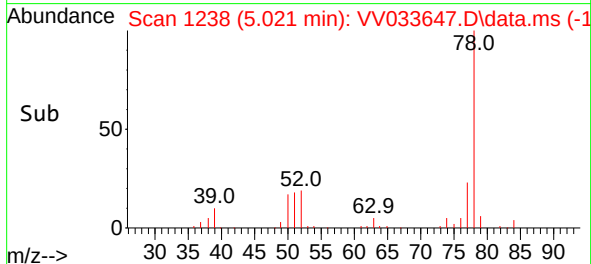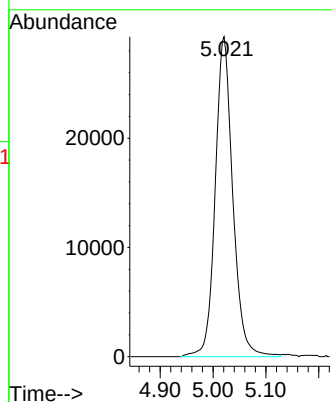


#34
Trichloroethene
Concen: 0.331 ug/L
RT: 5.850 min Scan# 1496
Delta R.T. 0.019 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion: 95 Resp: 3088

Ion	Ratio	Lower	Upper
95	100		
97	68.2	45.1	83.9
132	97.2	65.2	121.2
130	88.7	66.0	122.6


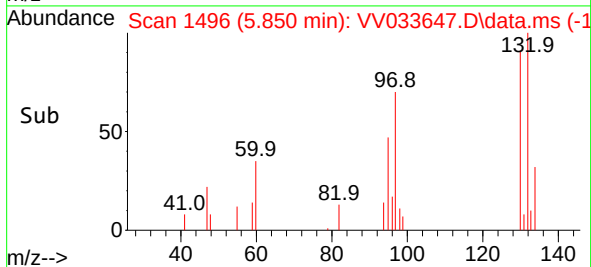
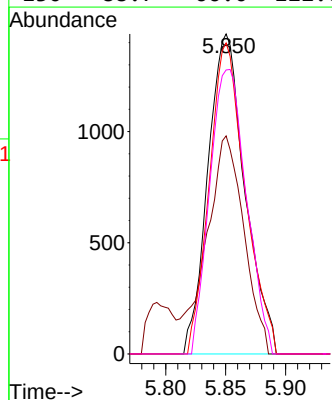
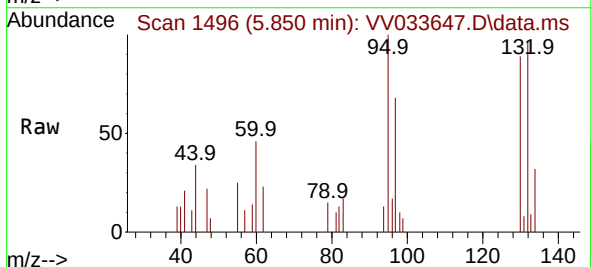




#35
Methylcyclohexane
Concen: 0.287 ug/L
RT: 6.063 min Scan# 11
Delta R.T. 0.016 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
C0AX0


Tgt Ion: 83 Resp: 4541
Ion Ratio Lower Upper
83 100
55 72.6 68.7 103.1
98 40.9 38.3 57.5

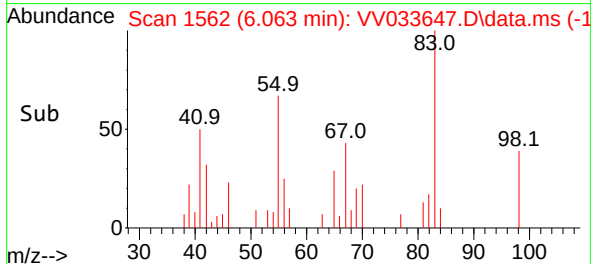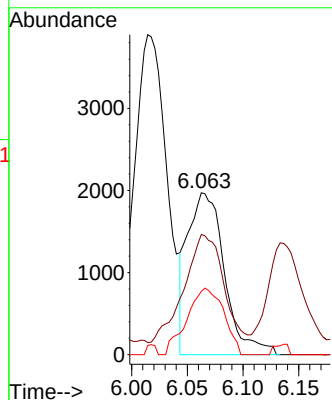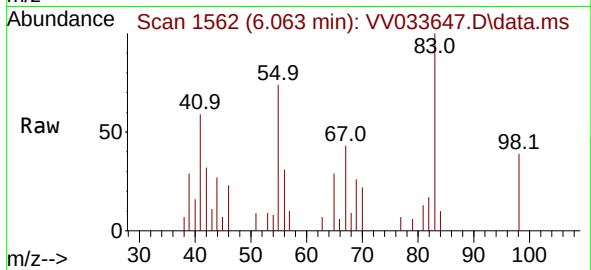

#42
Toluene
Concen: 0.136 ug/L
RT: 7.346 min Scan# 1961
Delta R.T. 0.032 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion: 91 Resp: 5032
Ion Ratio Lower Upper
91 100
92 57.9 40.5 75.3


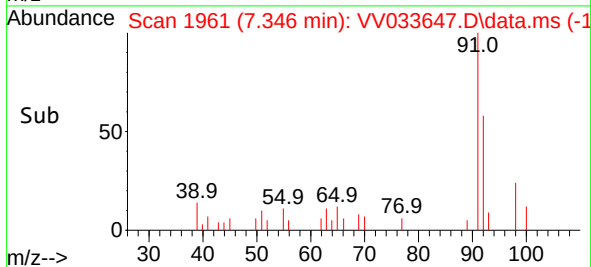
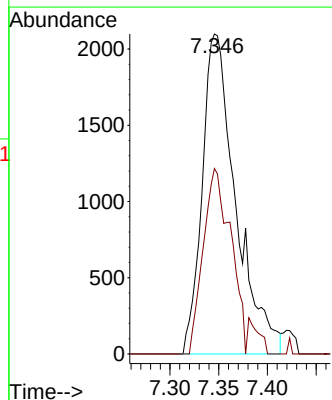
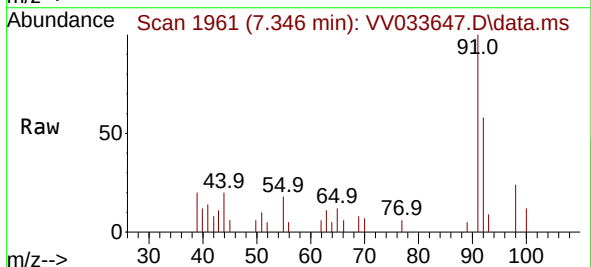




#51
Chlorobenzene
Concen: 3.202 ug/L
RT: 8.825 min Scan# 2417
Delta R.T. 0.013 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
C0AX0


Tgt Ion:112 Resp: 72775
Ion Ratio Lower Upper
112 100
114 31.9 22.9 42.5
77 63.7 50.8 76.2

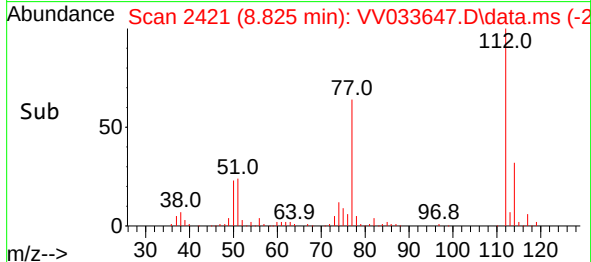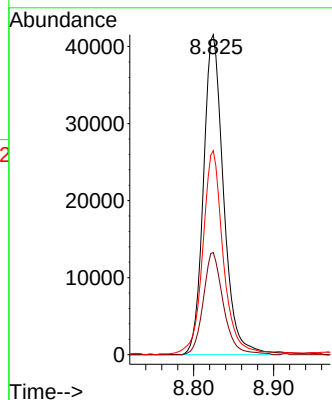

#52
Ethylbenzene
Concen: 0.084 ug/L
RT: 8.963 min Scan# 2464
Delta R.T. 0.019 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion: 91 Resp: 3631
Ion Ratio Lower Upper
91 100
106 30.2 20.6 38.4


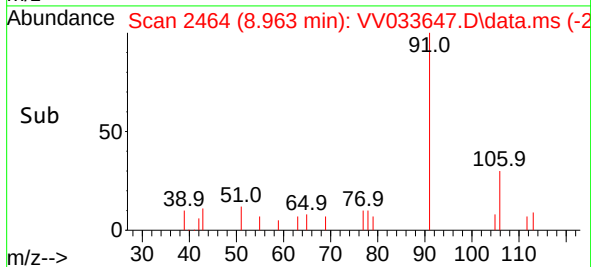
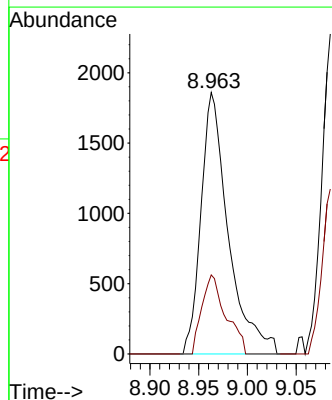
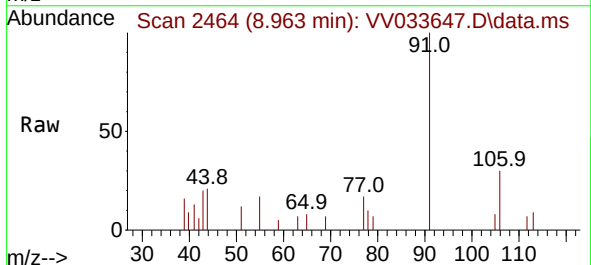




#53
m,p-Xylene
Concen: 0.131 ug/L
RT: 9.085 min Scan# 21
Delta R.T. 0.013 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
C0AX0


Tgt Ion:106 Resp: 2071
Ion Ratio Lower Upper
106 100
91 193.9 146.2 271.4

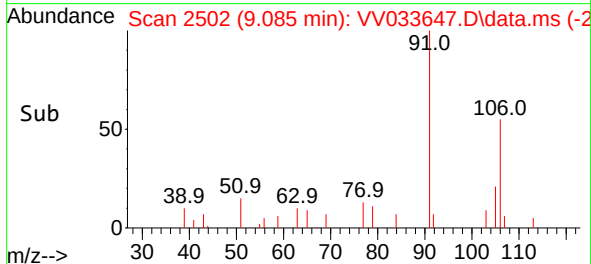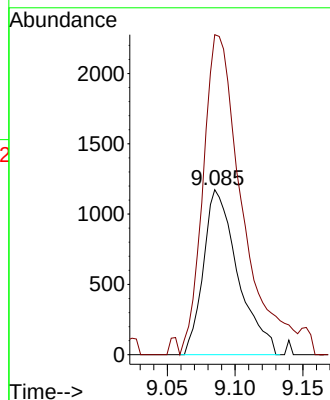

#60
Isopropylbenzene
Concen: 0.132 ug/L
RT: 9.876 min Scan# 2748
Delta R.T. 0.010 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion:105 Resp: 5178
Ion Ratio Lower Upper
105 100
120 27.4 21.0 31.6
77 0.0 13.4 20.0#



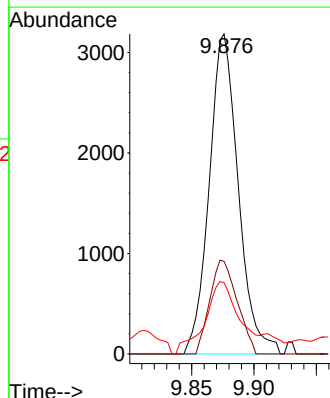
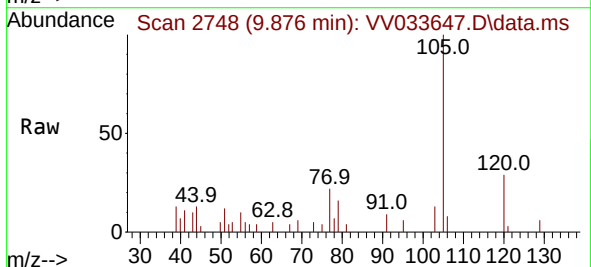




#64
1,3-Dichlorobenzene
Concen: 0.303 ug/L
RT: 11.127 min Scan# 3137
Delta R.T. 0.010 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58




Instrument :
MSVOA_V
ClientSampleId :
COAX0


Tgt Ion:146 Resp: 5270
Ion Ratio Lower Upper
146 100
111 44.8 29.2 54.2
148 61.8 44.1 81.9

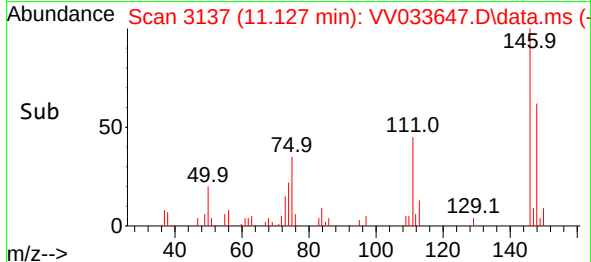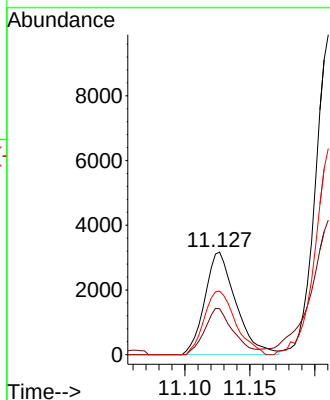

#65
1,4-Dichlorobenzene
Concen: 1.026 ug/L
RT: 11.214 min Scan# 3164
Delta R.T. 0.006 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion:146 Resp: 17489
Ion Ratio Lower Upper
146 100
111 42.7 27.5 51.1
148 65.4 43.3 80.5


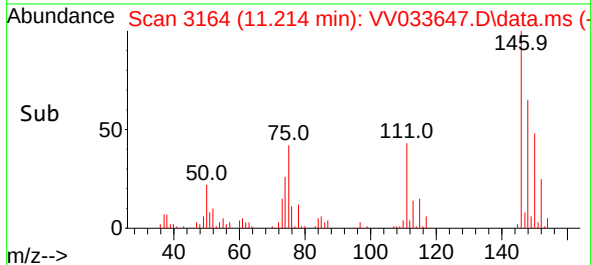
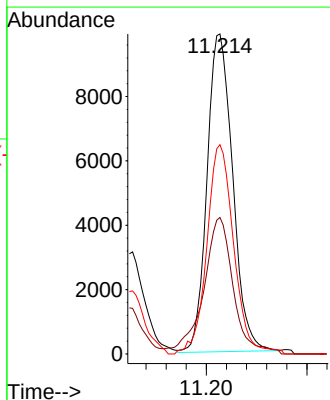
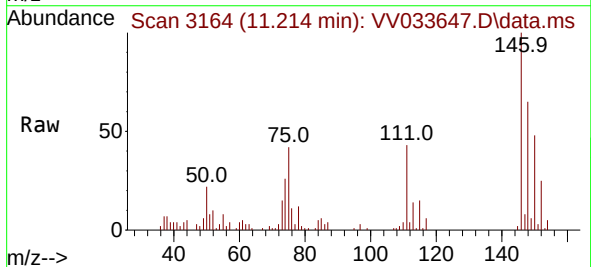




#67
1,2-Dichlorobenzene
Concen: 4.944 ug/L
RT: 11.580 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Instrument :
MSVOA_V
ClientSampleId :
COAX0

Tgt Ion:146 Resp: 74793
Ion Ratio Lower Upper
146 100
111 44.2 36.1 54.1
148 65.6 52.2 78.2

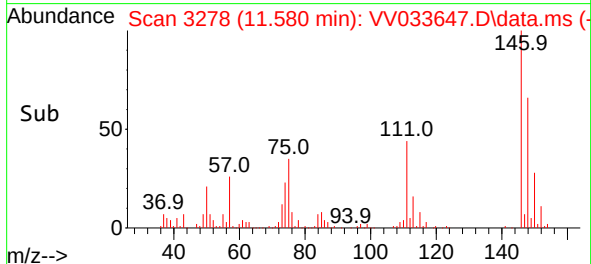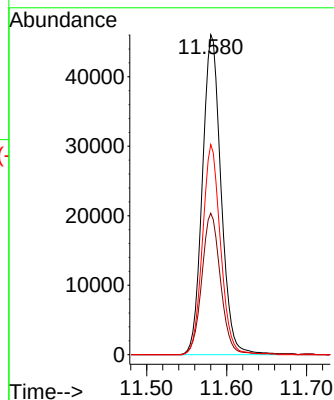

#70
1,2,4-trichlorobenzene
Concen: 0.247 ug/L
RT: 13.204 min Scan# 3783
Delta R.T. 0.006 min
Lab File: VV033647.D
Acq: 15 Jan 2024 16:58

Tgt Ion:180 Resp: 2779
Ion Ratio Lower Upper
180 100
182 99.9 75.0 112.6
145 57.8 24.8 37.2#

