

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011524\
 Data File : VW033653.D
 Acq On : 15 Jan 2024 19:21
 Operator : SY/MD
 Sample : P1131-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Quant Time: Jan 16 03:49:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 16 03:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	112236	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	104548	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	53316	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	23001	3.748	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.535	69	23532	4.323	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.400%
11) 1,1-Dichloroethene-d2	2.063	65	11947	4.319	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.400%
20) 2-Butanone-d5	3.815	46	70464	46.958	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.920%
24) Chloroform-d	4.252	84	60916	4.590	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
26) 1,2-Dichloroethane-d4	4.947	65	29455	4.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	4.963	84	114217	4.528	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	5.992	67	37534	4.463	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.246	98	101846	4.522	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
43) trans-1,3-Dichloroprop...	7.558	79	12784	4.397	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.000%
46) 2-Hexanone-d5	8.030	63	59222	51.878	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.760%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	24605	5.007	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	38065	4.650	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds						
25) Chloroform	4.278	83	10642	0.653	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033653.D
Acq On : 15 Jan 2024 19:21
Operator : SY/MD
Sample : P1131-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Time: Jan 16 03:49:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 16 03:40:53 2024
Response via : Initial Calibration

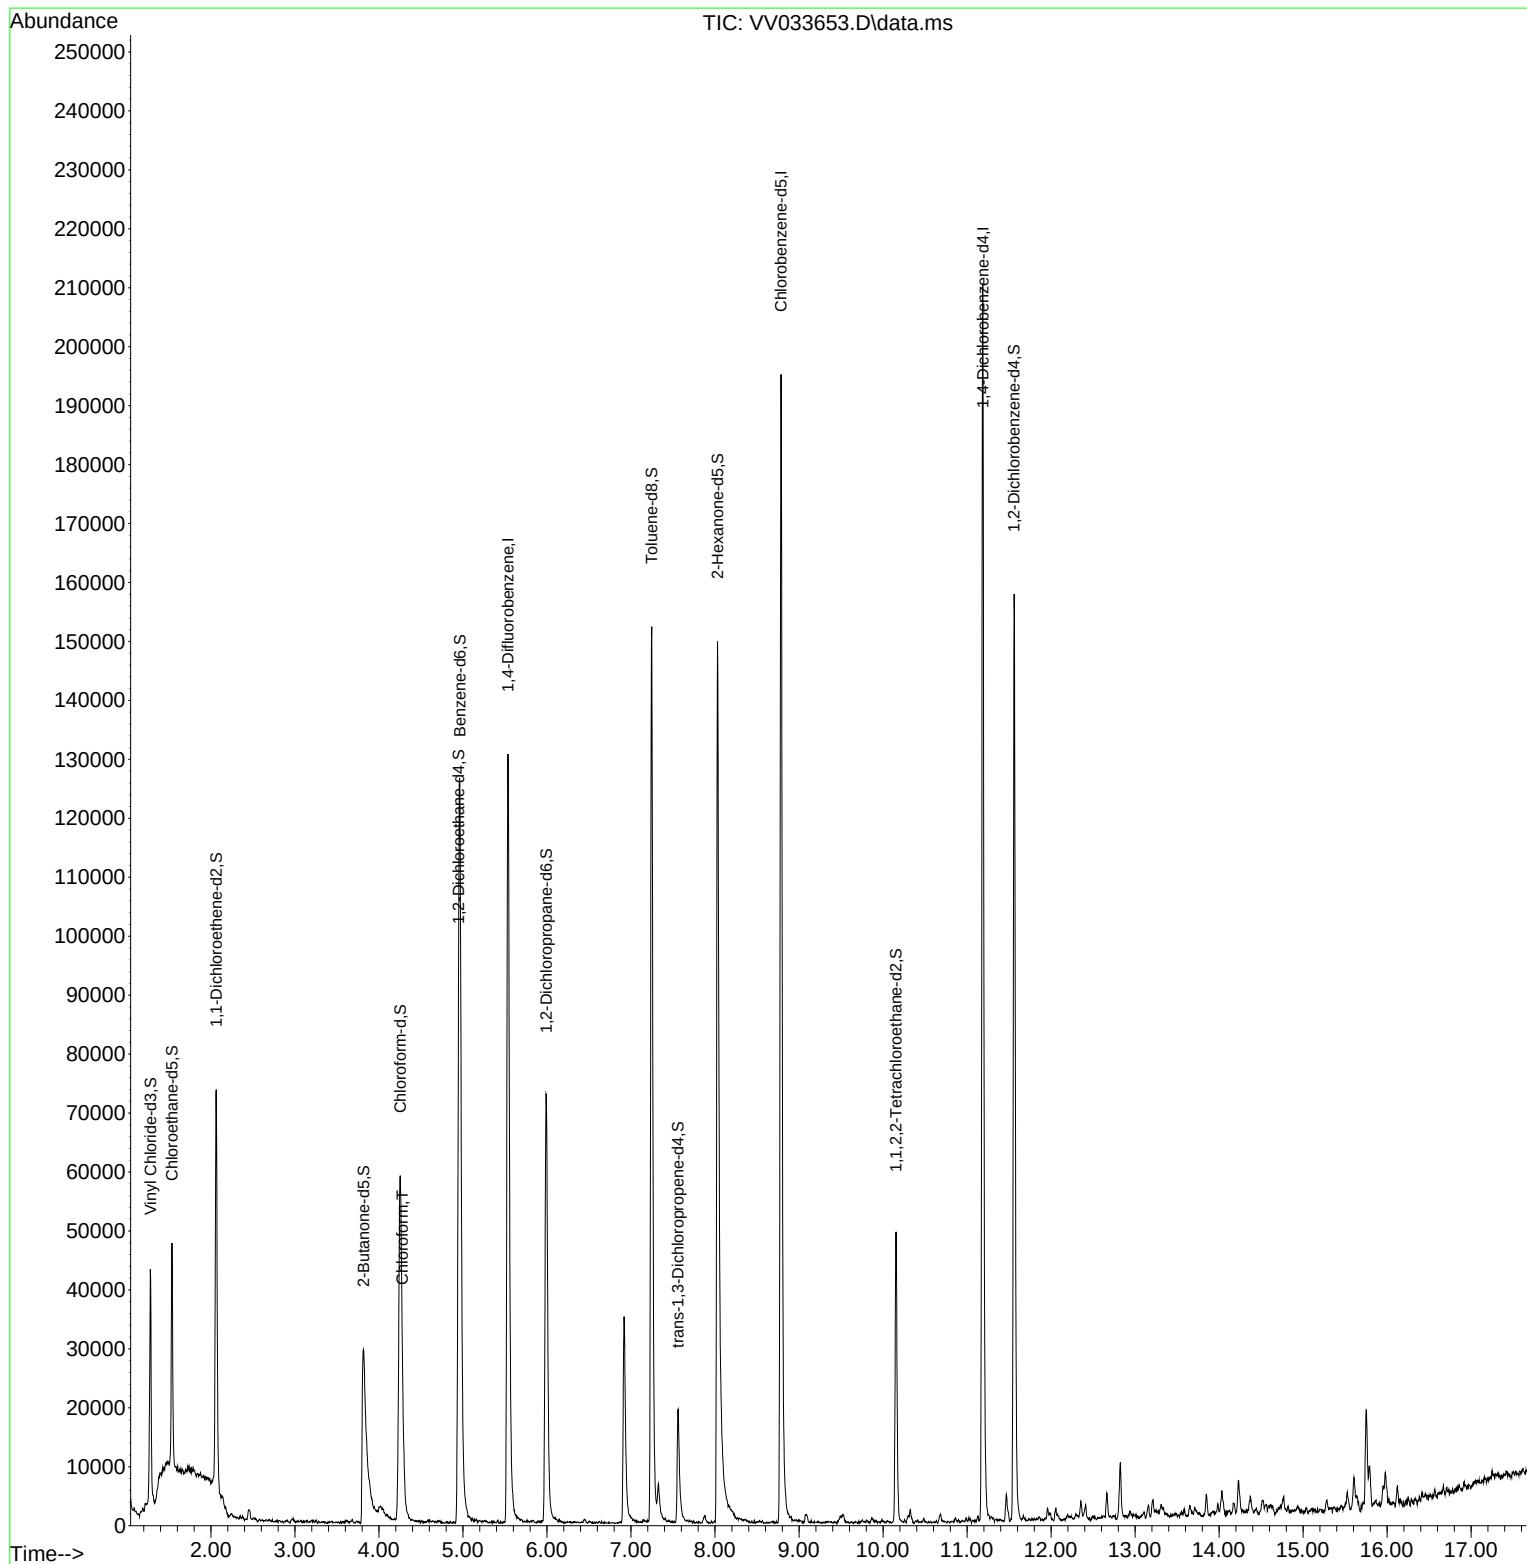

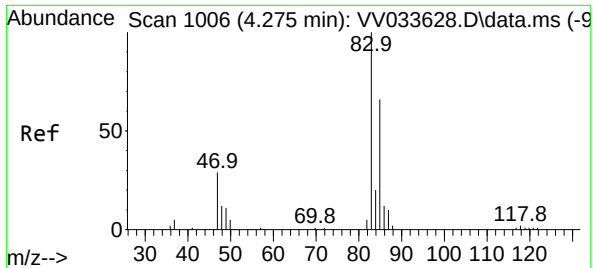

#25
Chloroform
Concen: 0.653 ug/L
RT: 4.278 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV033653.D
Acq: 15 Jan 2024 19:21

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Tgt Ion: 83 Resp: 10642
Ion Ratio Lower Upper
83 100
85 61.8 45.1 83.9

