

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
 Data File : VV033646.D
 Acq On : 15 Jan 2024 16:34
 Operator : SY/MD
 Sample : P1131-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	26	rVB2	8936	11574	3.14%	0.351%
2	1.230	41	59	62	rBV4	11427	31551	8.57%	0.958%
3	1.278	67	74	84	rVB	45002	58034	15.76%	1.762%
4	1.532	147	153	165	rVB	41053	50218	13.64%	1.525%
5	2.060	308	317	336	rVB	76091	120749	32.80%	3.667%
6	2.696	506	515	525	rVB7	2153	3929	1.07%	0.119%
7	3.825	852	866	908	rBV3	45660	177678	48.26%	5.396%
8	4.253	983	999	1025	rBV	57744	152005	41.29%	4.616%
9	4.960	1205	1219	1254	rBV2	138595	368182	100.00%	11.181%
10	5.535	1384	1398	1431	rBV	132200	280637	76.22%	8.522%
11	5.992	1527	1540	1563	rBV	79083	169907	46.15%	5.160%
12	6.918	1819	1828	1860	rBV	35961	75947	20.63%	2.306%
13	7.246	1918	1930	1958	rBV	161817	299018	81.21%	9.080%
14	7.561	2016	2028	2049	rBV2	19932	42115	11.44%	1.279%
15	7.876	2117	2126	2133	rBV4	3070	5011	1.36%	0.152%
16	8.034	2166	2175	2212	rBV	140287	337955	91.79%	10.263%
17	8.786	2399	2409	2430	rBV	199726	348291	94.60%	10.577%
18	10.156	2824	2835	2851	rVB	49857	80356	21.83%	2.440%
19	10.326	2877	2888	2898	rBV2	6897	11592	3.15%	0.352%
20	11.185	3145	3155	3176	rVB	211812	344083	93.45%	10.449%
21	11.561	3261	3272	3295	rBV2	171967	324154	88.04%	9.844%




Sum of corrected areas: 3292986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033646.D
Acq On : 15 Jan 2024 16:34
Operator : SY/MD
Sample : P1131-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

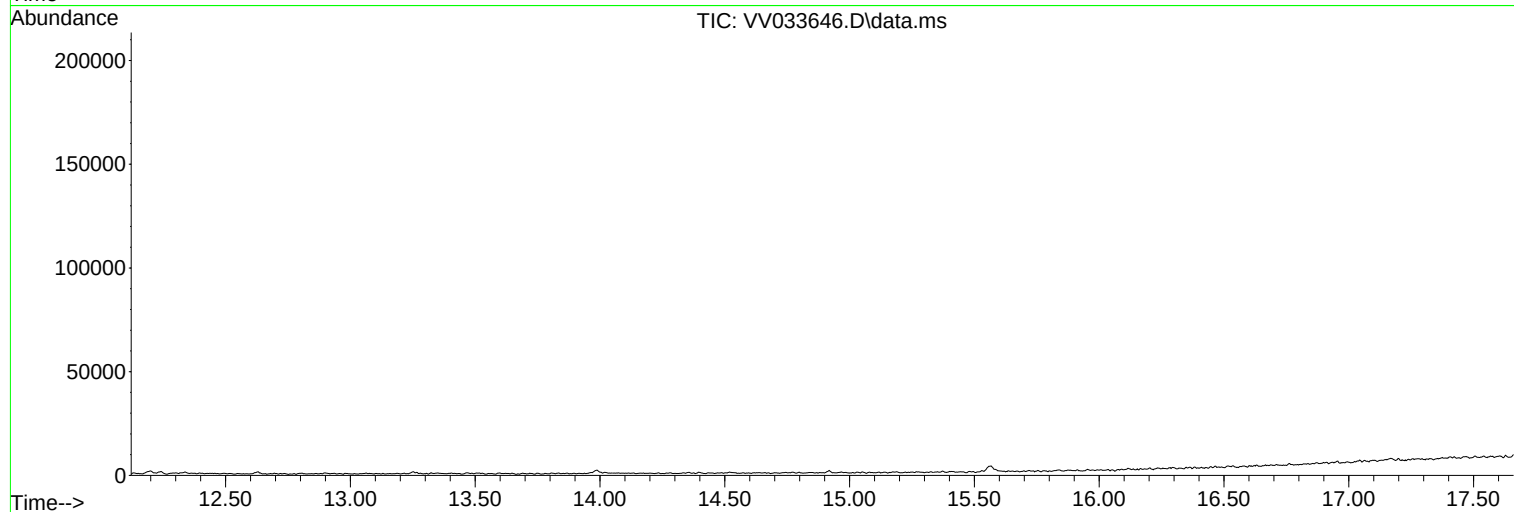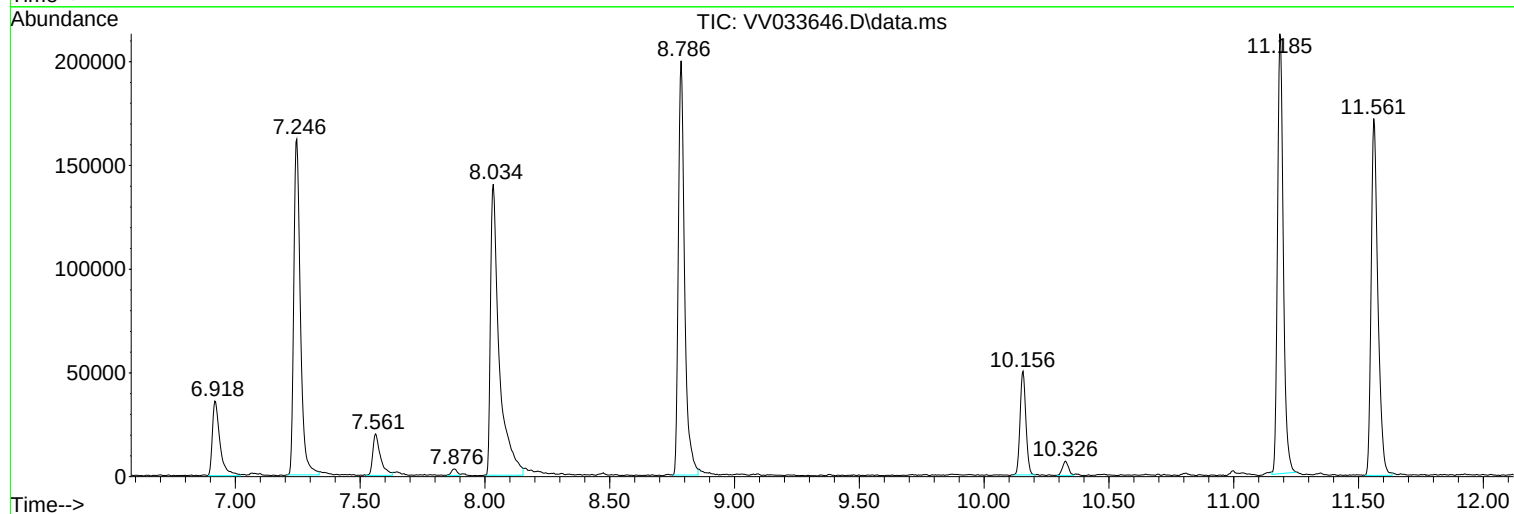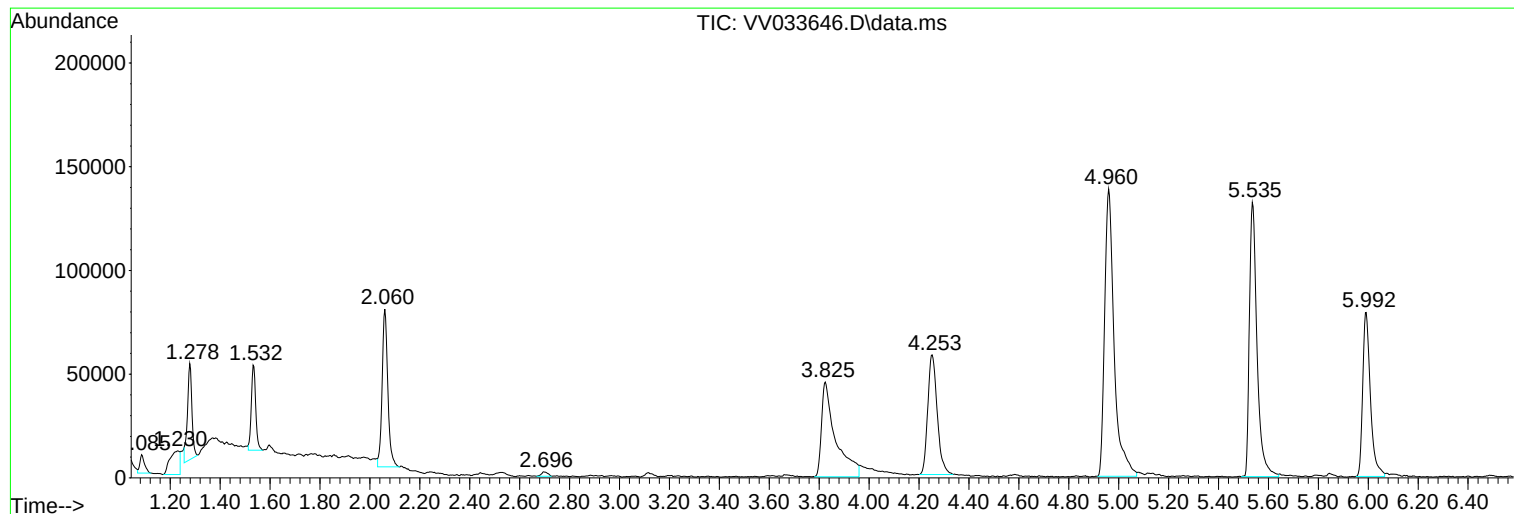

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033646.D
Acq On : 15 Jan 2024 16:34
Operator : SY/MD
Sample : P1131-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033646.D
Acq On : 15 Jan 2024 16:34
Operator : SY/MD
Sample : P1131-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc