


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011524\
Data File : VV033627.D
Acq On : 15 Jan 2024 08:28
Operator : SY/MD
Sample : BFB238
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB238

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 18 00:02:20 2024

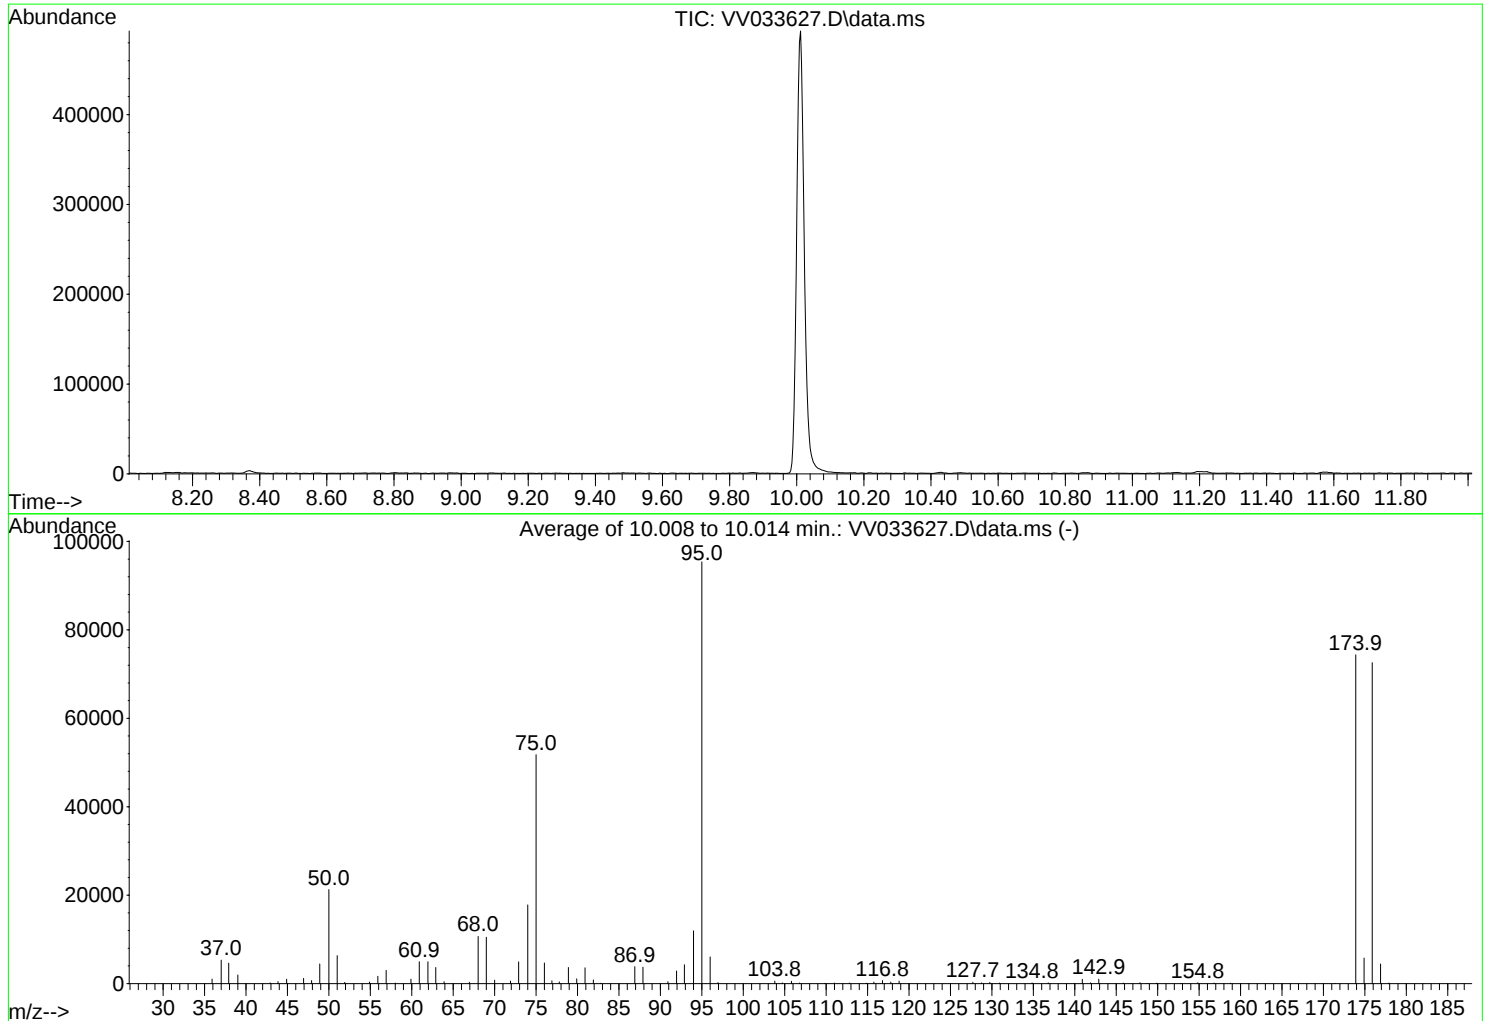

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	21267	PASS
75	95	30	80	54.3	51771	PASS
95	95	100	100	100.0	95384	PASS
96	95	5	9	6.3	6040	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.0	74363	PASS
175	174	5	9	7.8	5784	PASS
176	174	95	105	97.6	72595	PASS
177	176	5	10	6.1	4460	PASS

m/z	Abundance
39.80	193.0
40.90	159.0
43.80	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	1035.0
37.00	5611.0
37.90	4839.0
39.00	2063.0
39.90	187.0
40.90	151.0
42.90	167.0
43.90	769.0
44.90	1012.0
46.90	1277.0
47.90	754.0
48.90	4693.0
50.00	21680.0
51.00	6557.0
51.90	322.0
54.90	406.0
55.90	1777.0
56.90	3016.0
58.00	115.0
59.90	987.0
60.90	5082.0
62.00	5169.0
62.90	3691.0
63.90	486.0
67.00	369.0
68.00	10843.0
69.00	10760.0
70.00	874.0
71.90	556.0
72.90	4917.0
74.00	17952.0
75.00	52864.0
76.00	4901.0
76.90	616.0
77.80	432.0
78.90	3698.0
79.90	1065.0
80.90	3660.0
81.90	845.0
82.80	110.0
86.90	3960.0
87.90	3980.0
90.90	446.0
92.00	2989.0
92.90	4341.0
94.00	11885.0
95.00	95976.0
96.00	6249.0
96.90	260.0
103.80	574.0
104.70	213.0
105.80	528.0
106.80	165.0
111.00	140.0
112.80	145.0
114.80	109.0
115.80	395.0
116.80	721.0
117.80	358.0
118.80	530.0
127.70	387.0
128.80	160.0
129.70	296.0
130.90	164.0
134.80	199.0
136.80	192.0
140.00	119.0
140.90	1033.0
141.90	171.0
142.90	1035.0
145.90	132.0
147.90	216.0
148.70	104.0
149.80	125.0
154.90	220.0
156.80	139.0
158.80	123.0
173.90	73224.0
174.90	5808.0
175.90	71512.0
176.90	4535.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	1087.0
37.00	5511.0
37.90	4764.0
39.00	1989.0
39.90	192.0
40.90	139.0
42.90	203.0
43.90	768.0
44.90	1081.0
46.90	1267.0
47.90	712.0
48.90	4587.0
50.00	22064.0
51.00	6579.0
51.90	291.0
54.90	385.0
55.90	1689.0
56.90	3091.0
58.00	142.0
59.90	1066.0
60.90	5082.0
61.90	5137.0
62.90	3791.0
63.90	421.0
66.90	341.0
68.00	11010.0
69.00	10870.0
70.00	810.0
71.90	583.0
72.90	5100.0
74.00	18488.0
75.00	53368.0
76.00	4794.0
76.90	675.0
77.80	434.0
78.90	3768.0
79.90	1136.0
80.90	3712.0
81.90	899.0
82.80	123.0
86.90	3987.0
87.90	3832.0
90.90	467.0
91.90	2965.0
92.90	4367.0
94.00	12303.0
95.00	98608.0
96.00	6200.0
97.00	259.0
103.80	598.0
104.70	200.0
105.80	574.0
106.80	180.0
109.90	114.0
111.00	138.0
112.80	157.0
114.90	113.0
115.80	350.0
116.80	715.0
117.80	351.0
118.80	601.0
127.70	350.0
128.80	177.0
129.80	317.0
130.90	168.0
134.90	202.0
136.80	190.0
139.90	110.0
140.90	982.0
141.90	189.0
142.90	1048.0
145.80	139.0
147.90	211.0
148.70	106.0
149.90	122.0
152.80	121.0
154.90	233.0
156.80	161.0
158.80	137.0
171.40	115.0
173.90	76888.0
174.90	6010.0
175.90	75096.0
176.90	4621.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	985.0
37.00	4886.0
37.90	4246.0
39.00	1803.0
39.80	185.0
41.00	134.0
42.90	202.0
43.90	719.0
44.90	995.0
47.00	1101.0
47.90	655.0
48.90	4100.0
50.00	20056.0
51.00	5899.0
51.90	253.0
54.90	311.0
55.90	1510.0
56.90	2869.0
58.00	131.0
59.90	993.0
60.90	4760.0
61.90	4619.0
62.90	3511.0
63.90	397.0
66.90	268.0
68.00	10196.0
69.00	9859.0
70.00	680.0
71.90	574.0
72.90	4740.0
74.00	16976.0
75.00	49080.0
76.00	4292.0
76.90	637.0
77.80	373.0
78.90	3490.0
79.90	1072.0
80.90	3366.0
81.90	808.0
82.80	132.0
86.90	3591.0
87.90	3343.0
90.90	433.0
91.90	2665.0
92.90	4064.0
94.00	11595.0
95.00	91568.0
96.00	5671.0
97.00	215.0
103.80	554.0
104.70	157.0
105.80	543.0
106.80	128.0
109.80	102.0
111.00	111.0
112.80	127.0
114.80	109.0
115.70	307.0
116.80	652.0
117.80	348.0
118.80	578.0
127.70	282.0
128.70	163.0
129.80	313.0
130.90	137.0
134.90	173.0
136.80	153.0
140.90	898.0
141.90	165.0
142.90	984.0
145.80	126.0
147.80	199.0
149.90	106.0
152.80	101.0
154.80	205.0
156.80	148.0
158.80	121.0
160.90	111.0
171.40	114.0
173.90	72976.0
174.90	5534.0
175.90	71176.0
176.90	4225.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238