

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011620\
 Data File : VV014315.D
 Acq On : 16 Jan 2020 10:37
 Operator : SY/MD
 Sample : VV0116WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK50

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	38	43	49	rBV2	36503	33085	1.25%	0.148%
2	1.319	64	71	83	rVB	369861	365822	13.79%	1.637%
3	1.585	147	154	167	rVB	278444	319894	12.06%	1.431%
4	2.129	314	323	335	rBV	510148	717291	27.04%	3.209%
5	2.537	442	450	466	rVB2	37896	71244	2.69%	0.319%
6	3.949	878	889	922	rBV2	207074	766925	28.91%	3.431%
7	4.396	1012	1028	1049	rVB	450715	1097140	41.36%	4.909%
8	5.093	1225	1245	1264	rBV2	1088937	2640590	99.54%	11.815%
9	5.659	1403	1421	1441	rBV	997267	1978933	74.60%	8.854%
10	6.113	1548	1562	1579	rBV	631052	1267751	47.79%	5.672%
11	7.026	1830	1846	1865	rBV	359327	647394	24.40%	2.897%
12	7.354	1936	1948	1966	rBV	1328609	2319551	87.44%	10.378%
13	7.659	2031	2043	2062	rBV	200596	358373	13.51%	1.603%
14	8.132	2179	2190	2228	rBV	1236732	2652830	100.00%	11.869%
15	8.891	2414	2426	2454	rBV	1437610	2344363	88.37%	10.489%
16	10.254	2840	2850	2866	rBV	411609	671253	25.30%	3.003%
17	11.289	3160	3172	3190	rBV	1441611	2220667	83.71%	9.936%
18	11.665	3275	3289	3305	rBV	1163033	1846049	69.59%	8.260%
19	12.292	3476	3484	3492	rVB2	18761	30893	1.16%	0.138%




Sum of corrected areas: 22350048

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV011620\
Data File : VV014315.D
Acq On : 16 Jan 2020 10:37
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

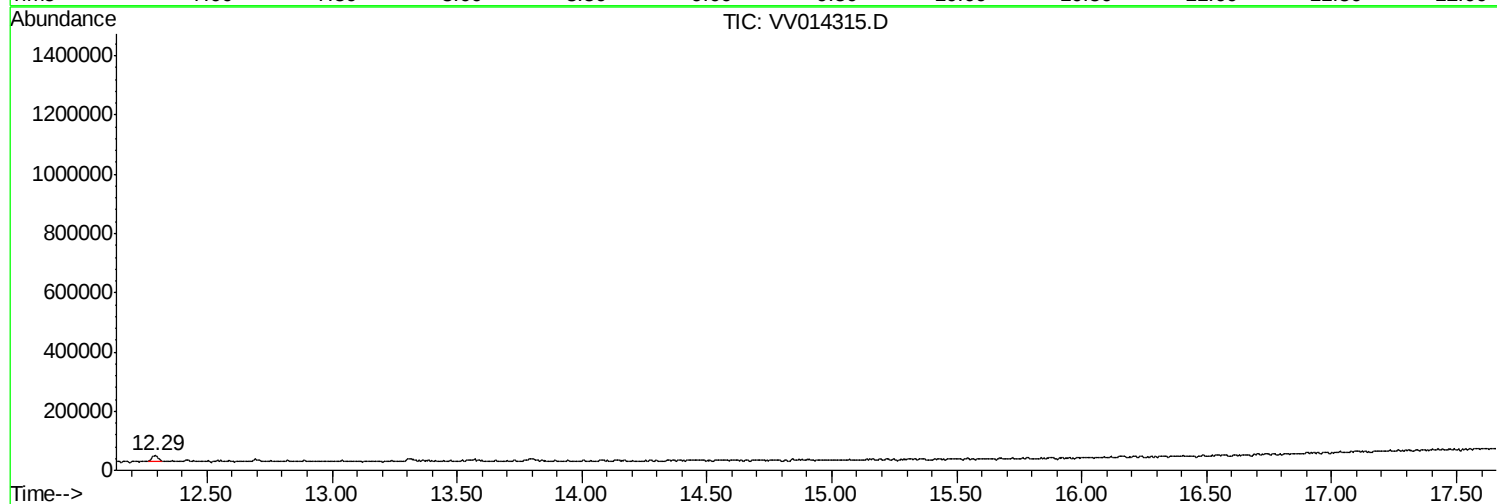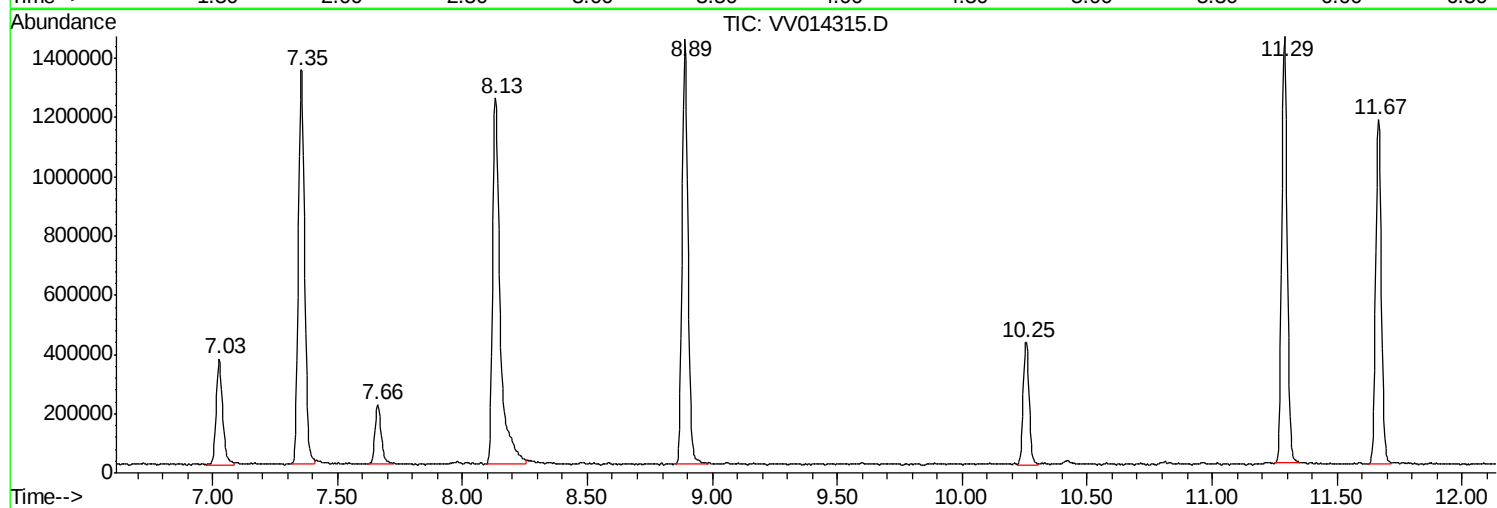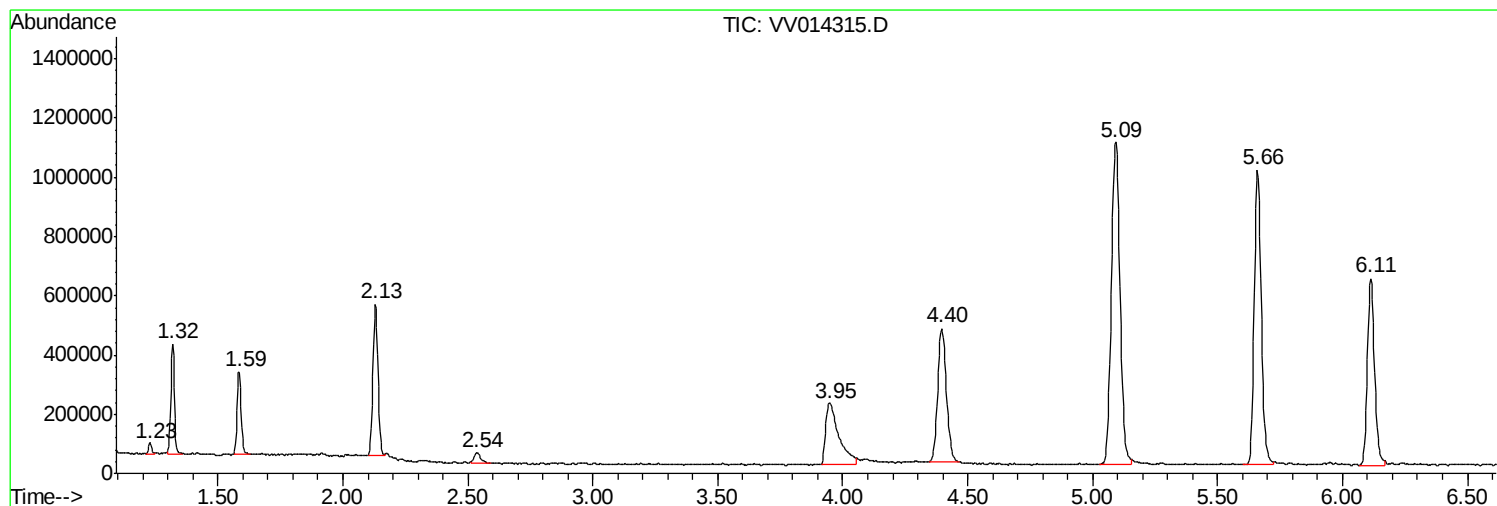

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV011620\
Data File : VV014315.D
Acq On : 16 Jan 2020 10:37
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK50

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV011620\
Data File : VV014315.D
Acq On : 16 Jan 2020 10:37
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK50

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc