

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
 Data File : VV029867.D
 Acq On : 16 Jan 2023 10:56
 Operator : SY/MD
 Sample : VV0116WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK292

Quant Time: Jan 17 00:37:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 12 22:05:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	200484	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	191186	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	91248	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	73446	4.830	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	96.600%	
7) Chloroethane-d5	1.565	69	68192	5.410	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.200%	
11) 1,1-Dichloroethene-d2	2.105	63	102469	3.696	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	74.000%	
20) 2-Butanone-d5	3.892	46	147507	54.729	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.460%	
24) Chloroform-d	4.339	84	155328	5.568	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	111.400%	
26) 1,2-Dichloroethane-d4	5.024	65	67988	5.755	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	115.200%	
32) Benzene-d6	5.043	84	315944	5.571	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	111.400%	
36) 1,2-Dichloropropane-d6	6.063	67	94999	5.724	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	114.400%	
41) Toluene-d8	7.307	98	270240	5.147	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.000%	
43) trans-1,3-Dichloroprop...	7.616	79	30113	4.968	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.400%	
46) 2-Hexanone-d5	8.085	63	135489	54.903	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.800%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	65970	5.424	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	108.400%	
66) 1,2-Dichlorobenzene-d4	11.612	152	95418	5.752	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.000%	
Target Compounds						
16) Methylene chloride	2.507	84	5162	0.243	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029867.D
Acq On : 16 Jan 2023 10:56
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Time: Jan 17 00:37:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 12 22:05:54 2023
Response via : Initial Calibration

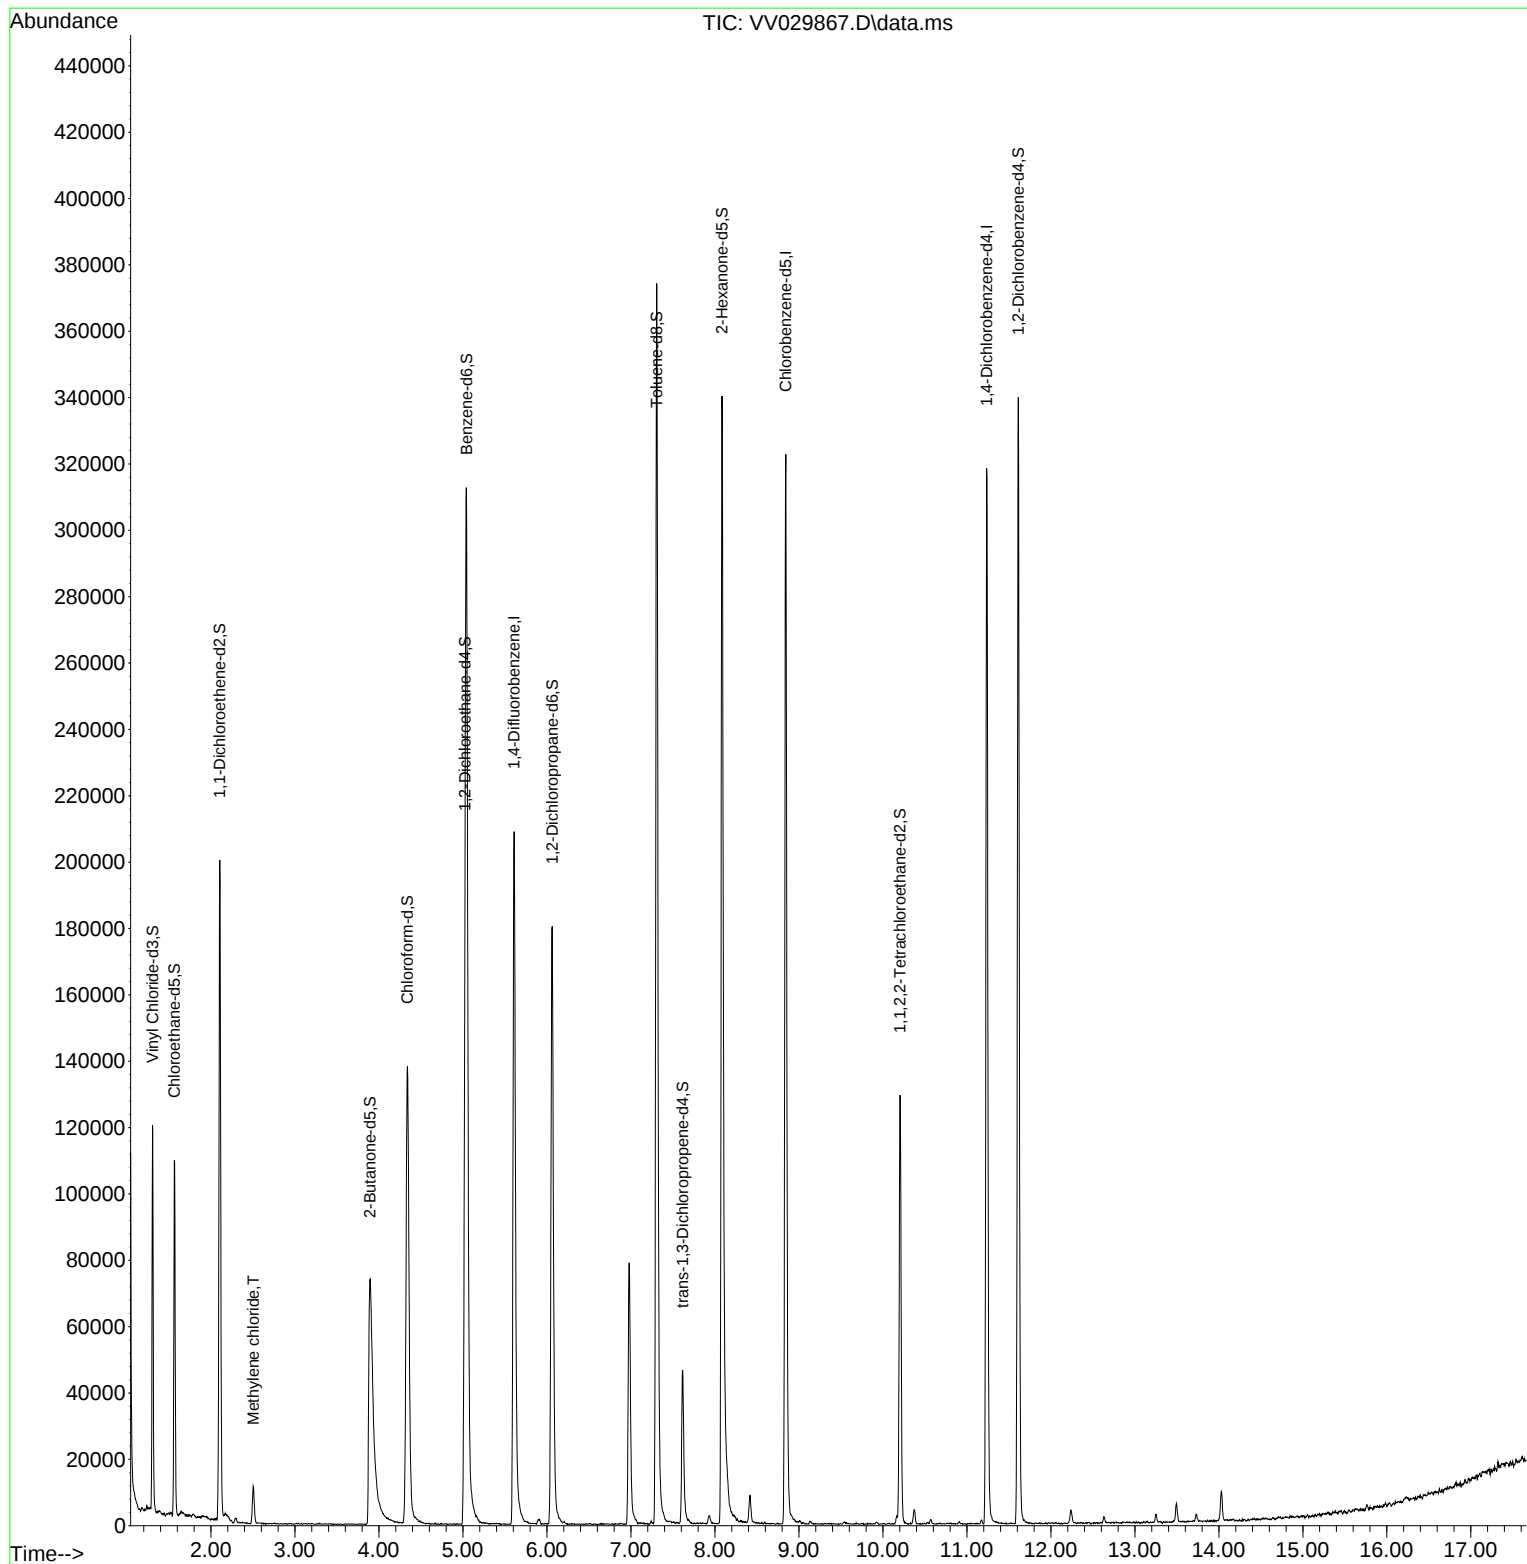

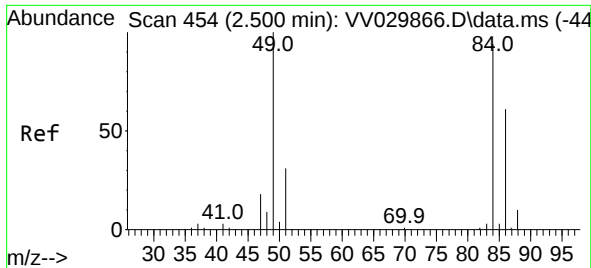

#16

Methylene chloride

Concen: 0.243 ug/L

RT: 2.507 min Scan# 4

Delta R.T. 0.010 min

Lab File: VV029867.D


Acq: 16 Jan 2023 10:56

Instrument :

MSVOA_V

ClientSampleId :

VBLK292

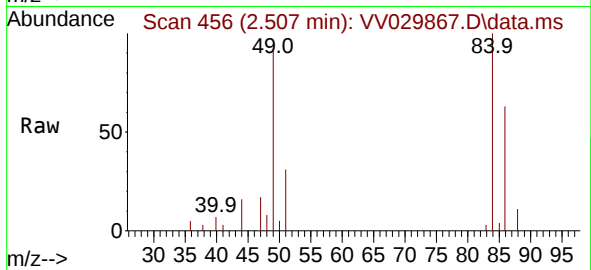

Tgt Ion: 84 Resp: 5162

Ion Ratio Lower Upper

84 100

86 63.0 45.0 83.6

49 90.9 71.5 132.7

