

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011623\
 Data File : VW029875.D
 Acq On : 16 Jan 2023 14:32
 Operator : SY/MD
 Sample : 01168-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1Z4

Quant Time: Jan 17 00:38:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 12 22:05:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	185688	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	181351	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	96705	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	60019	4.261	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.200%
7) Chloroethane-d5	1.564	69	58715	5.029	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.600%
11) 1,1-Dichloroethene-d2	2.105	63	86047	3.351	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%
20) 2-Butanone-d5	3.892	46	143009	57.288	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.580%
24) Chloroform-d	4.339	84	137094	5.306	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
26) 1,2-Dichloroethane-d4	5.024	65	60799	5.557	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.200%
32) Benzene-d6	5.043	84	275858	5.128	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
36) 1,2-Dichloropropane-d6	6.063	67	85319	5.419	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.307	98	235018	4.719	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.616	79	26260	4.567	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.085	63	128001	54.681	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.360%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	65181	5.650	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	96322	5.479	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.600%
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	7648	4.292	ug/L	88
53) m,p-Xylene	9.133	106	1231	0.046	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029875.D
Acq On : 16 Jan 2023 14:32
Operator : SY/MD
Sample : 01168-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z4

Quant Time: Jan 17 00:38:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 12 22:05:54 2023
Response via : Initial Calibration




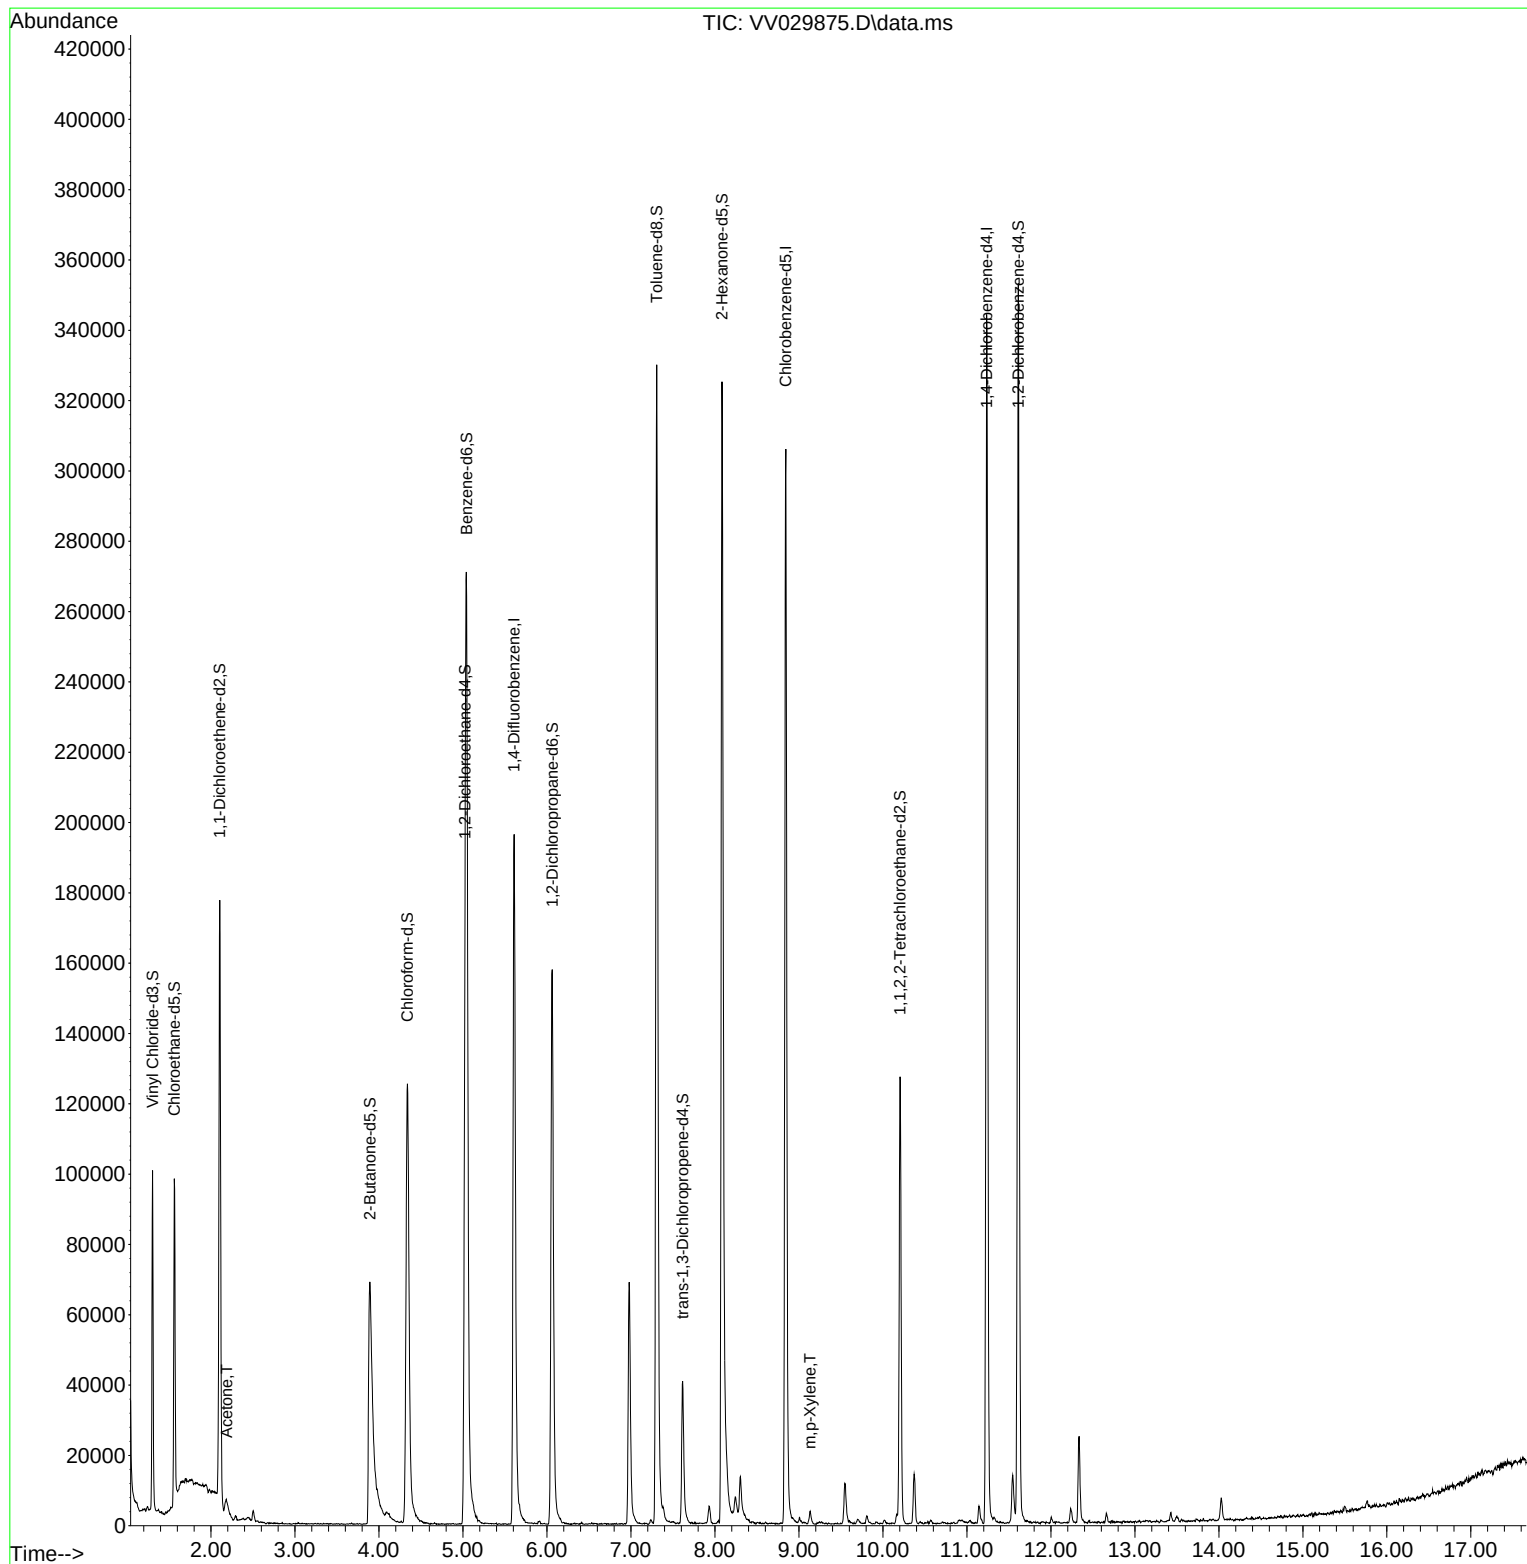


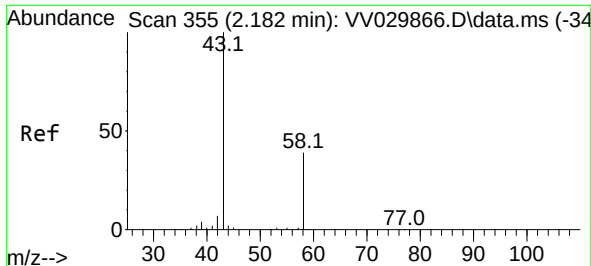

#13
Acetone
Concen: 4.292 ug/L
RT: 2.185 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV029875.D
Acq: 16 Jan 2023 14:32

Instrument :
MSVOA_V
ClientSampleId :
BH1Z4

Tgt Ion: 43 Resp: 7648
Ion Ratio Lower Upper
43 100
58 27.8 0.0 68.8

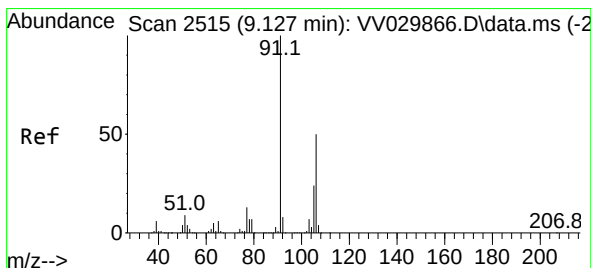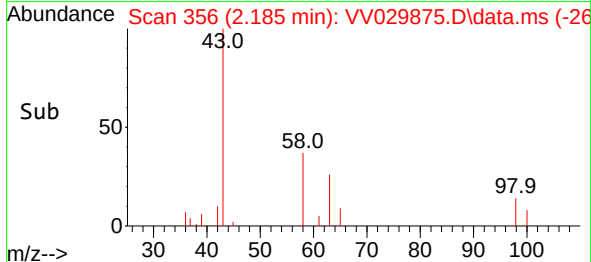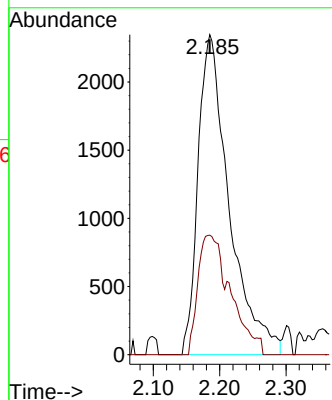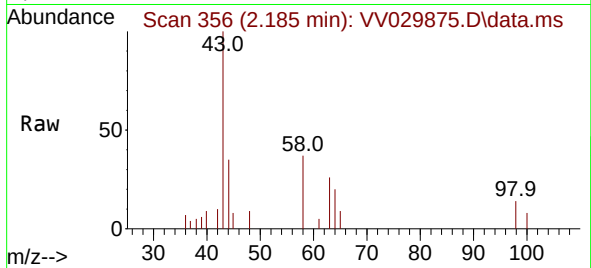

#53
m,p-Xylene
Concen: 0.046 ug/L
RT: 9.133 min Scan# 2517
Delta R.T. 0.003 min
Lab File: VV029875.D
Acq: 16 Jan 2023 14:32

Tgt Ion:106 Resp: 1231
Ion Ratio Lower Upper
106 100
91 210.5 138.7 257.7

