

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
 Data File : VV029867.D
 Acq On : 16 Jan 2023 10:56
 Operator : SY/MD
 Sample : VV0116WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK292

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	116658	117343	14.68%	1.894%
2	1.565	155	163	176	rBV	107238	122298	15.30%	1.974%
3	2.105	321	331	346	rBV	198698	285133	35.68%	4.603%
4	2.503	445	455	469	rBV2	11390	18305	2.29%	0.296%
5	3.896	872	888	934	rBV2	73971	287490	35.98%	4.641%
6	4.339	1009	1026	1054	rBV	137543	349462	43.73%	5.641%
7	5.040	1227	1244	1281	rBV2	312480	799074	100.00%	12.900%
8	5.609	1409	1421	1461	rBV	208749	437762	54.78%	7.067%
9	6.063	1548	1562	1596	rBV	180102	377518	47.24%	6.094%
10	6.979	1836	1847	1880	rBV	78814	151741	18.99%	2.450%
11	7.307	1937	1949	1973	rBV	373864	670220	83.87%	10.820%
12	7.616	2032	2045	2065	rBV2	46289	84789	10.61%	1.369%
13	8.085	2180	2191	2226	rBV	339688	661235	82.75%	10.675%
14	8.416	2284	2294	2308	rVB3	8130	13249	1.66%	0.214%
15	8.844	2412	2427	2458	rBV	322370	540063	67.59%	8.718%
16	10.204	2840	2850	2866	rVB	128783	205882	25.77%	3.324%
17	11.236	3159	3171	3196	rBV	318140	508562	63.64%	8.210%
18	11.612	3275	3288	3307	rBV	339582	541743	67.80%	8.746%
19	13.493	3864	3873	3882	rBV2	5409	8015	1.00%	0.129%
20	14.030	4028	4040	4053	rBV	8858	14635	1.83%	0.236%




Sum of corrected areas: 6194519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029867.D
Acq On : 16 Jan 2023 10:56
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

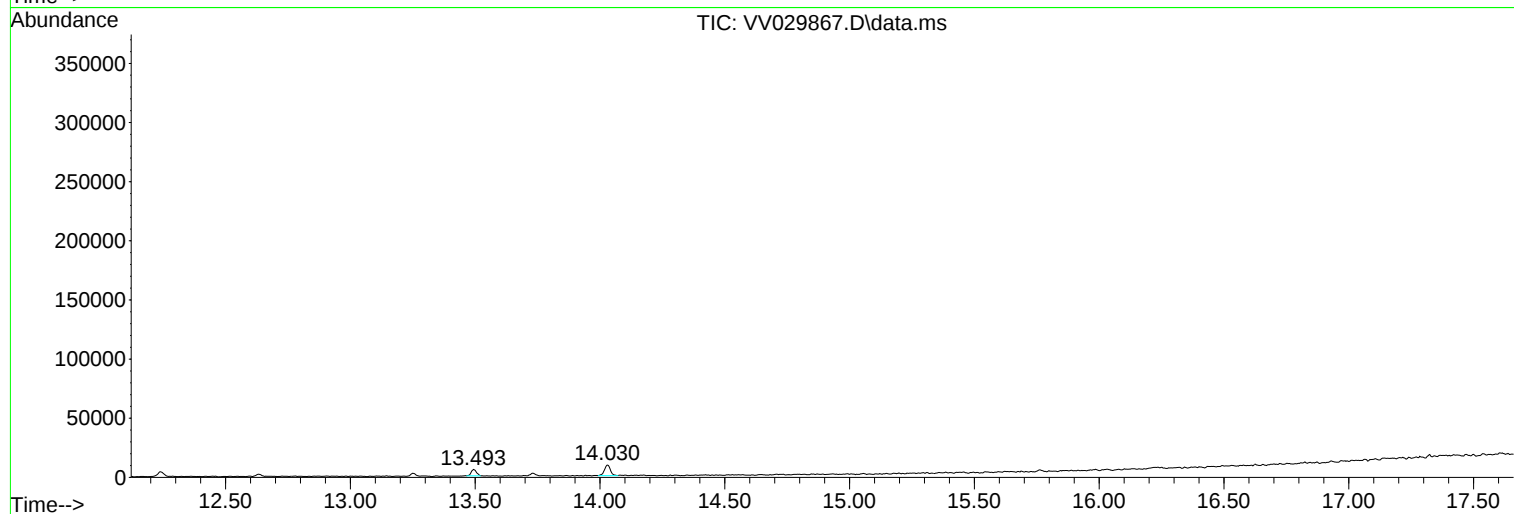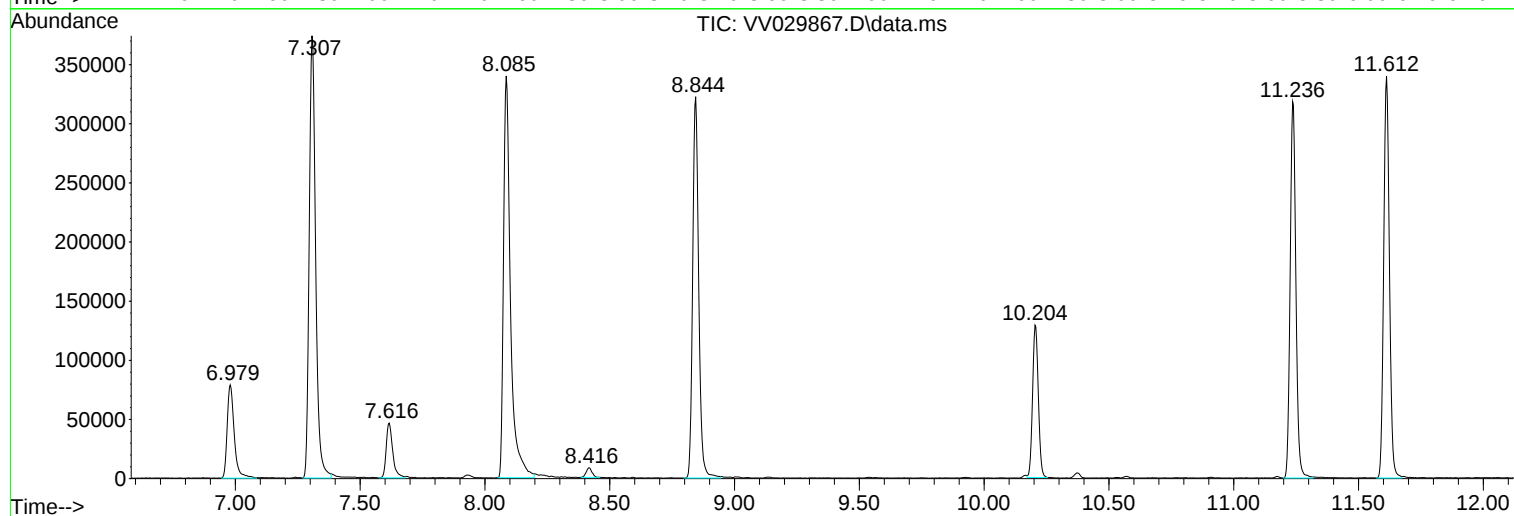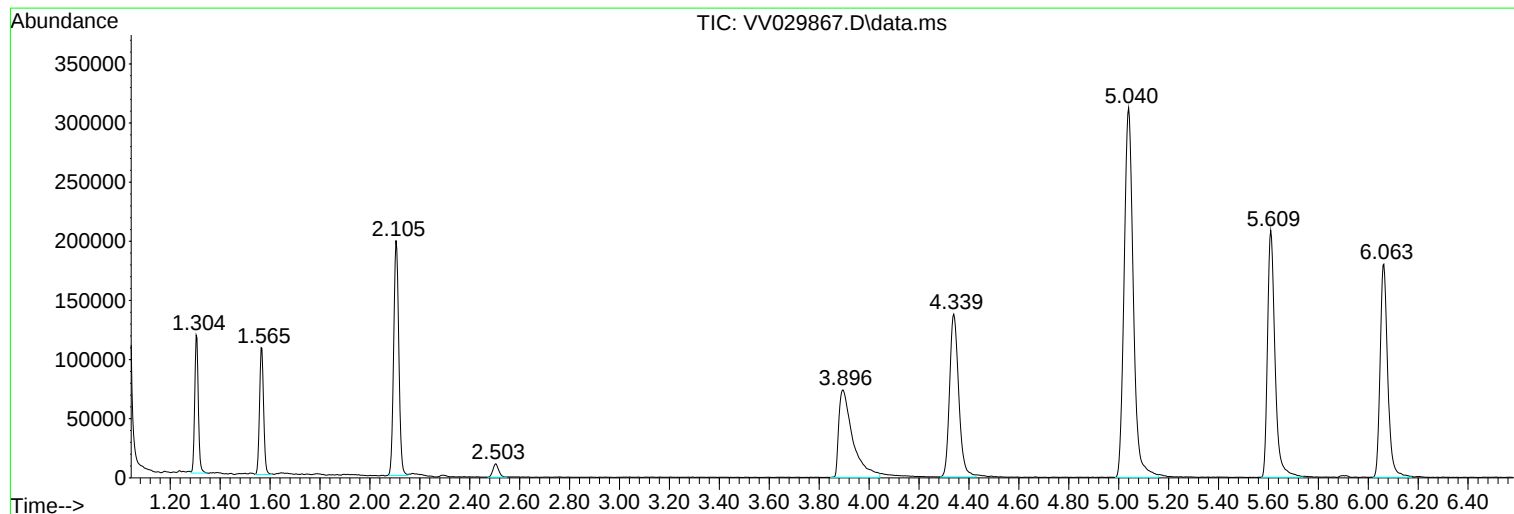

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029867.D
Acq On : 16 Jan 2023 10:56
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029867.D
Acq On : 16 Jan 2023 10:56
Operator : SY/MD
Sample : VV0116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK292

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
