

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
 Data File : VV029868.D
 Acq On : 16 Jan 2023 11:30
 Operator : SY/MD
 Sample : 01136-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	115965	121501	15.55%	1.892%
2	1.564	156	163	177	rBV2	105652	187180	23.96%	2.915%
3	2.105	321	331	344	rVB	210596	313835	40.17%	4.888%
4	2.175	347	353	370	rVB2	10170	22400	2.87%	0.349%
5	2.291	379	389	399	rVB	9345	14061	1.80%	0.219%
6	2.500	445	454	469	rVB2	12820	22404	2.87%	0.349%
7	2.757	523	534	548	rBV5	5027	10042	1.29%	0.156%
8	3.031	609	619	632	rVB2	5018	9958	1.27%	0.155%
9	3.182	651	666	680	rBV4	3783	8029	1.03%	0.125%
10	3.883	868	884	924	rBV	63961	217494	27.84%	3.387%
11	4.333	1007	1024	1049	rBV	135071	339225	43.42%	5.283%
12	5.034	1223	1242	1284	rBV2	300420	781182	100.00%	12.167%
13	5.606	1406	1420	1449	rBV	224695	467436	59.84%	7.280%
14	6.056	1548	1560	1597	rBV	173300	369395	47.29%	5.753%
15	6.976	1835	1846	1875	rBV	77636	147348	18.86%	2.295%
16	7.304	1936	1948	1966	rVV	364597	661083	84.63%	10.296%
17	7.381	1966	1972	1990	rVB	10572	22525	2.88%	0.351%
18	7.612	2031	2044	2062	rBV	44426	81510	10.43%	1.270%
19	7.931	2130	2143	2158	rBV2	8190	15706	2.01%	0.245%
20	8.082	2180	2190	2226	rBV	290148	565416	72.38%	8.806%
21	8.841	2415	2426	2447	rBV	353620	586069	75.02%	9.128%
22	9.133	2504	2517	2527	rBV	6758	11121	1.42%	0.173%
23	10.204	2840	2850	2867	rVB	130328	203287	26.02%	3.166%
24	10.371	2887	2902	2913	rBV2	22468	37652	4.82%	0.586%
25	11.236	3159	3171	3193	rBV	386534	598945	76.67%	9.329%
26	11.612	3276	3288	3311	rVB	378158	592283	75.82%	9.225%
27	12.233	3470	3481	3493	rBV5	6964	13444	1.72%	0.209%




Sum of corrected areas: 6420531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029868.D
Acq On : 16 Jan 2023 11:30
Operator : SY/MD
Sample : 01136-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

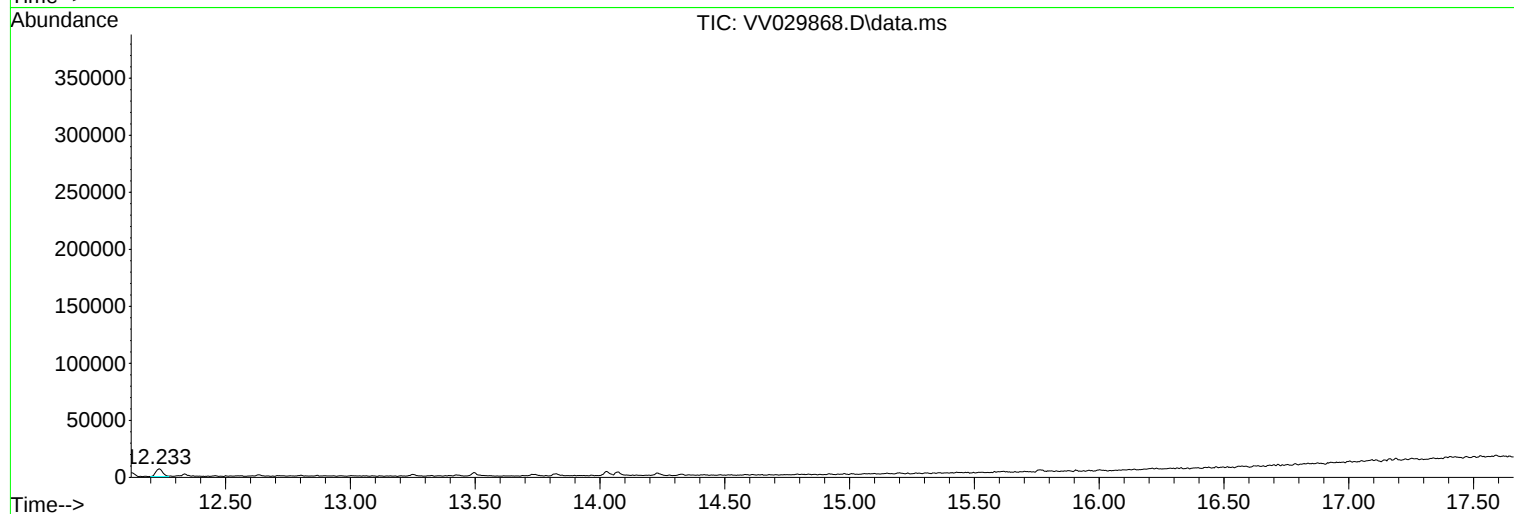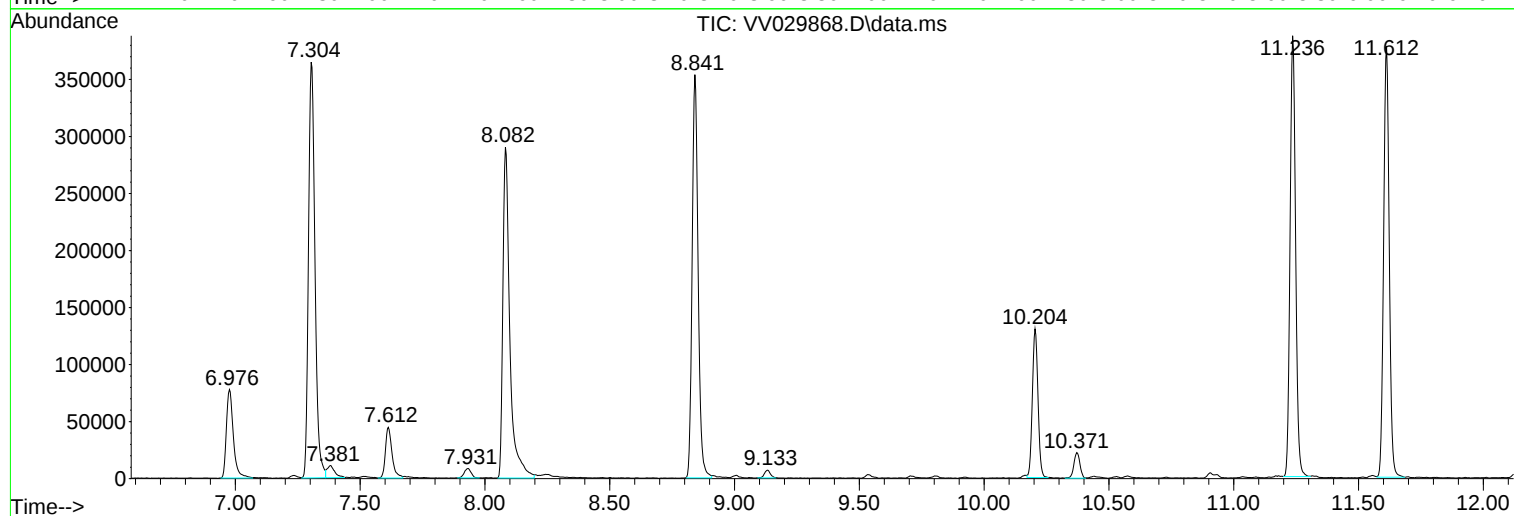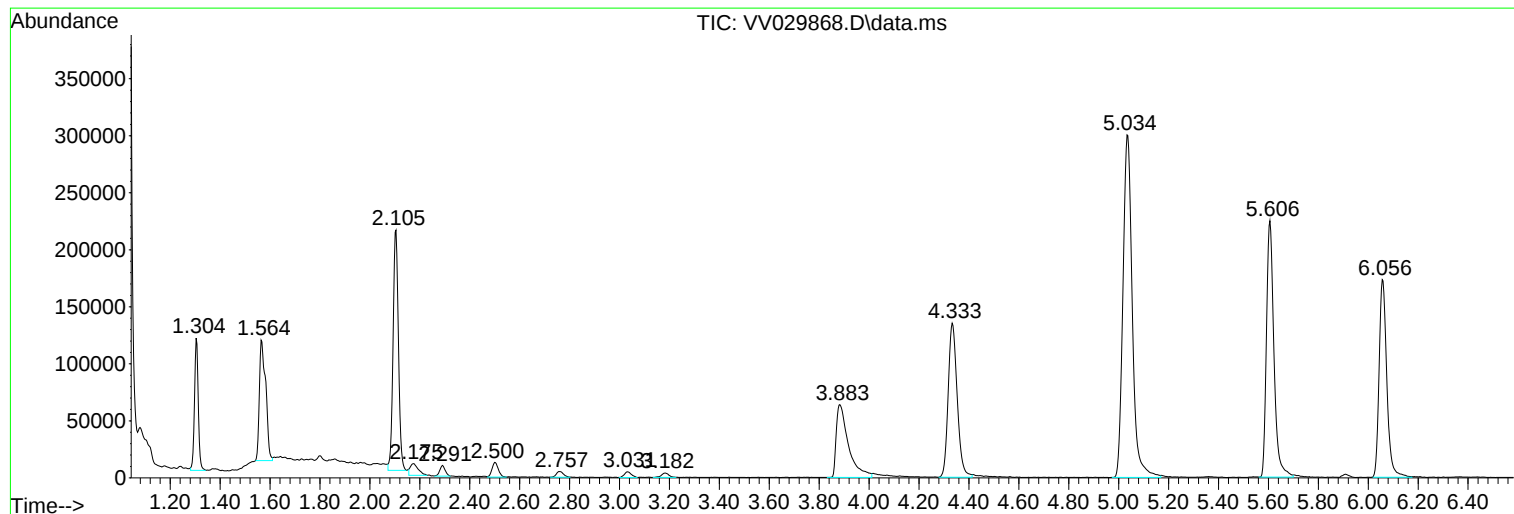

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029868.D
Acq On : 16 Jan 2023 11:30
Operator : SY/MD
Sample : 01136-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029868.D
Acq On : 16 Jan 2023 11:30
Operator : SY/MD
Sample : 01136-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc