

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
 Data File : VV029875.D
 Acq On : 16 Jan 2023 14:32
 Operator : SY/MD
 Sample : 01168-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1Z4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	96848	96876	13.71%	1.642%
2	1.564	155	163	175	rBV	93426	112305	15.89%	1.904%
3	2.105	321	331	346	rVB	173643	254536	36.01%	4.314%
4	2.182	348	355	381	rVB3	6020	18517	2.62%	0.314%
5	3.892	876	887	912	rBV	68707	228611	32.34%	3.875%
6	4.339	1008	1026	1056	rBV	124843	328777	46.51%	5.573%
7	5.040	1227	1244	1280	rBV2	270730	706852	100.00%	11.981%
8	5.609	1409	1421	1453	rBV	196160	406260	57.47%	6.886%
9	6.063	1548	1562	1600	rBV	157735	337810	47.79%	5.726%
10	6.979	1834	1847	1881	rBV	68794	131889	18.66%	2.235%
11	7.307	1937	1949	1970	rBV	329522	590823	83.59%	10.014%
12	7.616	2035	2045	2070	rBV	40270	73789	10.44%	1.251%
13	7.931	2133	2143	2152	rBV3	4808	8004	1.13%	0.136%
14	8.085	2181	2191	2227	rBV	324567	630575	89.21%	10.688%
15	8.243	2233	2240	2250	rVV6	4430	7434	1.05%	0.126%
16	8.304	2251	2259	2274	rVB2	10959	19084	2.70%	0.323%
17	8.844	2413	2427	2450	rBV	305563	510802	72.26%	8.658%
18	9.548	2633	2646	2659	rBV4	11530	22286	3.15%	0.378%
19	10.204	2840	2850	2870	rVB	127070	203790	28.83%	3.454%
20	10.371	2891	2902	2919	rVB2	14199	24112	3.41%	0.409%
21	11.143	3135	3142	3158	rVB8	5008	9107	1.29%	0.154%
22	11.236	3158	3171	3194	rBV	343863	539327	76.30%	9.141%
23	11.545	3253	3267	3277	rBV2	13571	25705	3.64%	0.436%
24	11.612	3277	3288	3313	rVB	352151	554772	78.48%	9.403%
25	12.236	3471	3482	3495	rBV3	4173	7363	1.04%	0.125%
26	12.336	3504	3513	3526	rBV3	24491	39996	5.66%	0.678%
27	14.027	4029	4039	4051	rVB2	6180	10384	1.47%	0.176%




Sum of corrected areas: 5899786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029875.D
Acq On : 16 Jan 2023 14:32
Operator : SY/MD
Sample : 01168-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

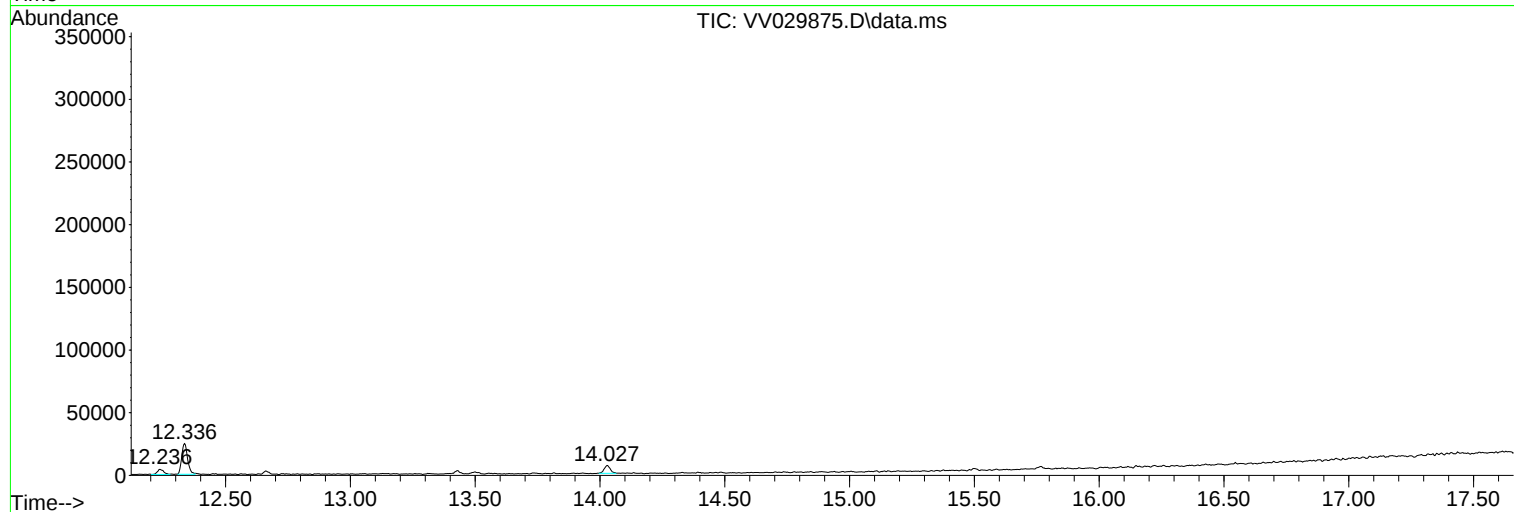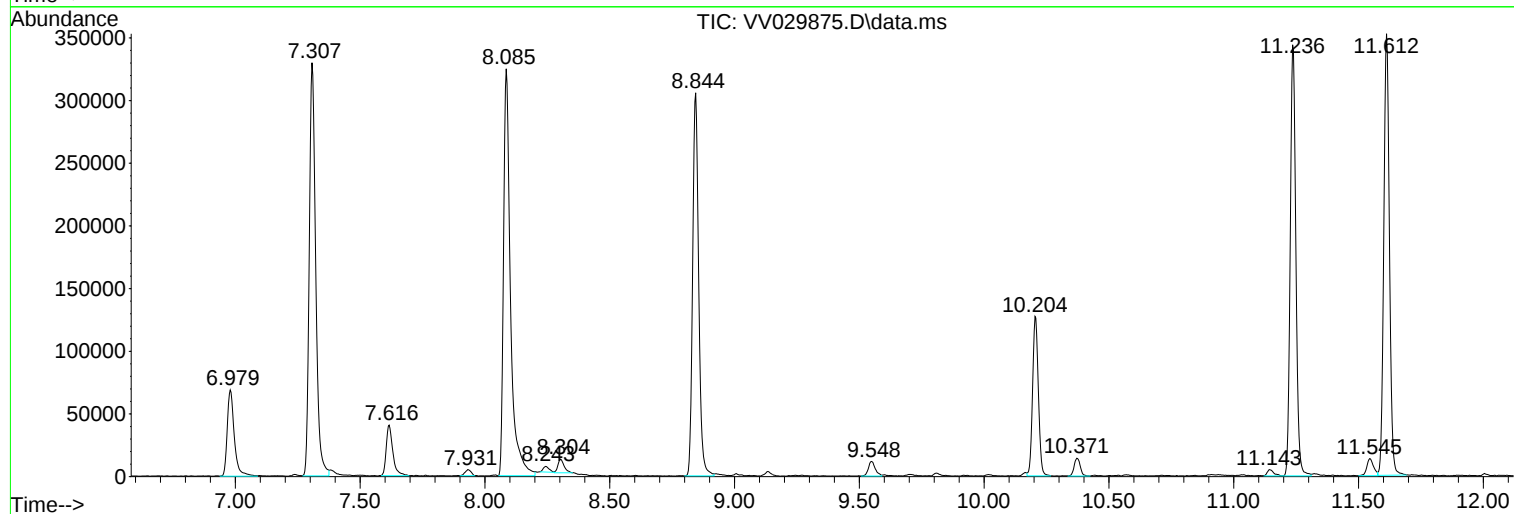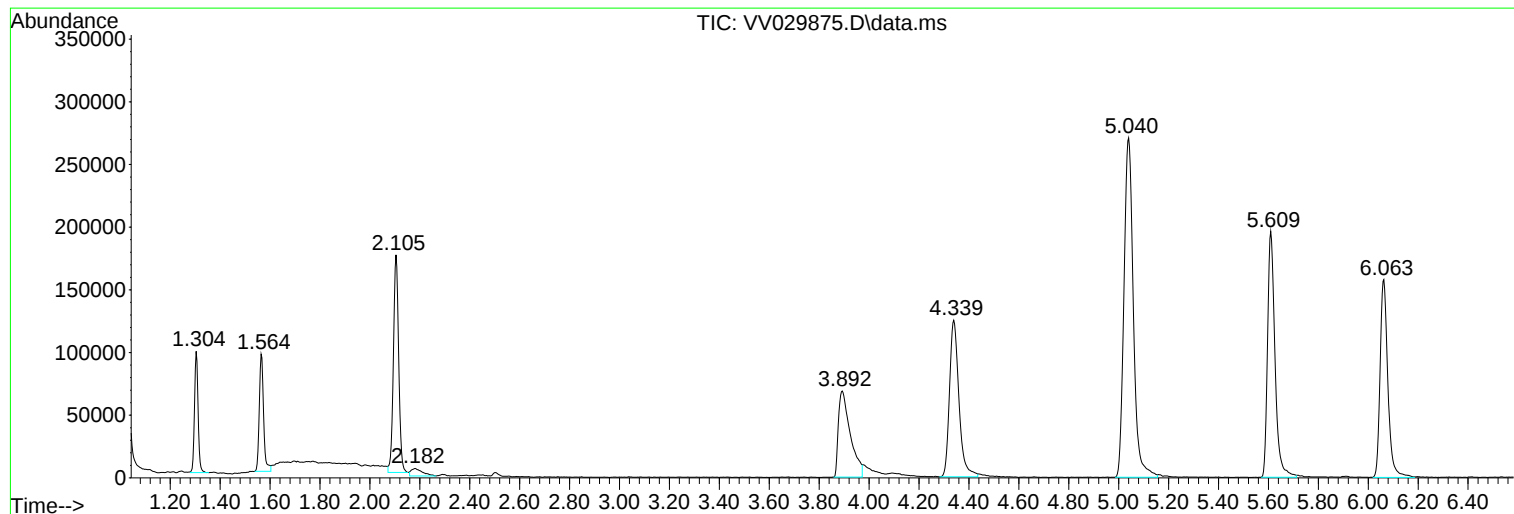

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029875.D
Acq On : 16 Jan 2023 14:32
Operator : SY/MD
Sample : 01168-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029875.D
Acq On : 16 Jan 2023 14:32
Operator : SY/MD
Sample : 01168-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
