

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
 Data File : VV029876.D
 Acq On : 16 Jan 2023 14:56
 Operator : SY/MD
 Sample : 01168-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1Z5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	96429	96267	13.50%	1.596%
2	1.564	155	163	174	rVB	91116	102177	14.33%	1.693%
3	2.104	319	331	347	rVB	168775	244808	34.33%	4.057%
4	3.889	872	886	935	rBV	70163	260960	36.60%	4.325%
5	4.339	1009	1026	1056	rBV	126315	330924	46.41%	5.485%
6	5.040	1226	1244	1291	rBV2	271278	705650	98.96%	11.695%
7	5.609	1408	1421	1446	rBV	201988	417527	58.55%	6.920%
8	6.063	1548	1562	1590	rBV	161677	338959	47.53%	5.618%
9	6.979	1836	1847	1874	rBV	69494	131568	18.45%	2.181%
10	7.307	1937	1949	1970	rBV	326658	589382	82.65%	9.768%
11	7.615	2035	2045	2070	rBV	40919	74873	10.50%	1.241%
12	7.934	2130	2144	2154	rBV3	5297	10435	1.46%	0.173%
13	8.085	2180	2191	2226	rBV	366293	713090	100.00%	11.819%
14	8.239	2232	2239	2251	rBV3	10686	18312	2.57%	0.303%
15	8.304	2251	2259	2278	rVB2	11026	21877	3.07%	0.363%
16	8.844	2415	2427	2460	rBV	332692	557741	78.21%	9.244%
17	9.548	2633	2646	2664	rBV4	11888	23364	3.28%	0.387%
18	10.207	2831	2851	2874	rVB	125960	209314	29.35%	3.469%
19	10.374	2886	2903	2916	rBV	17002	28760	4.03%	0.477%
20	11.143	3135	3142	3151	rBV6	5291	8035	1.13%	0.133%
21	11.236	3159	3171	3195	rBV	340798	539966	75.72%	8.949%
22	11.545	3255	3267	3276	rBV3	10964	19125	2.68%	0.317%
23	11.612	3276	3288	3307	rVB	337208	534312	74.93%	8.856%
24	12.239	3472	3483	3494	rBV2	4862	7809	1.10%	0.129%
25	12.336	3504	3513	3530	rBV3	23599	37627	5.28%	0.624%
26	14.030	4030	4040	4049	rBV	7059	10788	1.51%	0.179%


Sum of corrected areas: 6033650

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029876.D
Acq On : 16 Jan 2023 14:56
Operator : SY/MD
Sample : 01168-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

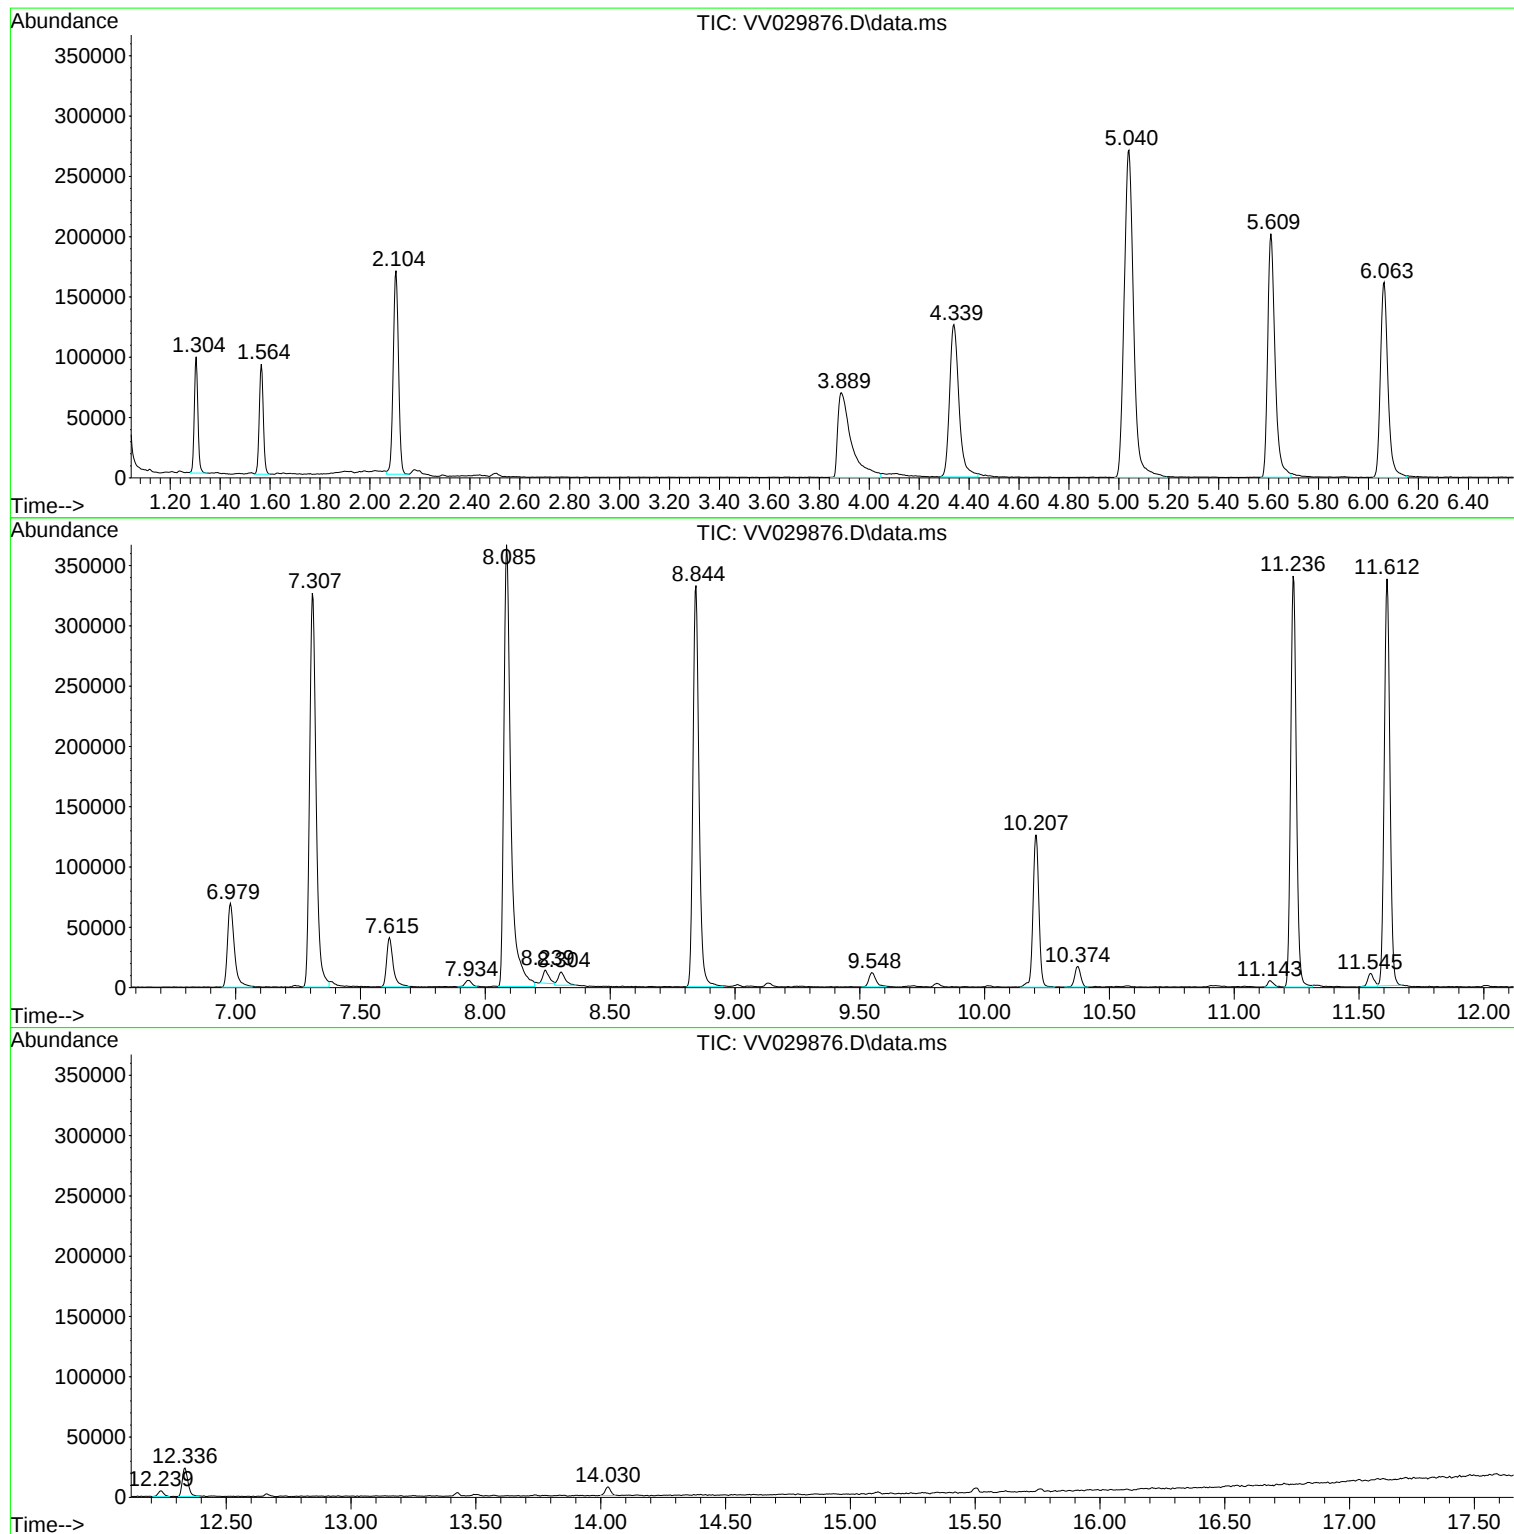

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029876.D
Acq On : 16 Jan 2023 14:56
Operator : SY/MD
Sample : 01168-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029876.D
Acq On : 16 Jan 2023 14:56
Operator : SY/MD
Sample : 01168-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc