


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011623\
Data File : VV029865.D
Acq On : 16 Jan 2023 09:05
Operator : SY/MD
Sample : BFB213
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB213

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 12 22:05:54 2023

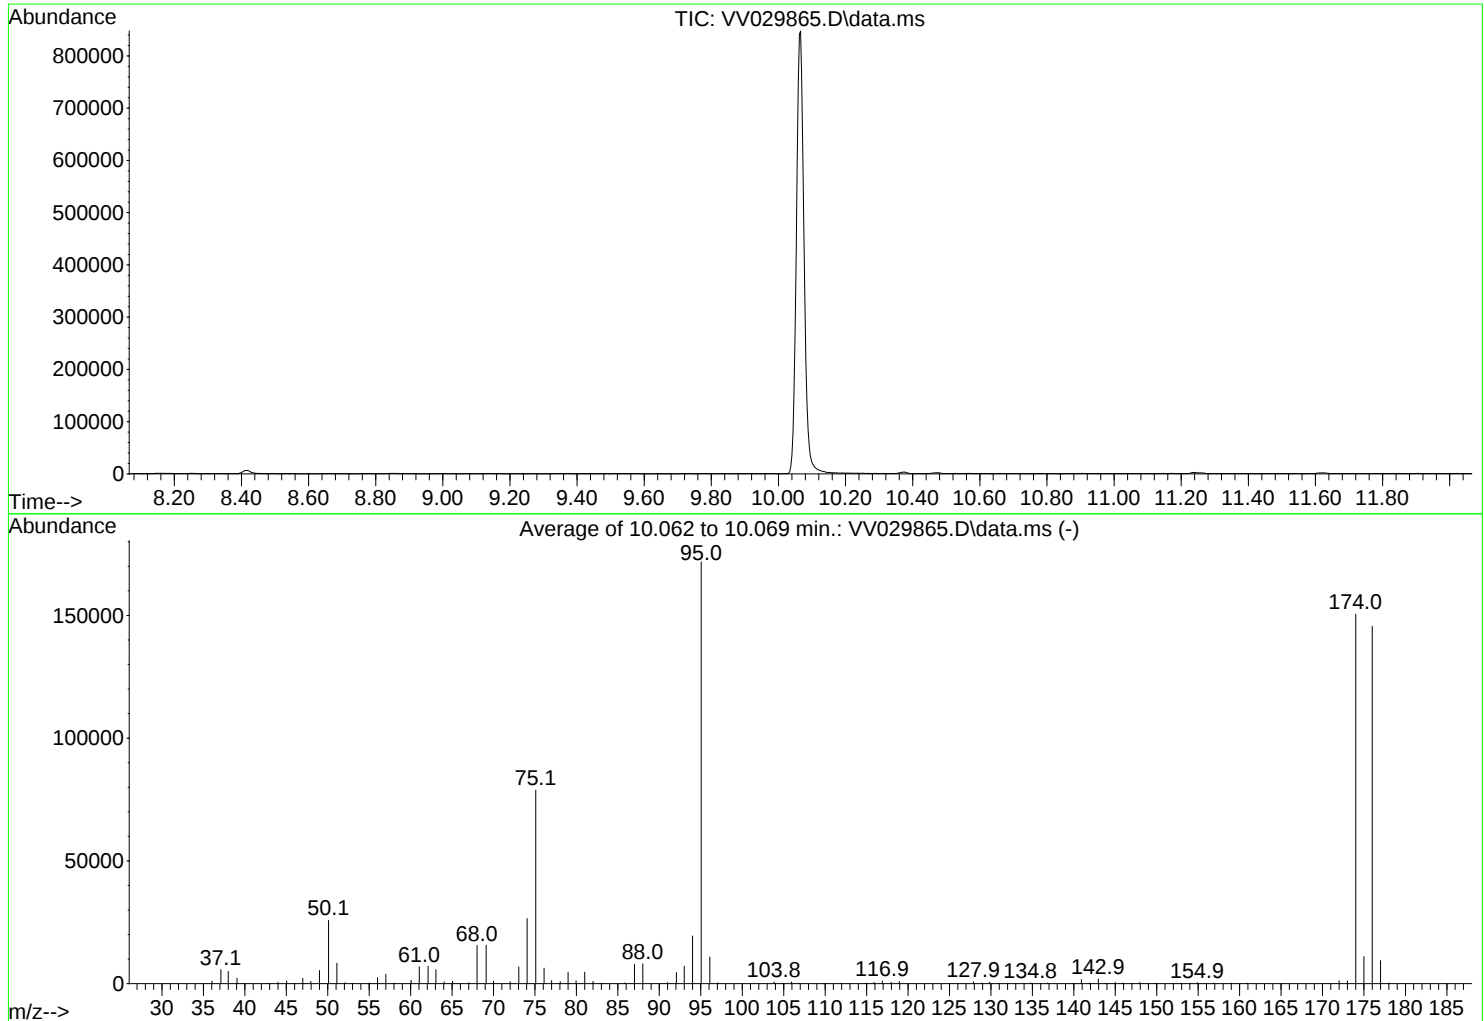

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	25781	PASS
75	95	30	80	45.9	78797	PASS
95	95	100	100	100.0	171819	PASS
96	95	5	9	6.3	10870	PASS
173	174	0.00	2	0.7	1092	PASS
174	95	50	120	87.6	150464	PASS
175	174	5	9	7.3	11051	PASS
176	174	95	105	96.8	145621	PASS
177	176	5	10	6.5	9400	PASS

m/z	Abundance
40.00	178.0
44.10	414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	1055.0
37.10	6102.0
38.00	5297.0
39.10	2252.0
40.00	242.0
42.80	105.0
44.00	979.0
45.10	1274.0
45.90	135.0
47.00	2172.0
47.90	936.0
49.00	5711.0
50.10	27104.0
51.10	8894.0
52.10	390.0
52.90	132.0
55.10	302.0
56.00	2548.0
57.00	4127.0
58.10	197.0
60.00	1418.0
61.10	7131.0
62.10	7495.0
63.00	5905.0
64.00	840.0
65.10	1050.0
67.10	419.0
68.00	16072.0
69.10	16161.0
70.00	1222.0
72.00	836.0
73.00	7009.0
74.00	27472.0
75.10	81992.0
76.10	6697.0
77.00	1243.0
78.10	784.0
79.00	4823.0
79.90	1222.0
81.00	4843.0
82.00	967.0
83.10	105.0
85.90	405.0
87.00	8210.0
88.00	8210.0
91.00	488.0
92.00	4514.0
93.00	7279.0
94.00	19704.0
95.00	177280.0
96.10	11096.0
97.00	356.0
103.80	743.0
104.90	246.0
105.90	654.0
106.90	192.0
109.80	124.0
111.90	184.0
112.90	122.0
114.90	245.0
115.90	520.0
116.90	1164.0
117.90	547.0
118.90	987.0
127.90	701.0
128.90	308.0
129.90	625.0
130.90	188.0
134.80	347.0
136.80	271.0
140.90	1619.0
141.90	263.0
142.90	2018.0
143.80	165.0
145.00	453.0
145.90	269.0
147.00	172.0
148.00	471.0
149.00	122.0
150.00	193.0
152.80	252.0
154.10	117.0
154.90	442.0
156.90	302.0
159.00	185.0
160.90	200.0
170.90	191.0
172.00	1225.0
173.00	1560.0
174.00	151616.0
175.00	11354.0
176.00	147392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

177.009435.0

178.00279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.10	1090.0
37.10	5968.0
38.00	5187.0
39.00	2257.0
40.00	205.0
42.80	122.0
44.00	995.0
45.10	1168.0
45.90	161.0
47.00	2196.0
48.00	922.0
49.00	5442.0
50.10	26552.0
51.10	8687.0
52.10	391.0
52.90	125.0
55.10	275.0
56.00	2472.0
57.00	3949.0
58.00	220.0
60.10	1382.0
61.10	7111.0
62.10	7330.0
63.10	5808.0
64.00	735.0
65.10	1029.0
66.00	119.0
67.00	382.0
68.00	16194.0
69.10	16166.0
70.00	1125.0
72.00	794.0
73.10	7069.0
74.10	27408.0
75.10	81256.0
76.10	6489.0
77.00	1271.0
78.10	805.0
79.00	4841.0
80.00	1245.0
81.00	4787.0
82.00	976.0
85.80	387.0
87.00	8192.0
88.00	8456.0
91.00	506.0
92.10	4643.0
93.00	7228.0
94.00	20032.0
95.10	177536.0
96.10	11237.0
97.10	363.0
103.90	785.0
104.90	231.0
106.00	678.0
106.90	199.0
109.90	138.0
111.80	168.0
112.90	110.0
115.00	212.0
115.90	601.0
116.90	1176.0
117.90	567.0
118.90	970.0
127.90	745.0
128.90	299.0
129.90	606.0
130.90	185.0
134.80	355.0
136.90	279.0
140.10	120.0
140.90	1696.0
141.90	246.0
143.00	1952.0
143.80	146.0
144.20	125.0
145.00	480.0
145.90	296.0
147.00	148.0
147.90	456.0
149.00	123.0
149.90	224.0
152.80	235.0
154.10	113.0
154.90	516.0
156.80	280.0
159.00	198.0
160.90	216.0
170.90	162.0
172.00	1247.0
173.00	1716.0
174.00	155584.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

175.00	11447.0
176.00	150464.0
177.00	9644.0
178.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	997.0
37.10	5240.0
38.00	4562.0
39.00	2095.0
40.10	206.0
42.90	109.0
44.00	955.0
45.00	947.0
45.90	146.0
47.00	2037.0
48.00	848.0
49.00	4857.0
50.10	23688.0
51.10	7514.0
52.10	342.0
53.00	111.0
54.90	240.0
56.00	2140.0
57.00	3415.0
58.00	205.0
60.00	1300.0
61.00	6453.0
62.10	6556.0
63.10	5271.0
64.10	633.0
65.00	917.0
66.00	118.0
67.00	339.0
68.00	14482.0
69.10	14665.0
70.00	882.0
72.00	756.0
73.10	6377.0
74.10	24640.0
75.10	73144.0
76.10	5857.0
77.00	1144.0
78.00	776.0
79.00	4360.0
79.90	1133.0
81.00	4363.0
82.00	898.0
85.80	289.0
87.00	7349.0
88.00	7601.0
91.00	481.0
92.10	4344.0
93.00	6602.0
94.00	18504.0
95.10	160640.0
96.10	10277.0
97.10	316.0
103.90	711.0
104.90	207.0
106.00	657.0
106.80	182.0
109.90	127.0
111.80	108.0
114.90	182.0
115.90	553.0
116.90	1064.0
118.00	533.0
119.00	864.0
127.90	688.0
128.90	267.0
129.80	505.0
131.00	189.0
134.80	314.0
136.90	238.0
140.10	125.0
140.90	1598.0
141.90	202.0
143.00	1745.0
143.80	103.0
144.20	105.0
145.00	487.0
145.90	294.0
146.80	118.0
147.90	403.0
149.00	130.0
149.90	214.0
152.90	165.0
153.90	111.0
154.90	517.0
156.80	261.0
159.00	198.0
160.90	223.0
171.00	142.0
172.00	1140.0
174.00	144192.0
175.00	10353.0
176.00	139008.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

177.009122.0

178.00252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213