

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011720\
 Data File : VV014327.D
 Acq On : 17 Jan 2020 10:50
 Operator : SY/MD
 Sample : L1169-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF759

Quant Time: Jan 17 23:06:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 17 22:51:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	938280	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	847461	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	382979	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	222986	3.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.00%
7) Chloroethane-d5	1.58	69	193221	3.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.20%
11) 1,1-Dichloroethene-d2	2.13	63	283004	2.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.40%#
20) 2-Butanone-d5	3.95	46	525678	33.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	66.66%
24) Chloroform-d	4.40	84	502767	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.20%
26) 1,2-Dichloroethane-d4	5.08	65	251151	3.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.00%
32) Benzene-d6	5.09	84	1070875	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
36) 1,2-Dichloropropane-d6	6.11	67	338884	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.40%
41) Toluene-d8	7.35	98	961276	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.66	79	131376	3.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.80%
46) 2-Hexanone-d5	8.13	63	573987	39.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.18%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	227366	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	306548	4.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.20%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	369121	5.409 ug/L	93
25) Chloroform	4.42	83	21271	0.180 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV011720\
Data File : VV014327.D
Acq On : 17 Jan 2020 10:50
Operator : SY/MD
Sample : L1169-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF759

Quant Time: Jan 17 23:06:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 17 22:51:36 2020
Response via : Initial Calibration




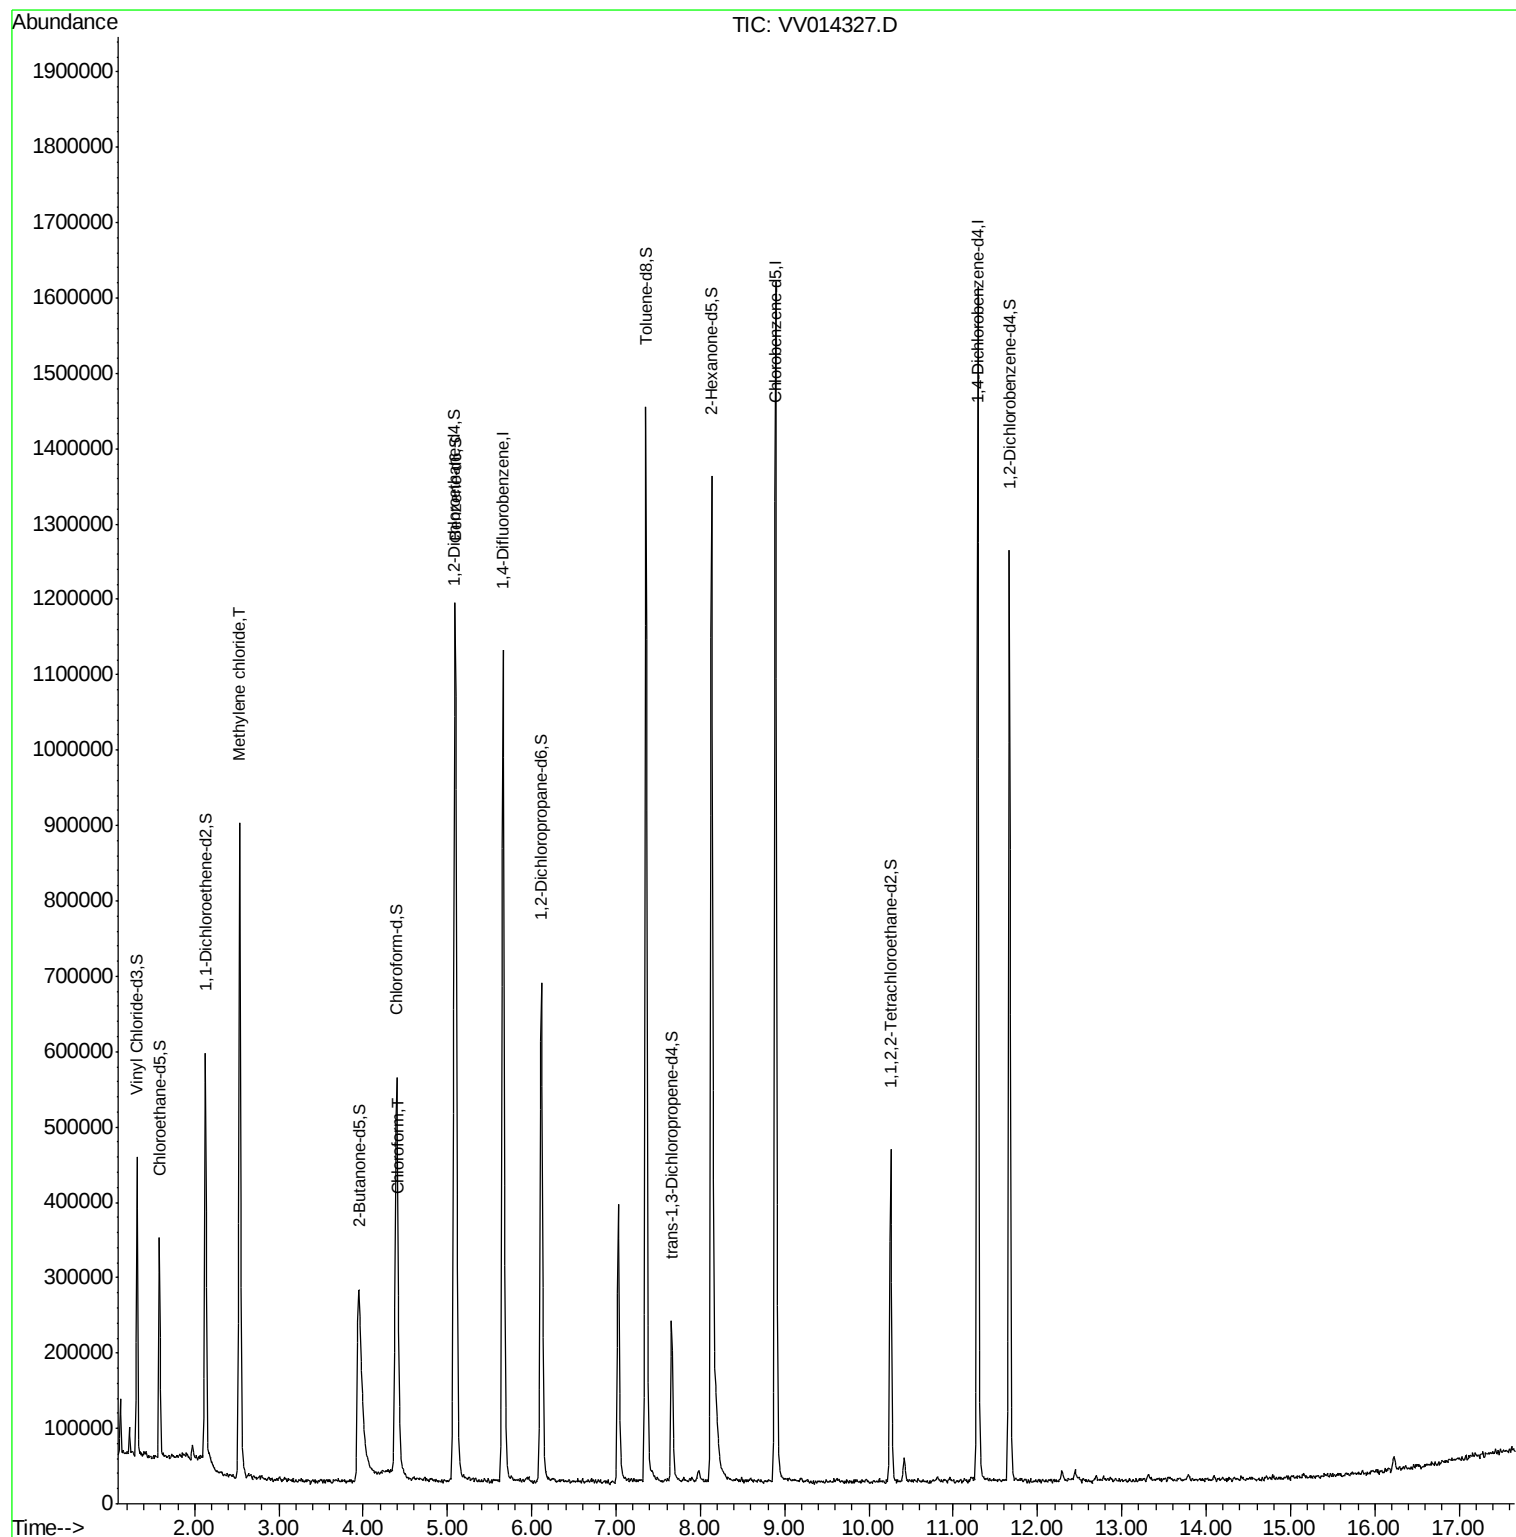


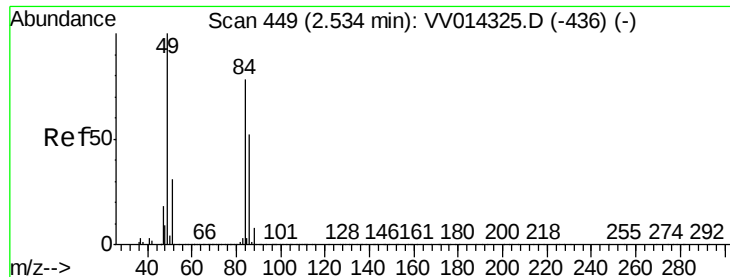

#16
Methvlene chloride
Concen: 5.409 ug/L
RT: 2.53 min Scan# 449
Delta R.T. 0.00 min
Lab File: VV014327.D
Acq: 17 Jan 2020 10:50

Instrument :
MSVOA_V
ClientSampleId :
BF759

Tot Ion: 84 Resp: 369121
Ion Ratio Lower Upper
84 100
86 62.6 43.1 80.1
49 128.1 82.1 152.5

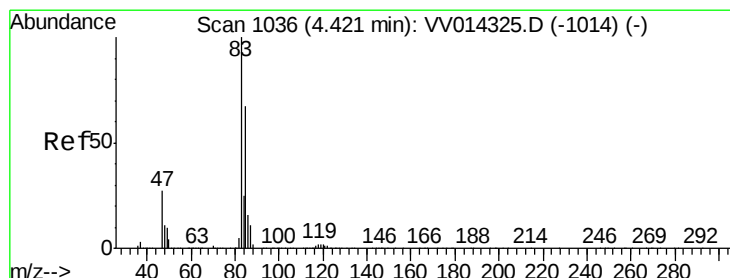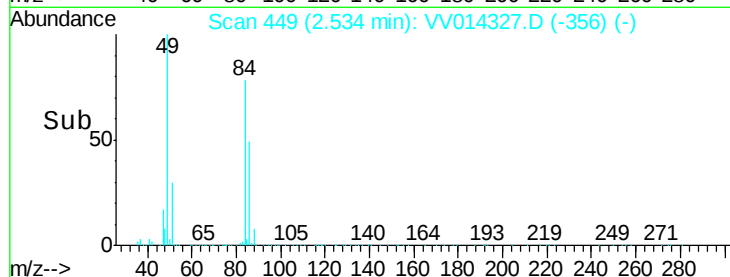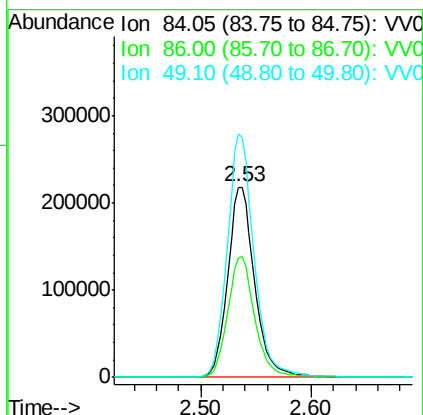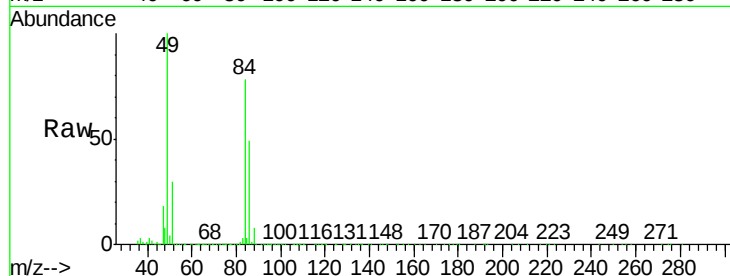

#25
Chloroform
Concen: 0.180 ug/L
RT: 4.42 min Scan# 1037
Delta R.T. 0.00 min
Lab File: VV014327.D
Acq: 17 Jan 2020 10:50

Tgt Ion: 83 Resp: 21271
Ion Ratio Lower Upper
83 100
85 74.9 46.2 85.8

