

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
 Data File : VV033723.D
 Acq On : 17 Jan 2024 16:55
 Operator : SY/MD
 Sample : P1143-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Quant Time: Jan 18 00:07:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 18 00:02:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	106901	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	100454	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	51937	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	16068	2.749	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.000%
7) Chloroethane-d5	1.536	69	17738	3.421	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.400%
11) 1,1-Dichloroethene-d2	2.060	65	8439	3.203	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.000%
20) 2-Butanone-d5	3.825	46	64447	45.091	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.180%
24) Chloroform-d	4.253	84	48910	3.869	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.400%
26) 1,2-Dichloroethane-d4	4.947	65	24314	4.290	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
32) Benzene-d6	4.963	84	88334	3.644	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.800%
36) 1,2-Dichloropropane-d6	5.992	67	29493	3.650	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	73.000%
41) Toluene-d8	7.246	98	76333	3.528	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.600%
43) trans-1,3-Dichloroprop...	7.561	79	10176	3.642	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.800%
46) 2-Hexanone-d5	8.031	63	49691	45.303	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.600%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	21173	4.484	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	32592	4.087	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	81.800%
Target Compounds						
					Qvalue	
25) Chloroform	4.281	83	9283	0.598	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
Data File : VV033723.D
Acq On : 17 Jan 2024 16:55
Operator : SY/MD
Sample : P1143-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Time: Jan 18 00:07:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 18 00:02:20 2024
Response via : Initial Calibration

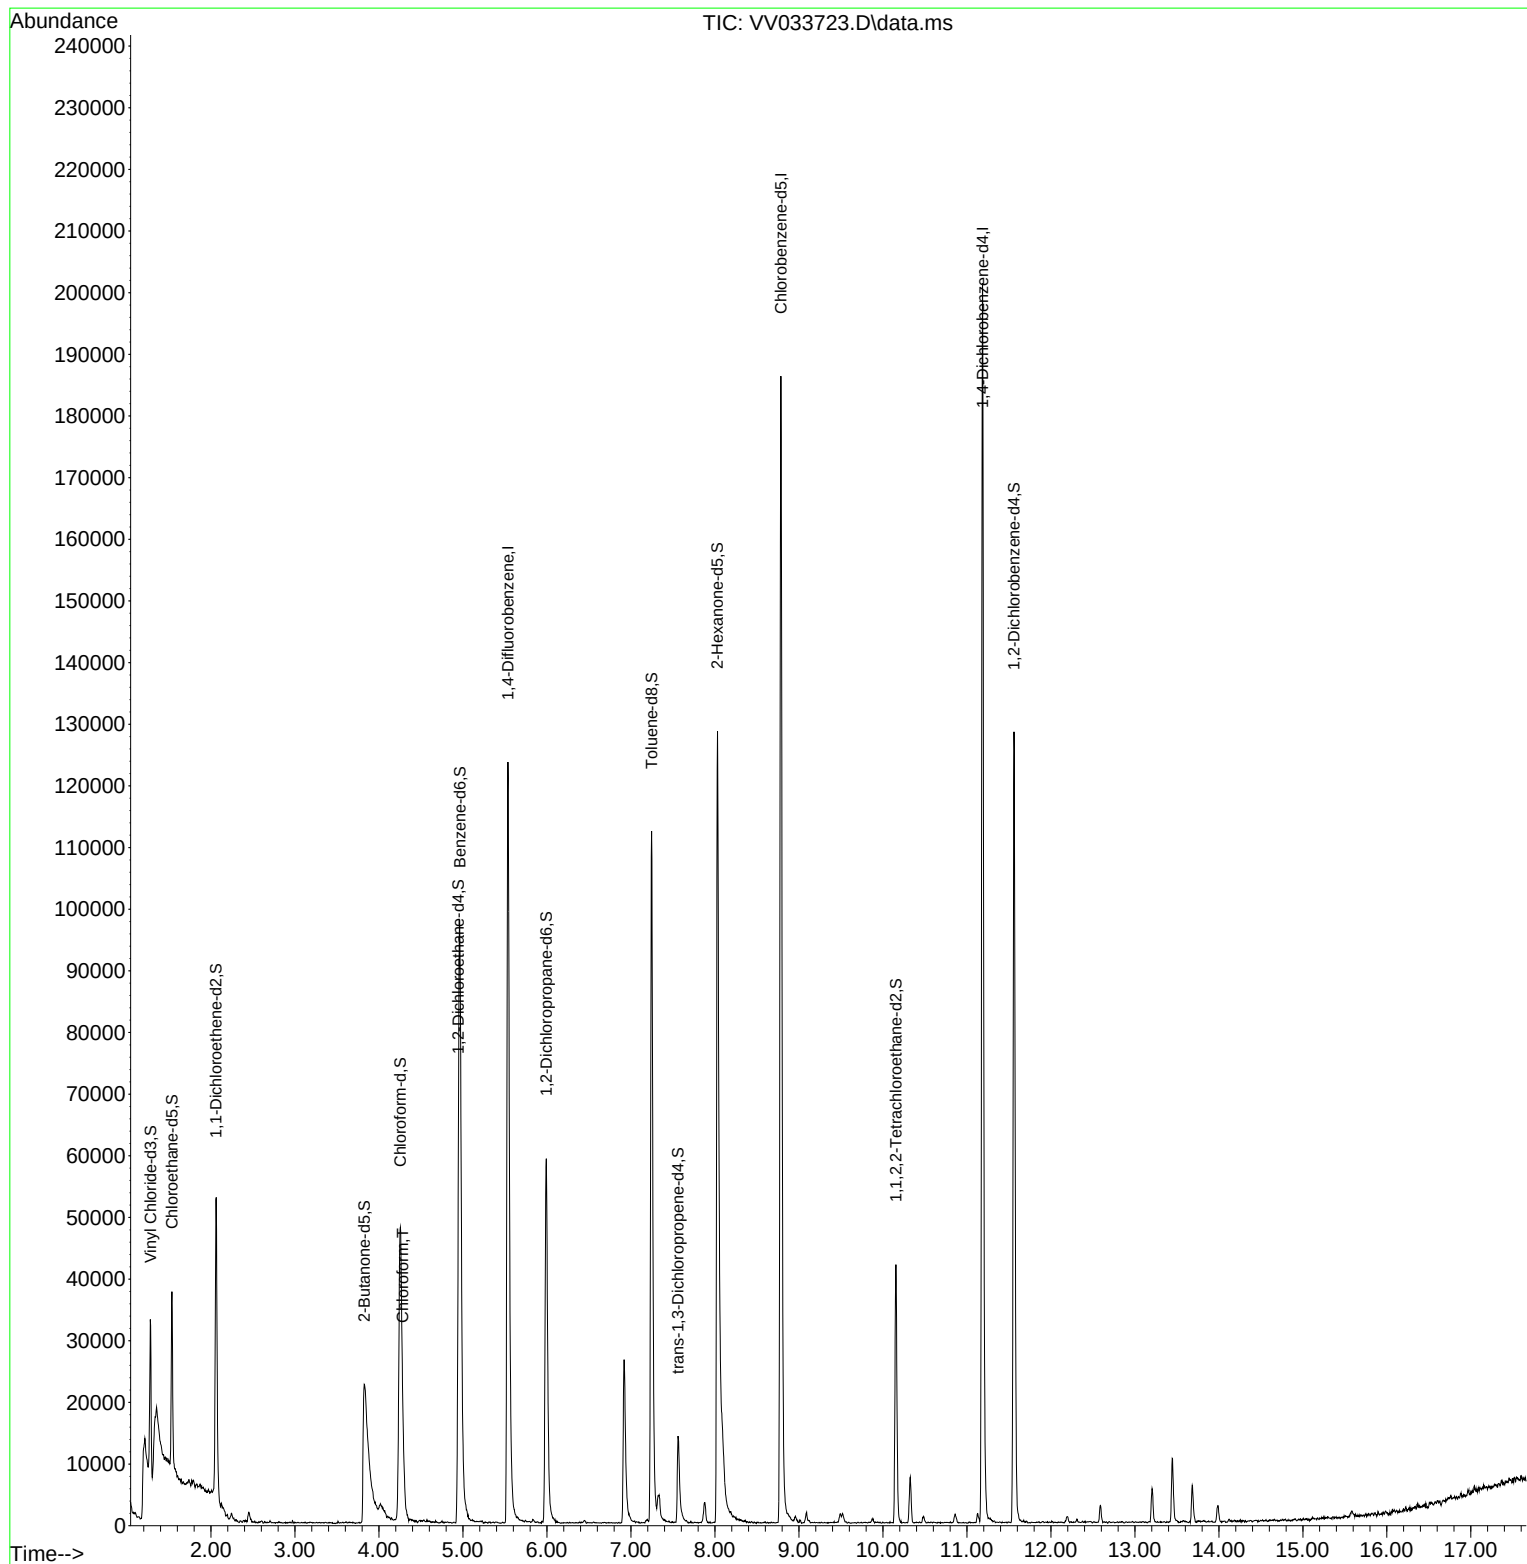

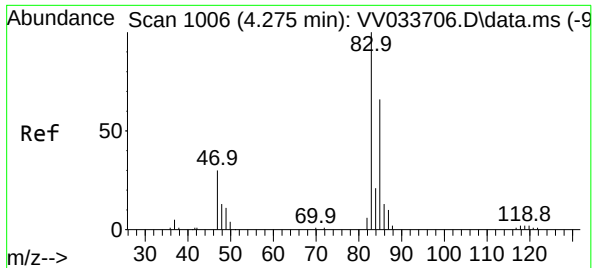

#25
 Chloroform
 Concen: 0.598 ug/L
 RT: 4.281 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV033723.D
 Acq: 17 Jan 2024 16:55

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Tgt Ion: 83 Resp: 9283
 Ion Ratio Lower Upper
 83 100
 85 65.7 45.1 83.9

