

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
 Data File : VV033710.D
 Acq On : 17 Jan 2024 11:24
 Operator : SY/MD
 Sample : P1131-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	65	75	89	rBV	29796	33562	10.39%	1.298%
2	1.535	147	154	165	rVB	30944	34974	10.83%	1.352%
3	2.063	308	318	330	rVB	54306	79882	24.74%	3.089%
4	3.815	854	863	894	rBV2	24848	90963	28.17%	3.518%
5	4.252	983	999	1027	rBV2	48968	127314	39.42%	4.923%
6	4.960	1205	1219	1248	rBV2	107095	272830	84.49%	10.551%
7	5.535	1388	1398	1421	rBV	126394	260703	80.73%	10.082%
8	5.989	1528	1539	1569	rBV2	62782	135985	42.11%	5.259%
9	6.918	1818	1828	1855	rBV	29238	58794	18.21%	2.274%
10	7.246	1920	1930	1954	rBV	124921	226986	70.29%	8.778%
11	7.561	2020	2028	2061	rBV	15811	31532	9.76%	1.219%
12	7.876	2114	2126	2139	rBV2	5065	9099	2.82%	0.352%
13	8.030	2165	2174	2209	rBV	121920	273948	84.83%	10.594%
14	8.786	2399	2409	2435	rBV	186931	317521	98.32%	12.279%
15	10.156	2824	2835	2850	rBV	40964	66727	20.66%	2.580%
16	10.326	2877	2888	2899	rBV2	11703	18253	5.65%	0.706%
17	11.185	3145	3155	3179	rBV	202001	322931	100.00%	12.488%
18	11.561	3261	3272	3293	rBV	133292	213423	66.09%	8.253%
19	12.194	3462	3469	3479	rVB2	3557	5319	1.65%	0.206%
20	13.985	4018	4026	4037	rVB	3347	5158	1.60%	0.199%




Sum of corrected areas: 2585904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
Data File : VV033710.D
Acq On : 17 Jan 2024 11:24
Operator : SY/MD
Sample : P1131-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

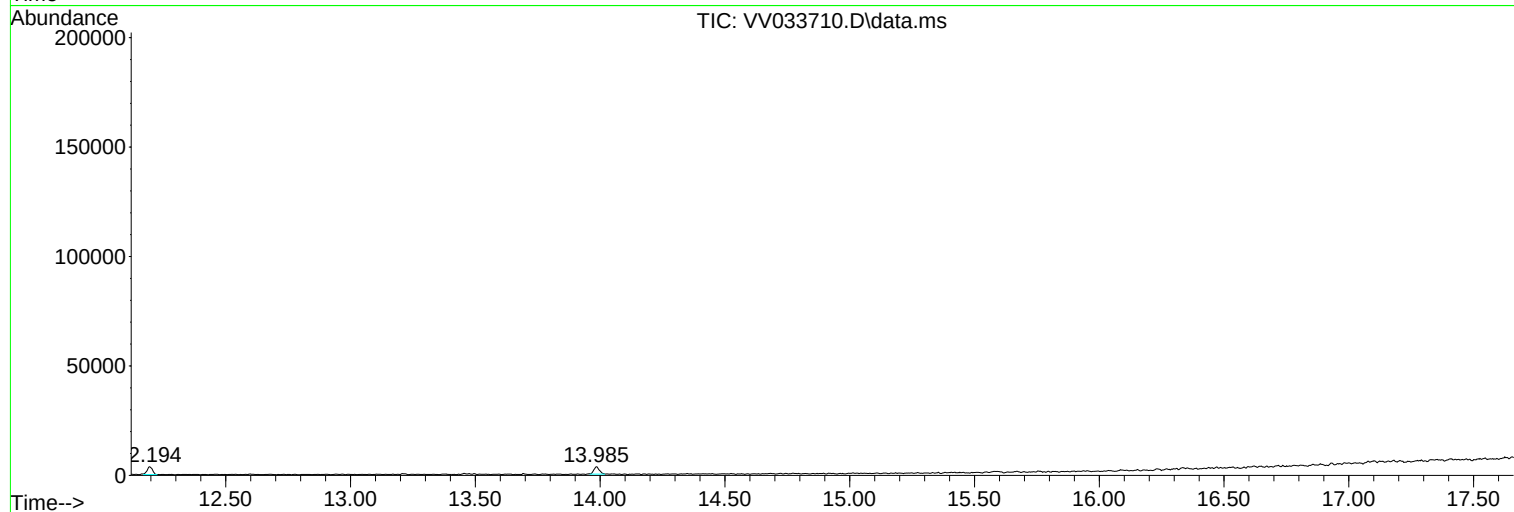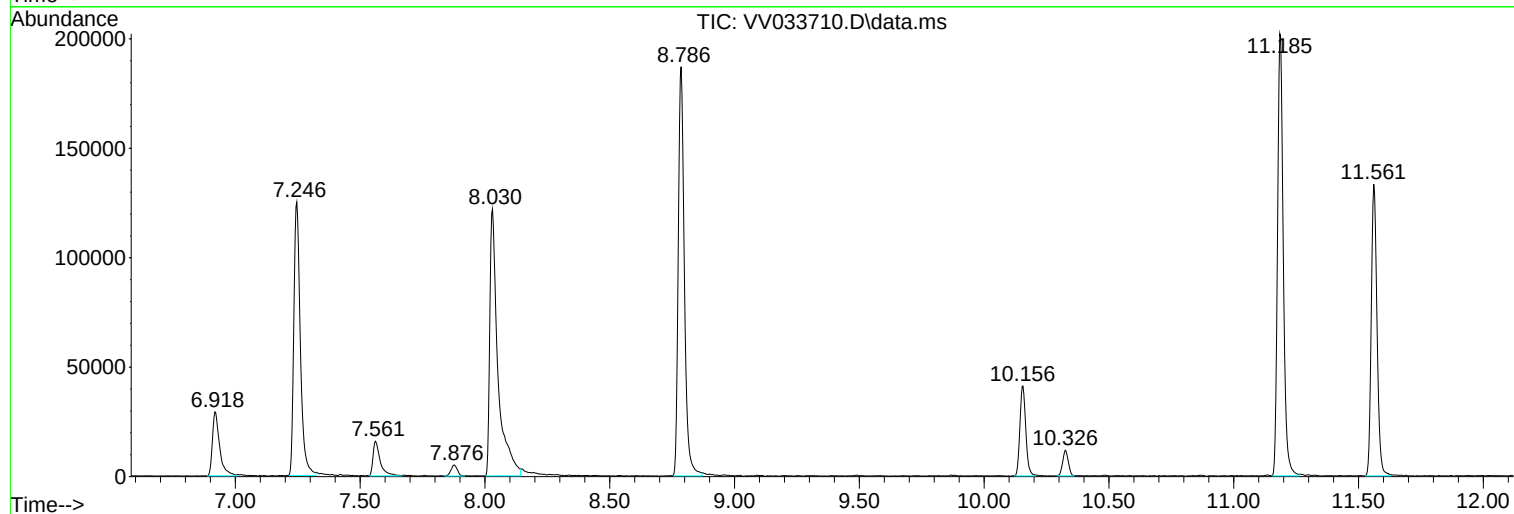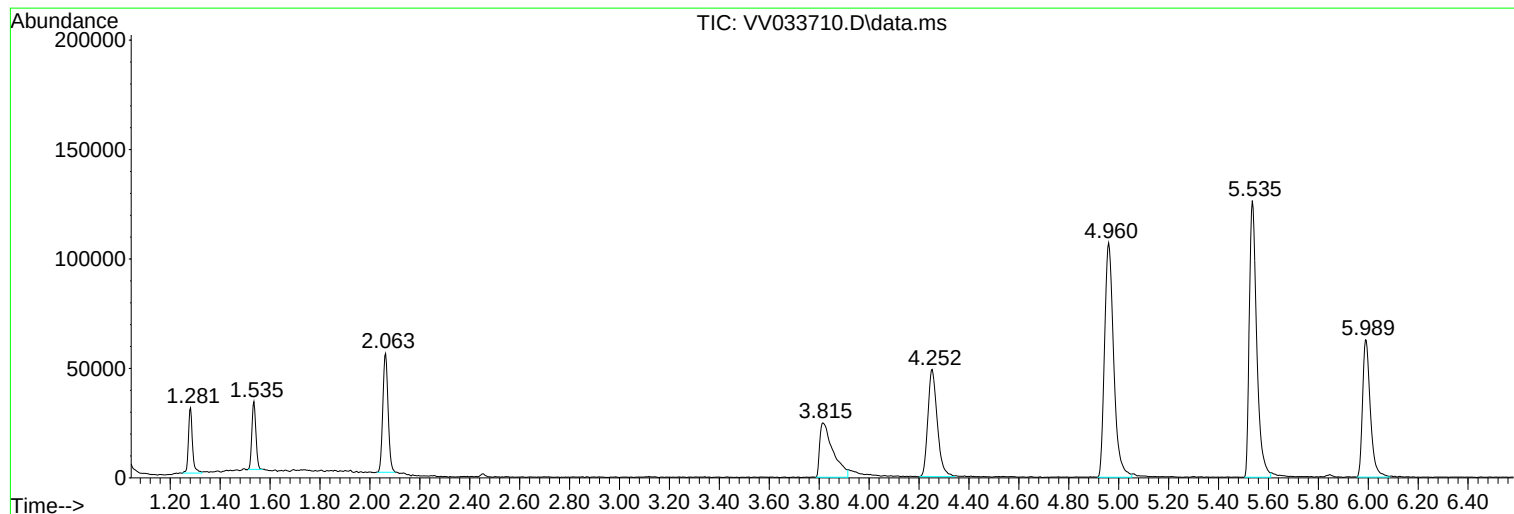

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
Data File : VV033710.D
Acq On : 17 Jan 2024 11:24
Operator : SY/MD
Sample : P1131-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
Data File : VV033710.D
Acq On : 17 Jan 2024 11:24
Operator : SY/MD
Sample : P1131-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc