
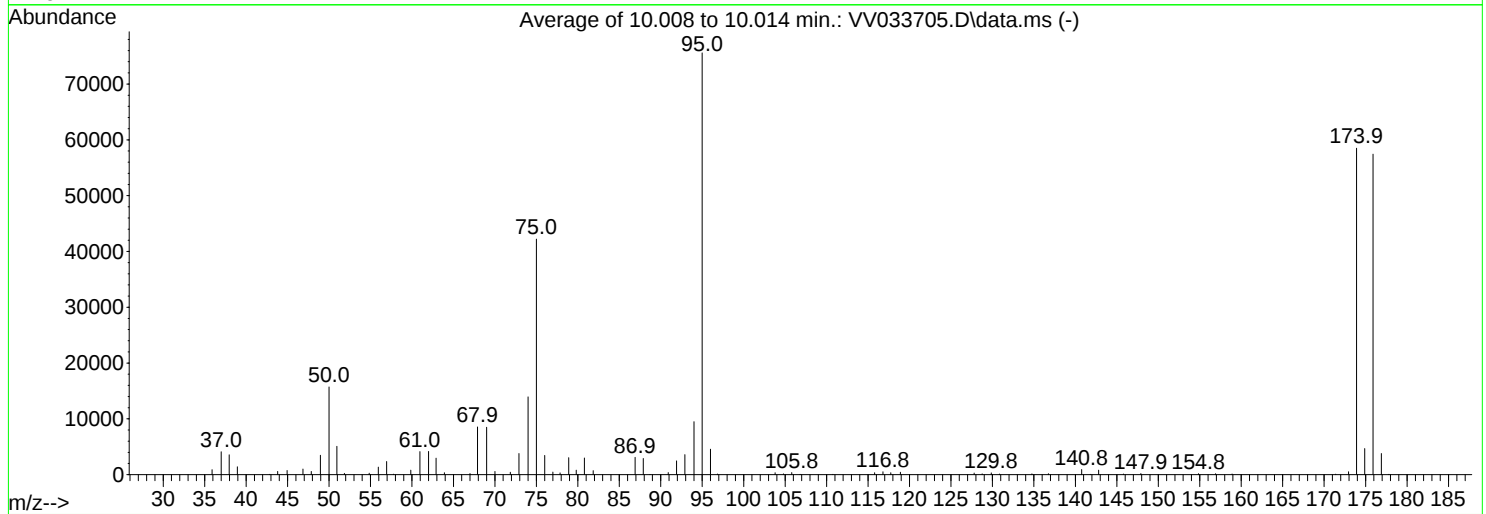


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011724\
Data File : VV033705.D
Acq On : 17 Jan 2024 08:40
Operator : SY/MD
Sample : BFB240
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB240

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 18 00:02:20 2024

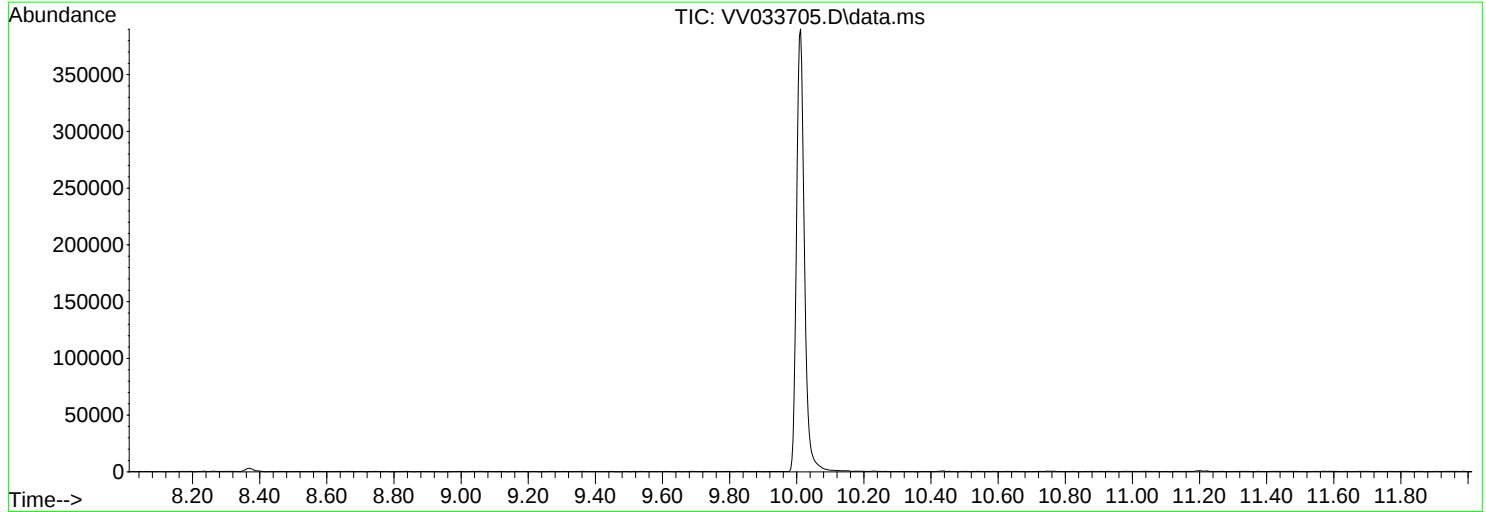

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	15724	PASS
75	95	30	80	55.9	42221	PASS
95	95	100	100	100.0	75595	PASS
96	95	5	9	6.0	4554	PASS
173	174	0.00	2	0.9	524	PASS
174	95	50	120	77.4	58488	PASS
175	174	5	9	8.0	4664	PASS
176	174	95	105	98.2	57427	PASS
177	176	5	10	6.6	3776	PASS

m/z	Abundance
39.90	153.0
43.80	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	938.0
37.00	4168.0
37.90	3621.0
39.00	1383.0
39.90	115.0
42.90	102.0
43.90	769.0
45.00	760.0
46.90	1164.0
47.90	627.0
48.90	3516.0
50.00	16193.0
50.90	5227.0
51.80	252.0
54.80	273.0
56.00	1382.0
56.90	2474.0
57.80	123.0
59.90	885.0
60.90	4254.0
62.00	4234.0
62.90	3026.0
63.90	364.0
66.90	172.0
67.90	8862.0
69.00	8750.0
70.00	627.0
71.90	490.0
72.90	3898.0
74.00	14277.0
75.00	43240.0
76.00	3537.0
77.00	511.0
77.80	366.0
78.90	3084.0
79.80	835.0
80.80	3063.0
81.90	743.0
86.90	3200.0
87.90	2922.0
90.90	344.0
91.90	2556.0
92.90	3594.0
94.00	9543.0
95.00	77552.0
96.00	4751.0
96.90	118.0
103.80	341.0
104.80	153.0
105.80	399.0
106.80	111.0
115.80	304.0
116.80	524.0
117.70	338.0
118.90	443.0
127.80	289.0
128.80	154.0
129.80	301.0
130.80	117.0
134.70	168.0
136.80	169.0
140.80	996.0
141.80	110.0
142.80	819.0
145.80	103.0
147.90	195.0
154.80	138.0
156.90	163.0
158.80	107.0
173.00	790.0
173.90	58288.0
174.90	4577.0
175.90	57232.0
176.90	3752.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	943.0
37.00	4227.0
37.90	3658.0
39.00	1430.0
39.90	133.0
42.80	103.0
43.90	760.0
45.00	793.0
46.90	1021.0
47.90	581.0
48.90	3570.0
50.00	16205.0
51.00	5201.0
51.90	237.0
54.90	273.0
56.00	1390.0
57.00	2418.0
57.80	123.0
59.80	803.0
61.00	4237.0
62.00	4304.0
62.90	3071.0
63.90	357.0
67.00	198.0
67.90	8839.0
69.00	8755.0
70.00	582.0
71.80	461.0
72.90	3947.0
74.00	14343.0
75.00	43384.0
76.00	3532.0
77.00	486.0
77.90	325.0
78.90	3170.0
79.80	817.0
80.80	3098.0
81.80	730.0
86.90	3194.0
87.90	2915.0
88.70	128.0
90.90	386.0
91.90	2555.0
92.90	3720.0
94.00	9756.0
95.00	77904.0
96.00	4634.0
96.80	135.0
103.80	348.0
104.80	162.0
105.80	400.0
106.80	112.0
110.80	102.0
115.80	349.0
116.80	522.0
117.70	361.0
118.90	446.0
127.80	300.0
128.70	131.0
129.90	319.0
130.90	124.0
134.70	155.0
136.70	182.0
140.80	966.0
141.80	107.0
142.80	826.0
145.80	123.0
147.90	225.0
154.90	172.0
156.90	165.0
158.90	108.0
171.40	121.0
172.90	781.0
173.90	60528.0
174.90	4867.0
175.90	59400.0
176.90	3893.0
177.80	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	799.0
37.00	3925.0
38.00	3387.0
38.90	1389.0
39.80	139.0
43.80	703.0
44.90	732.0
46.80	844.0
47.80	526.0
49.00	3343.0
50.00	14775.0
51.00	4776.0
51.90	208.0
54.90	245.0
55.90	1310.0
57.00	2130.0
59.80	699.0
61.00	3863.0
62.00	3969.0
62.90	2802.0
63.90	313.0
67.10	212.0
67.90	7952.0
69.00	7928.0
70.00	532.0
71.80	383.0
72.90	3552.0
74.00	13195.0
75.00	40040.0
76.00	3226.0
77.00	417.0
77.90	272.0
78.90	2897.0
79.80	739.0
80.80	2808.0
81.80	660.0
86.90	2874.0
87.90	2875.0
90.90	412.0
91.90	2305.0
92.90	3461.0
94.00	9204.0
95.00	71328.0
96.00	4277.0
96.80	138.0
103.80	347.0
104.80	154.0
105.80	370.0
110.70	120.0
115.80	370.0
116.80	477.0
117.80	328.0
118.90	426.0
127.80	268.0
128.70	111.0
129.90	316.0
130.90	120.0
134.80	139.0
136.70	178.0
140.70	838.0
142.80	786.0
145.80	124.0
147.90	206.0
154.90	202.0
156.90	152.0
159.00	118.0
171.40	122.0
173.90	56648.0
174.90	4548.0
175.90	55648.0
176.90	3683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240