
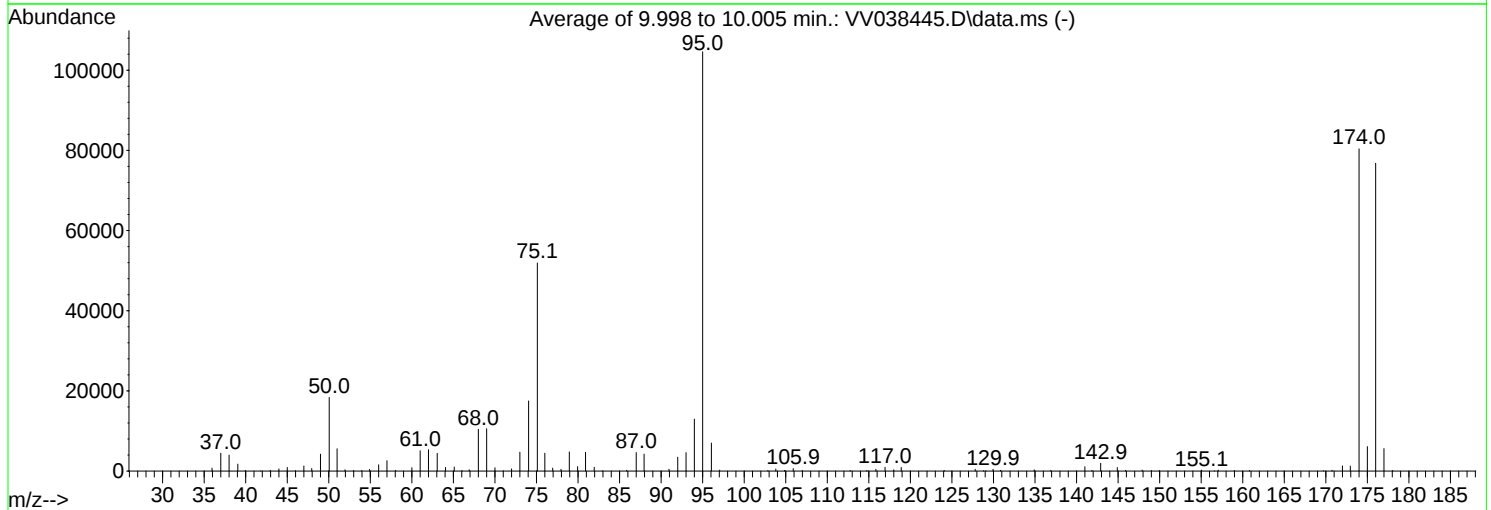


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV011725\
Data File : VV038445.D
Acq On : 17 Jan 2025 08:56
Operator : SY/MD
Sample : BFB298
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB298

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jan 18 02:24:22 2025

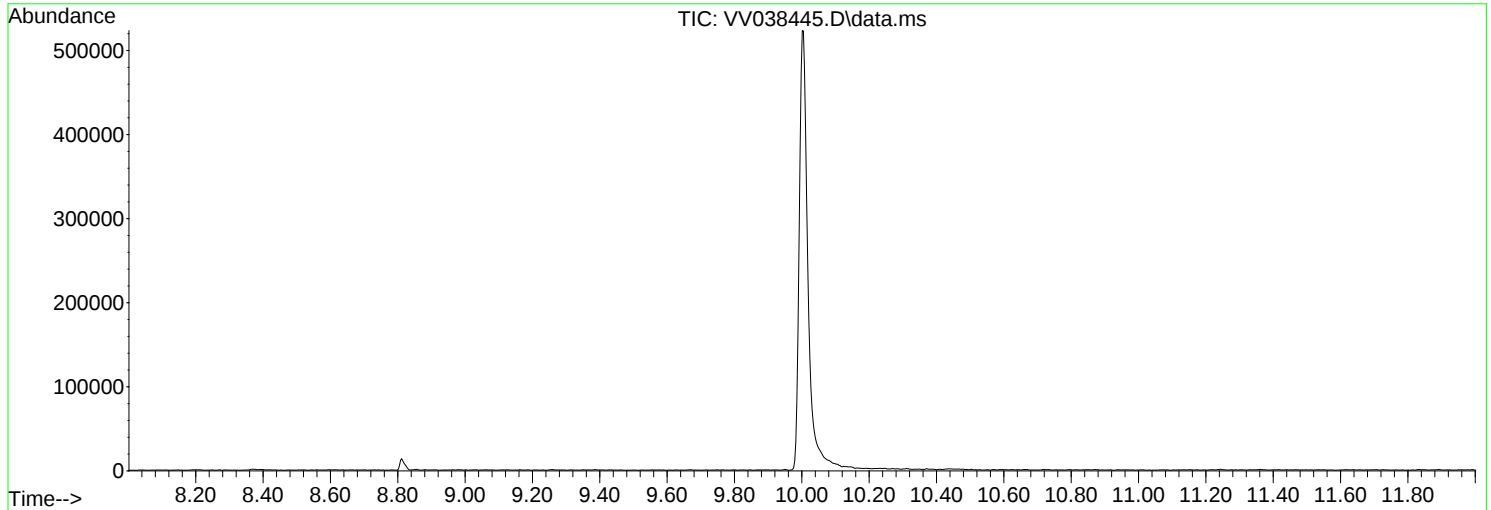

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	18365	PASS
75	95	30	80	49.6	51917	PASS
95	95	100	100	100.0	104616	PASS
96	95	5	9	6.7	6995	PASS
173	174	0.00	2	1.5	1244	PASS
174	95	50	120	76.8	80395	PASS
175	174	5	9	7.6	6114	PASS
176	174	95	105	95.5	76803	PASS
177	176	5	10	7.3	5618	PASS

m/z	Abundance
39.90	388.0
44.00	420.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
36.00	742.0
37.00	4262.0
38.00	3898.0
39.10	1655.0
40.10	574.0
42.90	170.0
44.00	996.0
45.00	798.0
47.00	1176.0
47.90	653.0
49.00	3982.0
50.10	17472.0
51.00	5328.0
52.00	380.0
53.00	148.0
54.90	415.0
56.00	1255.0
57.00	2425.0
58.10	158.0
60.00	799.0
61.00	4816.0
62.00	4718.0
63.00	4287.0
64.10	849.0
65.10	915.0
66.90	368.0
68.00	9765.0
69.00	9849.0
70.00	807.0
71.00	108.0
72.00	479.0
73.00	4401.0
74.10	16357.0
75.10	50248.0
76.00	4364.0
77.00	777.0
77.90	412.0
79.00	4557.0
79.90	1026.0
80.90	4437.0
81.90	905.0
85.90	206.0
87.00	4330.0
87.90	4045.0
91.00	461.0
92.00	3130.0
93.00	4269.0
94.00	11921.0
95.00	99200.0
96.00	6788.0
97.10	183.0
102.80	159.0
103.80	467.0
104.80	150.0
105.90	609.0
107.00	125.0
112.70	119.0
114.70	154.0
116.00	373.0
116.90	876.0
117.90	313.0
118.90	879.0
127.80	350.0
129.10	138.0
129.90	388.0
130.90	212.0
134.90	280.0
136.90	164.0
141.00	965.0
141.80	131.0
142.90	1821.0
144.90	757.0
145.90	119.0
147.90	300.0
149.00	123.0
149.90	124.0
155.00	187.0
157.10	221.0
159.00	138.0
160.70	146.0
169.70	113.0
170.80	183.0
172.00	1070.0
172.90	1105.0
174.00	73696.0
175.00	5565.0
176.00	70408.0
177.00	5193.0
178.10	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
35.90	778.0
37.00	4589.0
38.00	4061.0
39.10	1759.0
40.00	551.0
42.90	201.0
44.00	967.0
45.00	964.0
47.00	1271.0
48.00	693.0
49.00	4356.0
50.10	18920.0
51.00	5733.0
51.90	330.0
53.00	158.0
53.90	119.0
54.90	432.0
56.00	1661.0
57.00	2659.0
58.10	186.0
60.00	834.0
61.00	5307.0
62.00	5582.0
63.10	4584.0
64.10	913.0
65.10	1071.0
66.00	122.0
66.90	354.0
68.00	10781.0
69.00	10891.0
70.00	848.0
72.00	552.0
73.00	4898.0
74.10	18088.0
75.10	53640.0
76.00	4547.0
77.00	759.0
78.00	429.0
78.90	4942.0
80.00	1135.0
80.90	4890.0
81.90	954.0
85.90	188.0
87.00	4785.0
87.90	4356.0
90.90	486.0
92.00	3632.0
93.00	4817.0
94.00	13432.0
95.00	108216.0
96.10	7201.0
97.10	253.0
102.90	144.0
103.80	521.0
104.90	160.0
105.90	652.0
107.00	111.0
112.70	158.0
114.80	155.0
115.80	449.0
116.90	980.0
118.00	328.0
118.90	969.0
124.10	145.0
127.80	465.0
128.80	159.0
130.00	466.0
130.90	175.0
134.90	333.0
136.90	162.0
141.00	1126.0
141.80	161.0
142.90	2081.0
144.90	953.0
145.90	161.0
147.90	277.0
149.00	134.0
150.00	150.0
155.10	255.0
156.60	158.0
157.10	240.0
159.00	136.0
160.80	162.0
169.70	118.0
170.80	221.0
172.00	1300.0
173.00	1268.0
174.00	83016.0
175.00	6334.0
176.00	79032.0
177.00	5832.0
178.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

m/z	Abundance
35.90	718.0
37.00	4560.0
38.00	4007.0
39.00	1804.0
39.90	489.0
41.80	122.0
43.00	174.0
44.00	906.0
45.00	966.0
46.00	247.0
47.00	1379.0
47.90	608.0
49.00	4353.0
50.00	18704.0
51.00	5654.0
51.90	287.0
53.00	177.0
54.00	120.0
54.90	358.0
56.00	1785.0
57.00	2687.0
58.00	204.0
60.00	932.0
61.00	5107.0
62.00	5699.0
63.00	4414.0
64.00	940.0
65.10	1093.0
66.10	123.0
66.90	299.0
68.00	10733.0
69.00	10995.0
70.00	857.0
72.00	593.0
73.00	4873.0
74.00	18056.0
75.10	51864.0
76.00	4494.0
76.90	712.0
78.00	504.0
78.90	4841.0
80.00	1183.0
80.90	4772.0
82.00	1018.0
82.90	120.0
85.80	161.0
87.00	4745.0
88.00	4305.0
90.90	480.0
92.00	3614.0
93.00	4714.0
94.00	13548.0
95.00	106432.0
96.00	6997.0
97.00	289.0
102.90	131.0
103.80	565.0
104.90	183.0
105.90	612.0
107.00	106.0
112.80	156.0
114.80	116.0
115.80	525.0
117.00	1028.0
118.10	351.0
118.90	933.0
124.10	167.0
127.80	511.0
128.80	176.0
130.00	510.0
130.80	154.0
134.90	358.0
136.90	147.0
141.00	1190.0
141.90	166.0
142.90	1950.0
144.90	965.0
145.90	168.0
148.00	190.0
149.00	139.0
150.00	130.0
155.10	319.0
157.00	247.0
159.00	147.0
160.90	151.0
170.70	247.0
172.00	1464.0
173.00	1359.0
174.00	84472.0
175.00	6444.0
176.00	80968.0
177.00	5829.0

Instrument :
MSVOA_V
ClientSampleId :
BFB298

178.00

161.0

Instrument :

MSVOA_V

ClientSampleId :

BFB298