


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV011819\
 Data File : VV009220.D
 Acq On : 18 Jan 2019 12:46
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00 G/5ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\82V011819S.M
 Title : SW846 8260
 Last Update : Sat Jan 19 03:39:51 2019

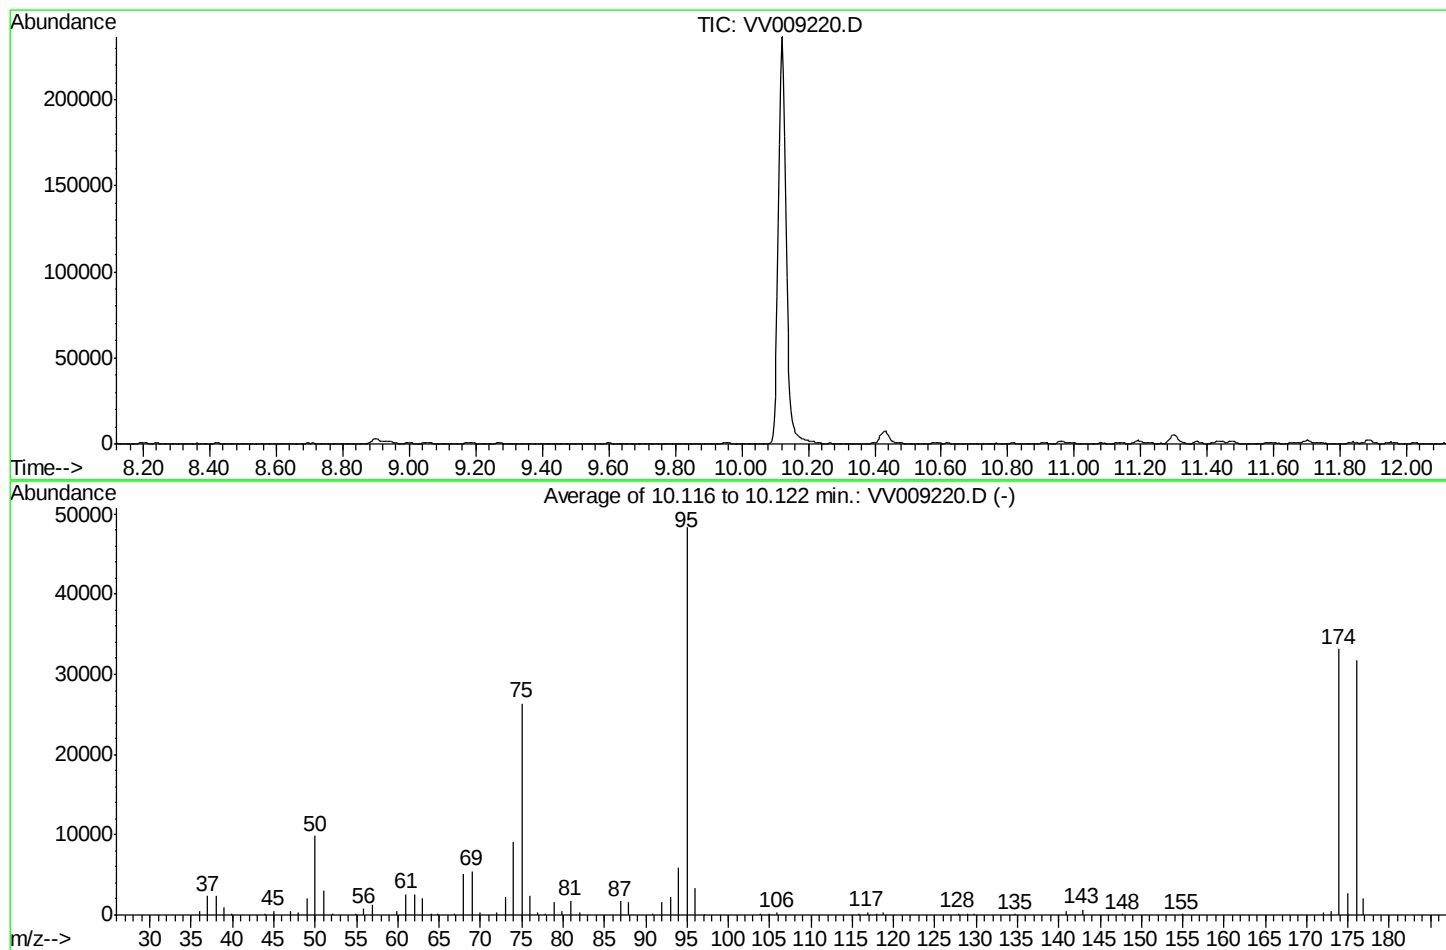

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	9892	PASS
75	95	30	60	54.5	26357	PASS
95	95	100	100	100.0	48328	PASS
96	95	5	9	7.0	3385	PASS
173	174	0.00	2	1.4	456	PASS
174	95	50	100	68.6	33173	PASS
175	174	5	9	8.2	2706	PASS
176	174	95	101	95.7	31736	PASS
177	176	5	9	6.6	2093	PASS