

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020036.D
 Acq On : 18 Jan 2021 11:47
 Operator : SY/MD
 Sample : VV0118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	255970	264256	15.65%	1.983%
2	1.569	142	149	159	rBV	221320	248202	14.70%	1.863%
3	2.110	307	317	350	rVB	486832	742278	43.97%	5.570%
4	2.601	468	470	471	rBV	642	246	0.01%	0.002%
5	2.994	584	592	595	rBV4	1424	1330	0.08%	0.010%
6	3.036	602	605	608	rBV4	815	791	0.05%	0.006%
7	3.100	621	625	627	rBV5	618	454	0.03%	0.003%
8	3.158	641	643	645	rBV2	542	293	0.02%	0.002%
9	3.219	661	662	664	rVB3	719	208	0.01%	0.002%
10	3.245	667	670	674	rVB4	566	426	0.03%	0.003%
11	3.264	674	676	678	rBV2	491	262	0.02%	0.002%
12	3.367	705	708	709	rBV2	373	194	0.01%	0.001%
13	3.425	724	726	727	rBV2	507	265	0.02%	0.002%
14	3.476	738	742	745	rBV2	832	542	0.03%	0.004%
15	3.511	751	753	756	rBV2	513	288	0.02%	0.002%
16	3.601	779	781	784	rVB4	466	293	0.02%	0.002%
17	3.621	785	787	791	rVV3	448	326	0.02%	0.002%
18	3.663	796	800	802	rBV2	248	184	0.01%	0.001%
19	3.724	811	819	820	rBV4	710	703	0.04%	0.005%
20	3.756	826	829	831	rBV2	367	254	0.02%	0.002%
21	3.769	831	833	834	rBV	714	248	0.01%	0.002%
22	3.817	847	848	854	rVB2	464	320	0.02%	0.002%
23	3.855	854	860	862	rBV5	766	853	0.05%	0.006%
24	3.900	862	874	913	rBV	110194	373308	22.11%	2.802%
25	4.354	1000	1015	1041	rBV2	274386	674230	39.94%	5.060%
26	4.708	1123	1125	1130	rVB3	1127	693	0.04%	0.005%
27	4.830	1161	1163	1167	rVB3	1013	588	0.03%	0.004%
28	4.862	1171	1173	1177	rVV2	1024	628	0.04%	0.005%
29	4.881	1177	1179	1181	rVB2	342	155	0.01%	0.001%
30	5.052	1215	1232	1265	rBV2	659950	1688189	100.00%	12.669%
31	5.460	1358	1359	1362	rBV3	501	190	0.01%	0.001%
32	5.505	1371	1373	1379	rVV5	682	462	0.03%	0.003%
33	5.531	1379	1381	1384	rVB2	578	265	0.02%	0.002%
34	5.572	1393	1394	1395	rBV2	539	198	0.01%	0.001%
35	5.621	1397	1409	1436	rVV	486755	971936	57.57%	7.294%
36	5.910	1488	1499	1514	rBV3	31909	65573	3.88%	0.492%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020036.D
 Acq On : 18 Jan 2021 11:47
 Operator : SY/MD
 Sample : VV0118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.016	1529	1532	1535	rBV4	735	543	0.03%	0.004%
38	6.074	1535	1550	1580	rVV	378869	771845	45.72%	5.792%
39	6.463	1669	1671	1674	rBV4	535	210	0.01%	0.002%
40	6.518	1684	1688	1690	rBV2	576	444	0.03%	0.003%
41	6.569	1702	1704	1705	rBV2	701	184	0.01%	0.001%
42	6.630	1719	1723	1724	rBV3	619	466	0.03%	0.003%
43	6.817	1777	1781	1783	rBV3	441	328	0.02%	0.002%
44	6.926	1812	1815	1818	rBV3	781	572	0.03%	0.004%
45	6.990	1824	1835	1855	rBV	207816	373649	22.13%	2.804%
46	7.322	1925	1938	1960	rBV	754755	1320861	78.24%	9.912%
47	7.624	2022	2032	2053	rBV2	143774	254072	15.05%	1.907%
48	7.823	2092	2094	2096	rBV3	577	281	0.02%	0.002%
49	8.029	2155	2158	2160	rBV3	359	245	0.01%	0.002%
50	8.045	2160	2163	2167	rVB2	1016	773	0.05%	0.006%
51	8.093	2167	2178	2213	rBV2	397485	798015	47.27%	5.989%
52	8.733	2375	2377	2381	rVB3	1045	442	0.03%	0.003%
53	8.858	2403	2416	2435	rBV	754486	1221586	72.36%	9.167%
54	9.077	2481	2484	2487	rBV3	796	722	0.04%	0.005%
55	9.116	2494	2496	2497	rBV2	596	224	0.01%	0.002%
56	9.219	2526	2528	2531	rBV3	595	392	0.02%	0.003%
57	9.276	2544	2546	2548	rVB4	668	296	0.02%	0.002%
58	9.296	2550	2552	2555	rBV2	746	445	0.03%	0.003%
59	9.328	2560	2562	2564	rBV2	482	285	0.02%	0.002%
60	9.460	2600	2603	2606	rVB2	517	308	0.02%	0.002%
61	9.489	2608	2612	2614	rBV3	347	232	0.01%	0.002%
62	9.508	2616	2618	2622	rBV3	335	215	0.01%	0.002%
63	9.550	2628	2631	2632	rBV2	438	233	0.01%	0.002%
64	9.762	2694	2697	2698	rBV2	439	221	0.01%	0.002%
65	9.772	2698	2700	2702	rBV2	342	193	0.01%	0.001%
66	9.900	2734	2740	2743	rBV3	442	395	0.02%	0.003%
67	9.916	2743	2745	2746	rBV2	432	201	0.01%	0.002%
68	10.051	2783	2787	2790	rBV2	654	376	0.02%	0.003%
69	10.180	2823	2827	2828	rBV2	306	217	0.01%	0.002%
70	10.222	2828	2840	2863	rVV	545459	851478	50.44%	6.390%
71	10.325	2870	2872	2873	rBV2	438	156	0.01%	0.001%
72	10.495	2922	2925	2931	rBV2	473	454	0.03%	0.003%
73	10.543	2935	2940	2943	rBV3	666	746	0.04%	0.006%
74	10.653	2969	2974	2975	rBV2	667	500	0.03%	0.004%
75	10.788	3012	3016	3018	rBV	402	325	0.02%	0.002%
76	10.858	3034	3038	3039	rBV2	338	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020036.D
 Acq On : 18 Jan 2021 11:47
 Operator : SY/MD
 Sample : VV0118WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.923	3056	3058	3062	rBV3	782	647	0.04%	0.005%
78	11.016	3080	3087	3089	rBV4	612	659	0.04%	0.005%
79	11.093	3108	3111	3113	rBV	426	233	0.01%	0.002%
80	11.170	3133	3135	3137	rBV	531	282	0.02%	0.002%
81	11.186	3137	3140	3141	rBV	1091	626	0.04%	0.005%
82	11.254	3149	3161	3190	rBV	915112	1425034	84.41%	10.694%
83	11.563	3254	3257	3260	rBV3	935	582	0.03%	0.004%
84	11.630	3265	3278	3299	rBV	782571	1238629	73.37%	9.295%
85	11.977	3383	3386	3387	rBV2	444	279	0.02%	0.002%
86	12.000	3392	3393	3396	rVB	454	177	0.01%	0.001%
87	12.042	3403	3406	3408	rBV2	842	572	0.03%	0.004%
88	12.077	3415	3417	3418	rBV	521	251	0.01%	0.002%
89	12.653	3593	3596	3598	rBV4	1795	1239	0.07%	0.009%
90	12.723	3616	3618	3621	rBV	702	275	0.02%	0.002%
91	12.797	3637	3641	3647	rBV5	827	845	0.05%	0.006%
92	12.833	3650	3652	3655	rBV2	494	259	0.02%	0.002%
93	12.968	3692	3694	3700	rBV5	699	512	0.03%	0.004%
94	13.009	3705	3707	3710	rBV	530	281	0.02%	0.002%
95	13.273	3784	3789	3797	rBB7	2693	3598	0.21%	0.027%
96	13.521	3858	3866	3875	rBV5	2547	4988	0.30%	0.037%
97	13.704	3920	3923	3926	rBV5	816	649	0.04%	0.005%
98	13.849	3966	3968	3974	rBV5	806	742	0.04%	0.006%
99	14.160	4061	4065	4068	rBV4	538	517	0.03%	0.004%
100	14.270	4097	4099	4102	rBV3	627	423	0.03%	0.003%


Sum of corrected areas: 13325277

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020036.D
Acq On : 18 Jan 2021 11:47
Operator : SY/MD
Sample : VV0118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

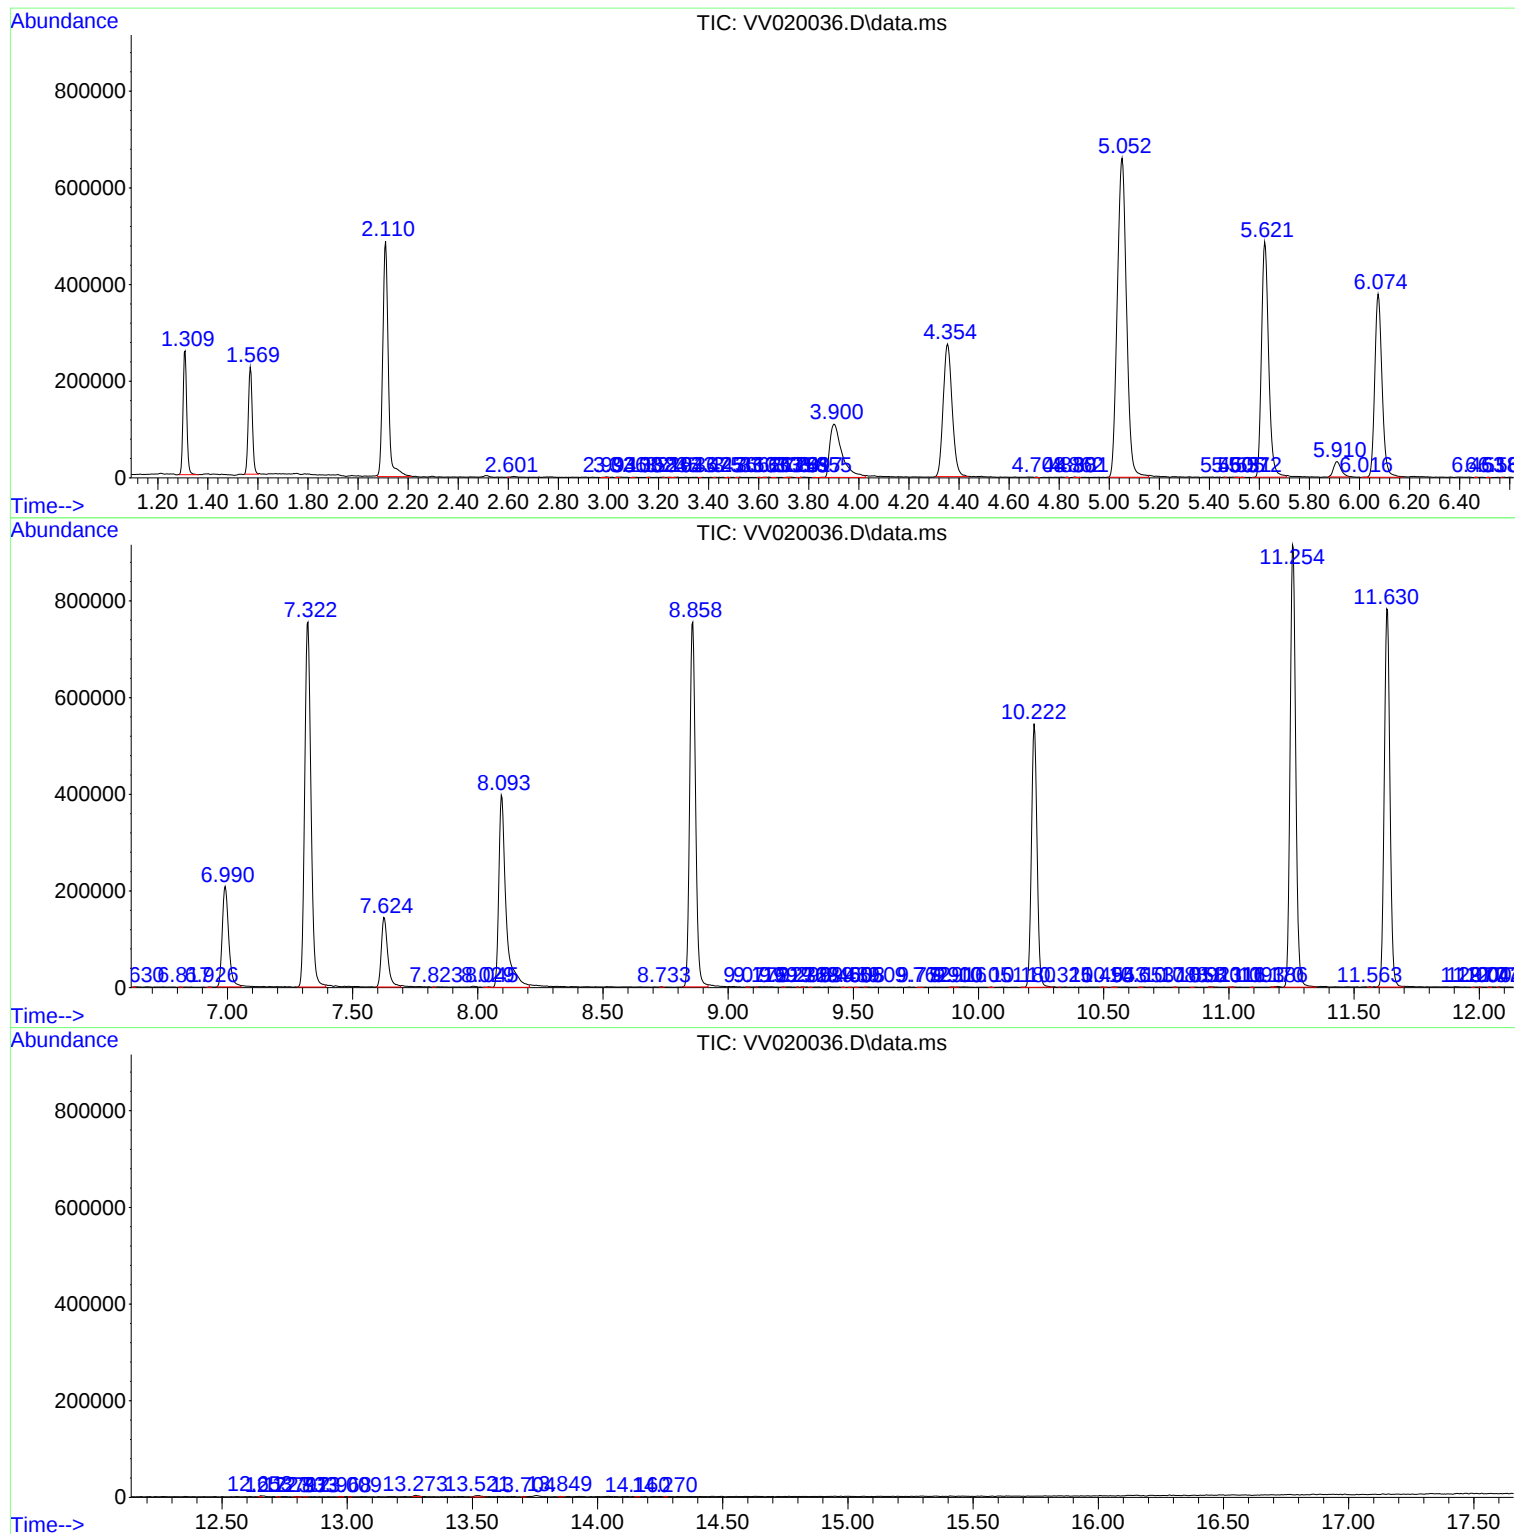

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020036.D
Acq On : 18 Jan 2021 11:47
Operator : SY/MD
Sample : VV0118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020036.D
Acq On : 18 Jan 2021 11:47
Operator : SY/MD
Sample : VV0118WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
