

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020037.D
 Acq On : 18 Jan 2021 12:10
 Operator : SY/MD
 Sample : VV0118MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	260491	269852	15.99%	1.989%
2	1.569	142	149	159	rVB	219710	246459	14.61%	1.816%
3	2.110	307	317	352	rVB	480189	732258	43.40%	5.397%
4	2.348	389	391	395	rBV5	892	532	0.03%	0.004%
5	2.518	435	444	456	rVB5	2322	4776	0.28%	0.035%
6	2.605	468	471	473	rBV3	955	532	0.03%	0.004%
7	2.685	495	496	498	rBV	557	253	0.01%	0.002%
8	2.817	533	537	538	rBV	536	328	0.02%	0.002%
9	2.881	550	557	561	rBV4	829	1187	0.07%	0.009%
10	2.917	566	568	571	rVB2	549	317	0.02%	0.002%
11	2.971	583	585	589	rBV3	377	281	0.02%	0.002%
12	3.023	599	601	602	rBV	752	237	0.01%	0.002%
13	3.241	667	669	672	rBV3	399	216	0.01%	0.002%
14	3.274	676	679	683	rBV4	798	637	0.04%	0.005%
15	3.319	691	693	695	rVB3	593	226	0.01%	0.002%
16	3.331	695	697	699	rBV2	478	263	0.02%	0.002%
17	3.415	719	723	725	rBV3	769	477	0.03%	0.004%
18	3.467	737	739	741	rBV2	666	292	0.02%	0.002%
19	3.492	745	747	748	rBV	603	252	0.01%	0.002%
20	3.560	767	768	770	rBV	273	130	0.01%	0.001%
21	3.589	775	777	778	rBV	378	158	0.01%	0.001%
22	3.618	784	786	789	rVB3	593	289	0.02%	0.002%
23	3.634	789	791	793	rBV2	421	191	0.01%	0.001%
24	3.753	826	828	830	rVB	540	188	0.01%	0.001%
25	3.775	832	835	837	rVB3	504	322	0.02%	0.002%
26	3.791	838	840	842	rBV2	448	174	0.01%	0.001%
27	3.901	862	874	920	rBV	113068	382826	22.69%	2.821%
28	4.286	990	994	995	rBV2	911	649	0.04%	0.005%
29	4.354	1000	1015	1049	rVB	277586	686664	40.70%	5.061%
30	4.778	1146	1147	1150	rBV2	555	265	0.02%	0.002%
31	4.875	1174	1177	1180	rBV3	454	200	0.01%	0.001%
32	4.891	1180	1182	1183	rBV2	377	142	0.01%	0.001%
33	4.901	1183	1185	1192	rVV4	676	524	0.03%	0.004%
34	5.052	1214	1232	1263	rBV2	656551	1687325	100.00%	12.435%
35	5.357	1326	1327	1331	rBV2	851	618	0.04%	0.005%
36	5.621	1395	1409	1438	rBV	466291	945862	56.06%	6.971%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020037.D
 Acq On : 18 Jan 2021 12:10
 Operator : SY/MD
 Sample : VV0118MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.910	1488	1499	1518	rBV3	33622	67950	4.03%	0.501%
38	5.997	1524	1526	1528	rBV3	553	258	0.02%	0.002%
39	6.016	1528	1532	1536	rBV4	698	707	0.04%	0.005%
40	6.074	1536	1550	1577	rBV	380959	770201	45.65%	5.676%
41	6.457	1667	1669	1675	rVB4	692	423	0.03%	0.003%
42	6.489	1676	1679	1681	rBV3	634	389	0.02%	0.003%
43	6.518	1686	1688	1690	rVV2	377	124	0.01%	0.001%
44	6.553	1697	1699	1701	rBV2	374	106	0.01%	0.001%
45	6.563	1701	1702	1704	rBV	421	194	0.01%	0.001%
46	6.605	1711	1715	1716	rBV2	293	181	0.01%	0.001%
47	6.627	1716	1722	1724	rBV5	854	899	0.05%	0.007%
48	6.640	1724	1726	1729	rVV3	821	495	0.03%	0.004%
49	6.717	1747	1750	1752	rBV2	352	184	0.01%	0.001%
50	6.759	1757	1763	1766	rBV2	536	459	0.03%	0.003%
51	6.778	1766	1769	1774	rVB3	447	317	0.02%	0.002%
52	6.804	1774	1777	1781	rVB2	524	354	0.02%	0.003%
53	6.827	1781	1784	1787	rBV	356	214	0.01%	0.002%
54	6.855	1792	1793	1795	rBV	270	134	0.01%	0.001%
55	6.884	1798	1802	1804	rBV	314	204	0.01%	0.002%
56	6.920	1812	1813	1816	rVB	600	146	0.01%	0.001%
57	6.990	1822	1835	1860	rBV2	238141	438347	25.98%	3.230%
58	7.322	1925	1938	1973	rBV	927461	1604850	95.11%	11.827%
59	7.624	2023	2032	2063	rBV	142897	252657	14.97%	1.862%
60	7.981	2138	2143	2154	rVB10	2139	3146	0.19%	0.023%
61	8.026	2154	2157	2158	rBV2	604	331	0.02%	0.002%
62	8.093	2168	2178	2211	rBV2	408203	807906	47.88%	5.954%
63	8.543	2315	2318	2320	rBV4	790	587	0.03%	0.004%
64	8.621	2338	2342	2345	rBV3	972	841	0.05%	0.006%
65	8.653	2351	2352	2354	rBV2	365	96	0.01%	0.001%
66	8.669	2354	2357	2358	rBV2	849	422	0.03%	0.003%
67	8.855	2403	2415	2437	rBV	719587	1180678	69.97%	8.701%
68	9.299	2550	2553	2554	rBV2	668	421	0.02%	0.003%
69	9.424	2586	2592	2595	rBV5	920	999	0.06%	0.007%
70	9.688	2671	2674	2677	rBV	376	167	0.01%	0.001%
71	9.711	2679	2681	2685	rBV2	411	289	0.02%	0.002%
72	9.769	2696	2699	2702	rBV2	491	284	0.02%	0.002%
73	9.804	2708	2710	2715	rBV3	458	295	0.02%	0.002%
74	9.907	2740	2742	2747	rVB3	342	233	0.01%	0.002%
75	9.933	2747	2750	2751	rBV	607	366	0.02%	0.003%
76	10.019	2772	2777	2782	rVB2	377	443	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020037.D
 Acq On : 18 Jan 2021 12:10
 Operator : SY/MD
 Sample : VV0118MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.064	2789	2791	2792	rBV2	232	94	0.01%	0.001%
78	10.129	2808	2811	2813	rBV	311	190	0.01%	0.001%
79	10.222	2826	2840	2863	rBV	550086	860696	51.01%	6.343%
80	10.521	2932	2933	2936	rVB	370	150	0.01%	0.001%
81	10.579	2949	2951	2956	rBV3	450	251	0.01%	0.002%
82	10.627	2962	2966	2968	rBV	297	234	0.01%	0.002%
83	10.698	2986	2988	2991	rVB2	618	295	0.02%	0.002%
84	10.717	2991	2994	2997	rBV3	465	341	0.02%	0.003%
85	10.752	3004	3005	3008	rBV3	312	159	0.01%	0.001%
86	10.791	3015	3017	3018	rBV2	491	243	0.01%	0.002%
87	11.119	3115	3119	3122	rBV2	673	505	0.03%	0.004%
88	11.135	3122	3124	3125	rBV	427	194	0.01%	0.001%
89	11.254	3149	3161	3190	rBV	870719	1360128	80.61%	10.024%
90	11.537	3247	3249	3252	rBV3	592	255	0.02%	0.002%
91	11.633	3267	3279	3299	rBV	784937	1238604	73.41%	9.128%
92	11.849	3344	3346	3349	rBV2	667	473	0.03%	0.003%
93	12.058	3409	3411	3414	rBV3	493	363	0.02%	0.003%
94	12.405	3517	3519	3520	rBV2	716	261	0.02%	0.002%
95	12.444	3529	3531	3535	rBV3	644	493	0.03%	0.004%
96	12.527	3554	3557	3558	rBV	496	247	0.01%	0.002%
97	12.842	3653	3655	3656	rBV	751	303	0.02%	0.002%
98	12.952	3686	3689	3691	rBV3	881	540	0.03%	0.004%
99	13.270	3785	3788	3789	rBV3	878	568	0.03%	0.004%
100	13.981	4007	4009	4010	rBV	678	242	0.01%	0.002%




Sum of corrected areas: 13569028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020037.D
Acq On : 18 Jan 2021 12:10
Operator : SY/MD
Sample : VV0118MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

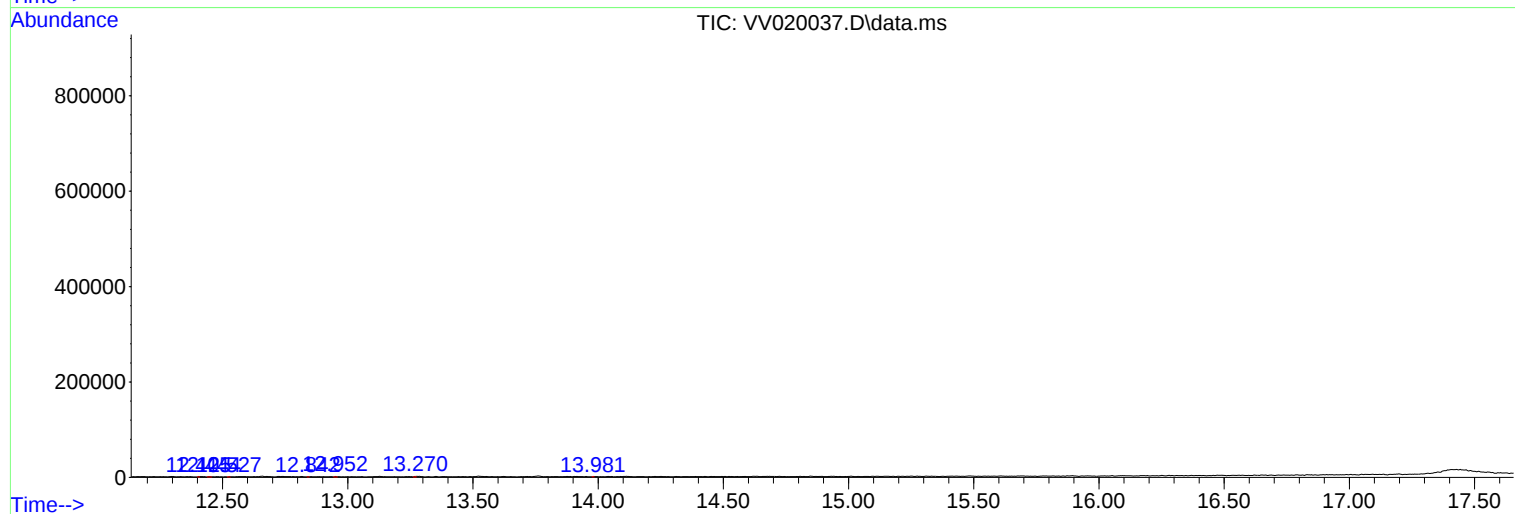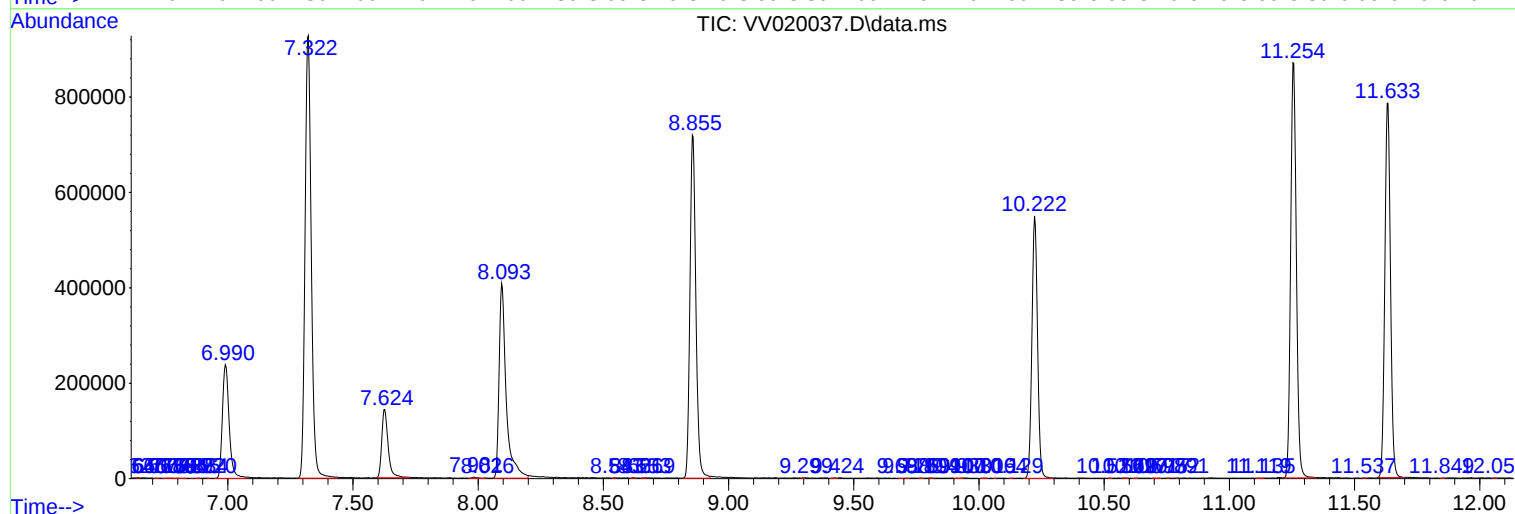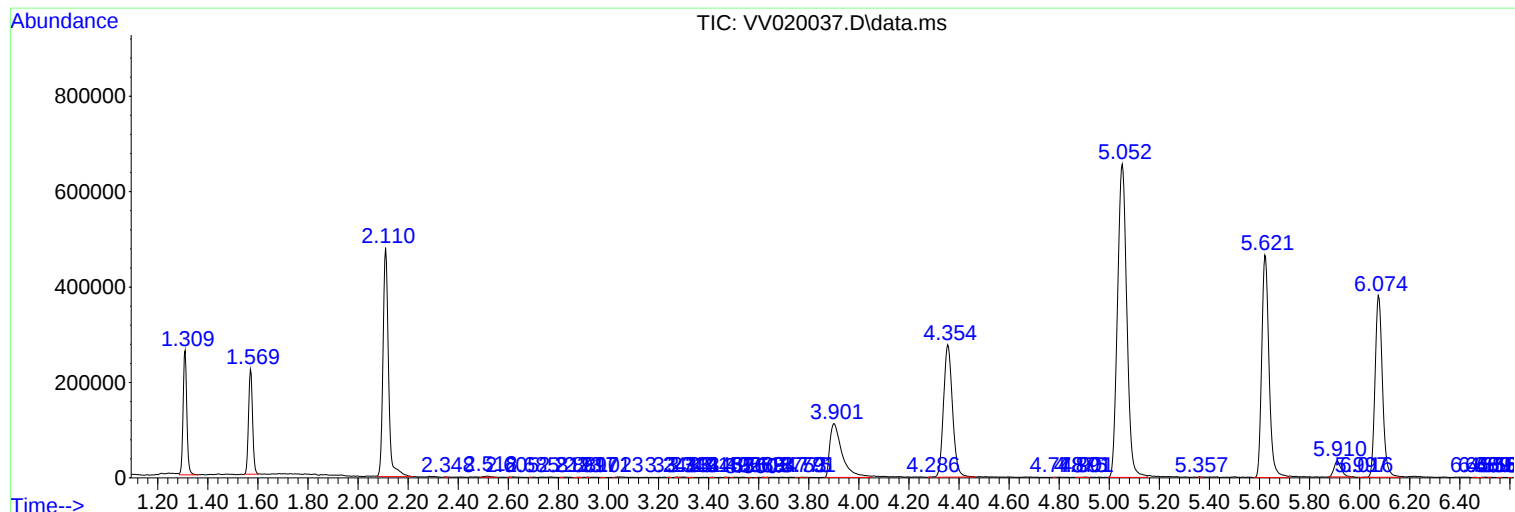

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020037.D
Acq On : 18 Jan 2021 12:10
Operator : SY/MD
Sample : VV0118MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020037.D
Acq On : 18 Jan 2021 12:10
Operator : SY/MD
Sample : VV0118MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
