

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011821\
 Data File : VW020039.D
 Acq On : 18 Jan 2021 13:11
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VW020039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	78	rVB	149875	152909	10.73%	1.276%
2	1.569	142	149	164	rVB	170439	192224	13.49%	1.604%
3	2.110	307	317	355	rVB	349347	544752	38.24%	4.546%
4	2.270	365	367	369	rBV3	687	400	0.03%	0.003%
5	2.508	436	441	443	rBV4	1817	1683	0.12%	0.014%
6	2.621	473	476	481	rBV3	873	832	0.06%	0.007%
7	2.749	514	516	519	rBV	566	423	0.03%	0.004%
8	2.801	530	532	536	rVB2	1176	594	0.04%	0.005%
9	2.836	540	543	546	rBV2	483	402	0.03%	0.003%
10	2.872	550	554	555	rBV3	786	544	0.04%	0.005%
11	2.897	560	562	564	rBV2	761	434	0.03%	0.004%
12	3.261	672	675	678	rBV4	769	516	0.04%	0.004%
13	3.325	691	695	696	rBV2	522	347	0.02%	0.003%
14	3.347	700	702	705	rVV2	774	483	0.03%	0.004%
15	3.376	707	711	713	rBV3	584	337	0.02%	0.003%
16	3.425	724	726	730	rBV2	591	446	0.03%	0.004%
17	3.492	746	747	749	rBV2	591	302	0.02%	0.003%
18	3.528	756	758	760	rBV2	736	313	0.02%	0.003%
19	3.608	779	783	787	rBV4	469	341	0.02%	0.003%
20	3.714	810	816	817	rVV3	805	559	0.04%	0.005%
21	3.740	821	824	826	rBV2	487	306	0.02%	0.003%
22	3.817	845	848	851	rBV	487	395	0.03%	0.003%
23	3.897	862	873	902	rBV	109711	339616	23.84%	2.834%
24	4.267	987	988	993	rBV4	744	632	0.04%	0.005%
25	4.354	999	1015	1039	rBV	245030	599260	42.07%	5.000%
26	4.547	1071	1075	1076	rBV4	717	475	0.03%	0.004%
27	4.746	1133	1137	1139	rBV2	815	489	0.03%	0.004%
28	4.782	1145	1148	1150	rVB3	728	388	0.03%	0.003%
29	4.794	1150	1152	1156	rVB3	555	315	0.02%	0.003%
30	4.814	1156	1158	1160	rBV2	644	301	0.02%	0.003%
31	4.868	1170	1175	1176	rVB4	672	466	0.03%	0.004%
32	4.888	1176	1181	1184	rBV5	813	924	0.06%	0.008%
33	4.920	1188	1191	1192	rBV2	542	367	0.03%	0.003%
34	5.052	1214	1232	1256	rBV2	549495	1424520	100.00%	11.887%
35	5.312	1311	1313	1316	rVB4	1046	516	0.04%	0.004%
36	5.486	1364	1367	1368	rBV	699	478	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011821\
 Data File : VW020039.D
 Acq On : 18 Jan 2021 13:11
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.524	1377	1379	1385	rVB4	1041	743	0.05%	0.006%
38	5.621	1393	1409	1440	rBV	461747	943271	66.22%	7.871%
39	5.865	1483	1485	1487	rBV2	651	381	0.03%	0.003%
40	5.910	1489	1499	1517	rVB2	37138	76004	5.34%	0.634%
41	6.074	1535	1550	1575	rBV	391313	794350	55.76%	6.628%
42	6.476	1671	1675	1678	rBV3	719	491	0.03%	0.004%
43	6.579	1705	1707	1711	rBV2	529	460	0.03%	0.004%
44	6.624	1719	1721	1722	rBV	844	451	0.03%	0.004%
45	6.736	1754	1756	1759	rBV3	530	329	0.02%	0.003%
46	6.814	1777	1780	1781	rBV3	601	366	0.03%	0.003%
47	6.823	1781	1783	1785	rVV2	911	447	0.03%	0.004%
48	6.849	1788	1791	1794	rVB3	523	333	0.02%	0.003%
49	6.865	1794	1796	1802	rVB3	588	555	0.04%	0.005%
50	6.920	1808	1813	1816	rBV4	543	471	0.03%	0.004%
51	6.990	1823	1835	1857	rBV2	170755	319730	22.44%	2.668%
52	7.322	1926	1938	1964	rBV	619196	1071394	75.21%	8.940%
53	7.560	2011	2012	2014	rBV2	715	298	0.02%	0.002%
54	7.627	2023	2033	2058	rBV	122848	217293	15.25%	1.813%
55	7.736	2065	2067	2071	rBV3	806	383	0.03%	0.003%
56	7.981	2140	2143	2146	rBV3	777	627	0.04%	0.005%
57	8.093	2168	2178	2210	rBV2	375136	752486	52.82%	6.279%
58	8.637	2341	2347	2351	rBV4	633	735	0.05%	0.006%
59	8.691	2359	2364	2369	rVB2	618	584	0.04%	0.005%
60	8.791	2392	2395	2397	rBV2	506	346	0.02%	0.003%
61	8.859	2403	2416	2441	rBV	860592	1394315	97.88%	11.635%
62	9.479	2602	2609	2610	rBV4	708	812	0.06%	0.007%
63	9.518	2618	2621	2622	rBV	568	319	0.02%	0.003%
64	9.572	2636	2638	2641	rVB3	627	324	0.02%	0.003%
65	9.723	2681	2685	2689	rBV6	645	714	0.05%	0.006%
66	9.762	2693	2697	2699	rBV3	681	510	0.04%	0.004%
67	9.830	2713	2718	2720	rBV3	707	669	0.05%	0.006%
68	9.878	2731	2733	2737	rVB4	928	445	0.03%	0.004%
69	9.945	2752	2754	2757	rVB2	720	333	0.02%	0.003%
70	10.029	2774	2780	2783	rBV4	668	776	0.05%	0.006%
71	10.132	2808	2812	2813	rBV2	645	369	0.03%	0.003%
72	10.222	2827	2840	2856	rBV	438129	691062	48.51%	5.767%
73	10.318	2868	2870	2874	rBV3	438	354	0.02%	0.003%
74	10.424	2901	2903	2906	rBV3	524	323	0.02%	0.003%
75	10.444	2907	2909	2912	rVB3	910	429	0.03%	0.004%
76	10.502	2925	2927	2930	rBV3	727	383	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020039.D
 Acq On : 18 Jan 2021 13:11
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.804	3019	3021	3024	rBV	606	471	0.03%	0.004%
78	10.971	3070	3073	3077	rBV3	833	687	0.05%	0.006%
79	11.096	3110	3112	3115	rVB2	853	381	0.03%	0.003%
80	11.119	3115	3119	3120	rBV2	734	436	0.03%	0.004%
81	11.190	3138	3141	3142	rBV2	843	534	0.04%	0.004%
82	11.257	3149	3162	3187	rBV	756150	1175143	82.49%	9.806%
83	11.511	3238	3241	3248	rBV6	733	811	0.06%	0.007%
84	11.585	3262	3264	3266	rBV	503	302	0.02%	0.003%
85	11.630	3266	3278	3301	rVV	793864	1254205	88.04%	10.466%
86	11.813	3332	3335	3339	rVB3	764	455	0.03%	0.004%
87	12.077	3414	3417	3421	rBV3	521	466	0.03%	0.004%
88	12.283	3475	3481	3484	rBV4	673	690	0.05%	0.006%
89	12.334	3495	3497	3502	rVB3	698	375	0.03%	0.003%
90	12.386	3511	3513	3515	rBV2	929	404	0.03%	0.003%
91	12.723	3616	3618	3623	rBV5	777	409	0.03%	0.003%
92	12.804	3641	3643	3647	rBV6	560	468	0.03%	0.004%
93	12.855	3656	3659	3661	rBV2	586	295	0.02%	0.002%
94	12.929	3678	3682	3684	rBV3	632	494	0.03%	0.004%
95	13.016	3707	3709	3715	rBV4	803	916	0.06%	0.008%
96	13.064	3722	3724	3730	rBV4	903	956	0.07%	0.008%
97	13.399	3827	3828	3833	rBV2	678	410	0.03%	0.003%
98	13.453	3842	3845	3849	rBV3	728	825	0.06%	0.007%
99	13.505	3855	3861	3862	rBV4	737	606	0.04%	0.005%
100	14.003	4014	4016	4018	rBV2	523	345	0.02%	0.003%




Sum of corrected areas: 11984038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020039.D
Acq On : 18 Jan 2021 13:11
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

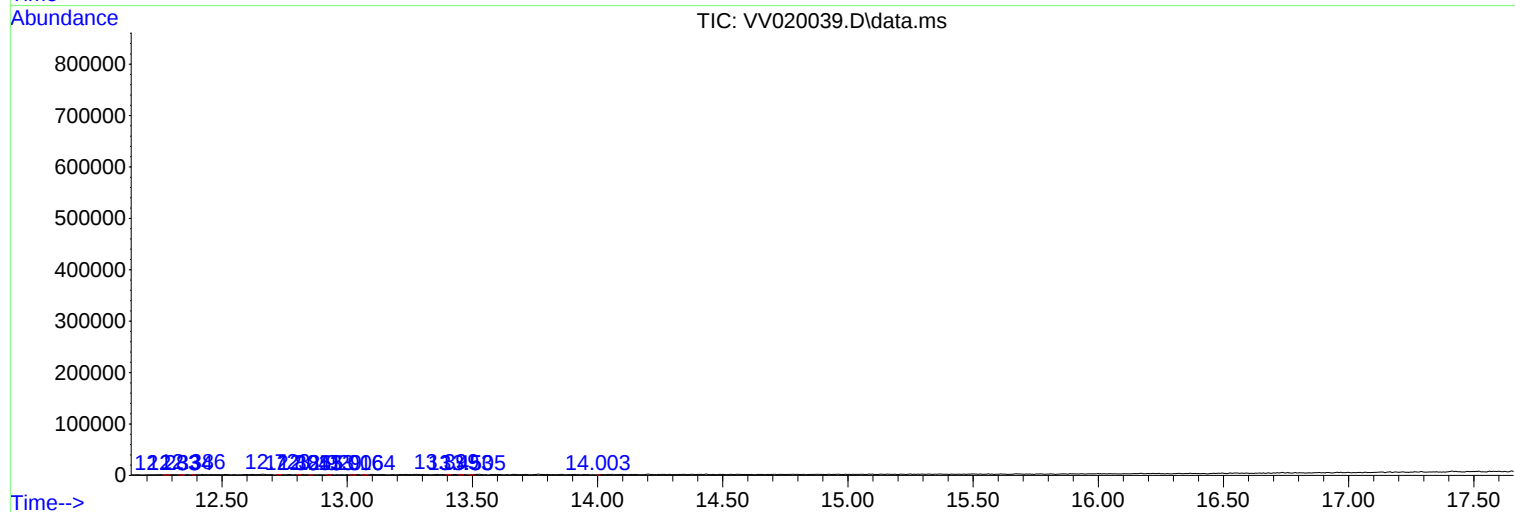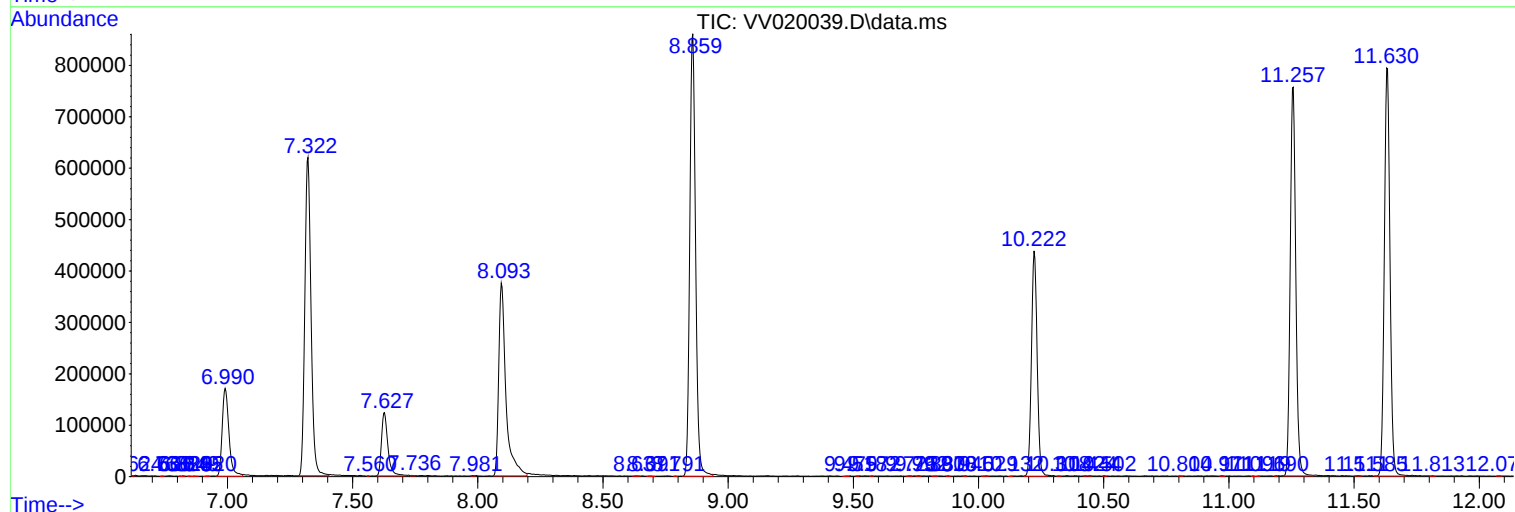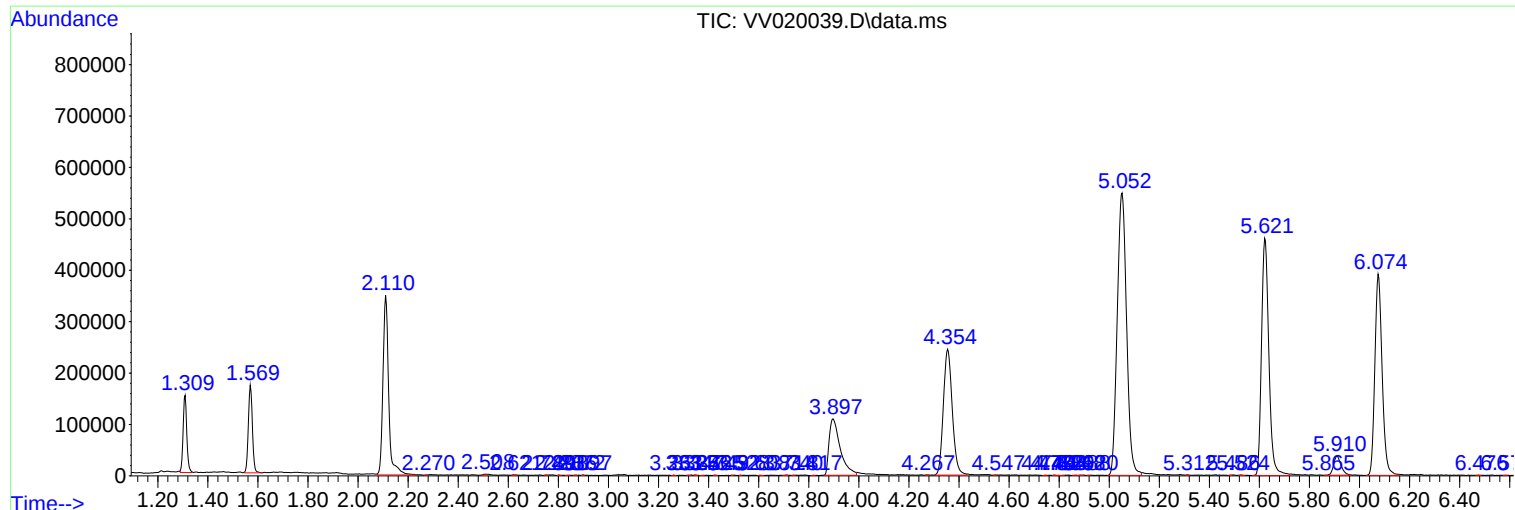

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020039.D
Acq On : 18 Jan 2021 13:11
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020039.D
Acq On : 18 Jan 2021 13:11
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
