

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020040.D
 Acq On : 18 Jan 2021 13:34
 Operator : SY/MD
 Sample : M1147-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	82	rVB	216416	215200	14.17%	1.728%
2	1.569	142	149	161	rBV	190092	211580	13.93%	1.699%
3	2.110	307	317	354	rVB	387349	605958	39.90%	4.866%
4	2.855	547	549	553	rVB4	670	357	0.02%	0.003%
5	2.897	559	562	563	rBV2	480	248	0.02%	0.002%
6	2.926	569	571	572	rBV2	566	286	0.02%	0.002%
7	3.048	597	609	622	rBV9	5374	11717	0.77%	0.094%
8	3.190	650	653	656	rBV3	697	463	0.03%	0.004%
9	3.254	669	673	675	rBV2	825	450	0.03%	0.004%
10	3.386	712	714	716	rVB2	507	222	0.01%	0.002%
11	3.434	727	729	731	rBV2	378	218	0.01%	0.002%
12	3.476	740	742	745	rVB	466	237	0.02%	0.002%
13	3.492	745	747	748	rBV2	577	221	0.01%	0.002%
14	3.560	762	768	771	rBV6	835	703	0.05%	0.006%
15	3.589	775	777	779	rBV	544	199	0.01%	0.002%
16	3.682	804	806	808	rBV2	506	288	0.02%	0.002%
17	3.765	819	832	847	rBV8	6501	16377	1.08%	0.132%
18	3.846	855	857	861	rVB3	589	350	0.02%	0.003%
19	3.897	861	873	911	rBV	105977	355109	23.39%	2.852%
20	4.354	1000	1015	1042	rBV	259378	628938	41.42%	5.051%
21	4.666	1107	1112	1114	rBV4	959	812	0.05%	0.007%
22	4.688	1114	1119	1120	rBV4	887	790	0.05%	0.006%
23	4.743	1134	1136	1138	rBV	604	369	0.02%	0.003%
24	4.801	1150	1154	1158	rVB3	647	479	0.03%	0.004%
25	4.984	1208	1211	1212	rVB	578	249	0.02%	0.002%
26	4.994	1212	1214	1215	rBV	553	206	0.01%	0.002%
27	5.052	1215	1232	1260	rBV2	593981	1518517	100.00%	12.195%
28	5.383	1333	1335	1336	rBV2	919	366	0.02%	0.003%
29	5.402	1339	1341	1345	rVB3	1181	607	0.04%	0.005%
30	5.418	1345	1346	1349	rBV3	854	491	0.03%	0.004%
31	5.482	1364	1366	1367	rBV2	751	312	0.02%	0.003%
32	5.560	1385	1390	1394	rVB6	971	974	0.06%	0.008%
33	5.621	1394	1409	1434	rBV	463383	938623	61.81%	7.538%
34	5.910	1487	1499	1517	rBV	50091	103986	6.85%	0.835%
35	6.074	1534	1550	1575	rBV	405853	827048	54.46%	6.642%
36	6.428	1657	1660	1666	rVB3	664	645	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020040.D
 Acq On : 18 Jan 2021 13:34
 Operator : SY/MD
 Sample : M1147-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.463	1666	1671	1676	rVB4	637	654	0.04%	0.005%
38	6.489	1676	1679	1681	rBV2	720	417	0.03%	0.003%
39	6.701	1743	1745	1748	rBV2	508	312	0.02%	0.003%
40	6.752	1758	1761	1764	rVB3	366	214	0.01%	0.002%
41	6.768	1764	1766	1768	rBV3	394	211	0.01%	0.002%
42	6.801	1774	1776	1780	rBV3	438	331	0.02%	0.003%
43	6.916	1809	1812	1814	rBV	438	274	0.02%	0.002%
44	6.936	1814	1818	1820	rBV3	343	309	0.02%	0.002%
45	6.990	1823	1835	1856	rBV	210364	386271	25.44%	3.102%
46	7.322	1925	1938	1961	rBV	653782	1143141	75.28%	9.180%
47	7.624	2020	2032	2050	rBV	129561	230450	15.18%	1.851%
48	7.846	2098	2101	2104	rBV3	1100	692	0.05%	0.006%
49	7.942	2128	2131	2132	rBV3	634	366	0.02%	0.003%
50	7.968	2135	2139	2142	rBV4	490	356	0.02%	0.003%
51	8.022	2153	2156	2157	rBV2	512	238	0.02%	0.002%
52	8.055	2162	2166	2167	rBV2	794	394	0.03%	0.003%
53	8.096	2168	2179	2215	rBV3	356368	755958	49.78%	6.071%
54	8.537	2312	2316	2317	rBV3	936	651	0.04%	0.005%
55	8.582	2328	2330	2332	rBV3	738	427	0.03%	0.003%
56	8.643	2347	2349	2351	rVB2	1013	449	0.03%	0.004%
57	8.685	2360	2362	2364	rVB	813	275	0.02%	0.002%
58	8.714	2368	2371	2372	rBV3	626	335	0.02%	0.003%
59	8.743	2378	2380	2382	rBV2	409	286	0.02%	0.002%
60	8.765	2385	2387	2389	rVV2	553	237	0.02%	0.002%
61	8.858	2403	2416	2442	rBV	715551	1173906	77.31%	9.427%
62	9.148	2502	2506	2508	rBV3	1090	879	0.06%	0.007%
63	9.186	2516	2518	2520	rBV3	512	235	0.02%	0.002%
64	9.283	2546	2548	2552	rVB	536	303	0.02%	0.002%
65	9.456	2599	2602	2603	rBV	752	424	0.03%	0.003%
66	9.489	2609	2612	2613	rBV	434	307	0.02%	0.002%
67	9.518	2617	2621	2622	rBV2	1097	618	0.04%	0.005%
68	9.672	2664	2669	2671	rBV4	816	716	0.05%	0.006%
69	9.736	2686	2689	2692	rVB2	742	535	0.04%	0.004%
70	9.813	2711	2713	2717	rBV3	505	322	0.02%	0.003%
71	9.981	2763	2765	2770	rVB2	476	256	0.02%	0.002%
72	10.222	2828	2840	2864	rVV	490998	781621	51.47%	6.277%
73	10.456	2910	2913	2915	rVV2	376	196	0.01%	0.002%
74	10.781	3011	3014	3017	rBV2	464	358	0.02%	0.003%
75	10.858	3034	3038	3041	rBV4	960	615	0.04%	0.005%
76	10.874	3041	3043	3045	rVB2	473	211	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020040.D
 Acq On : 18 Jan 2021 13:34
 Operator : SY/MD
 Sample : M1147-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.894	3045	3049	3055	rBV4	833	904	0.06%	0.007%
78	10.977	3072	3075	3078	rBV	489	386	0.03%	0.003%
79	11.016	3085	3087	3090	rBV2	381	244	0.02%	0.002%
80	11.157	3128	3131	3134	rVB3	762	542	0.04%	0.004%
81	11.173	3134	3136	3137	rBV	796	322	0.02%	0.003%
82	11.254	3149	3161	3182	rBV	891691	1354325	89.19%	10.876%
83	11.630	3266	3278	3302	rBV	729628	1158889	76.32%	9.307%
84	11.878	3352	3355	3361	rVB3	1008	974	0.06%	0.008%
85	11.903	3361	3363	3366	rBV2	486	241	0.02%	0.002%
86	11.919	3366	3368	3370	rBV2	438	212	0.01%	0.002%
87	11.997	3388	3392	3393	rBV3	741	559	0.04%	0.004%
88	12.093	3420	3422	3426	rBV4	799	550	0.04%	0.004%
89	12.148	3436	3439	3440	rBV2	1015	474	0.03%	0.004%
90	12.411	3518	3521	3522	rBV3	742	418	0.03%	0.003%
91	12.591	3575	3577	3578	rBV	739	344	0.02%	0.003%
92	12.630	3586	3589	3592	rBV2	870	570	0.04%	0.005%
93	12.794	3635	3640	3644	rBV6	712	683	0.04%	0.005%
94	12.839	3651	3654	3656	rBV2	622	362	0.02%	0.003%
95	13.106	3732	3737	3742	rBV4	749	720	0.05%	0.006%
96	13.244	3777	3780	3783	rBV4	765	487	0.03%	0.004%
97	13.585	3884	3886	3891	rBV3	1010	763	0.05%	0.006%
98	13.736	3931	3933	3936	rBV3	688	294	0.02%	0.002%
99	13.800	3951	3953	3956	rVB3	944	450	0.03%	0.004%
100	13.971	4003	4006	4007	rBV3	643	321	0.02%	0.003%




Sum of corrected areas: 12452379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020040.D
Acq On : 18 Jan 2021 13:34
Operator : SY/MD
Sample : M1147-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

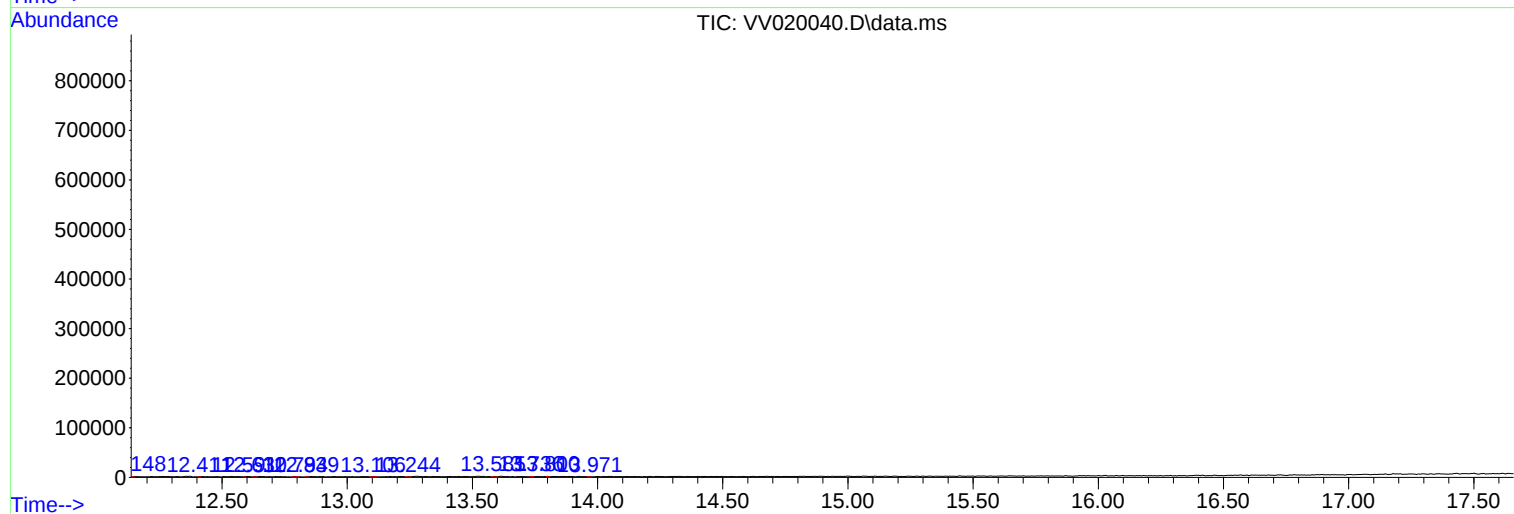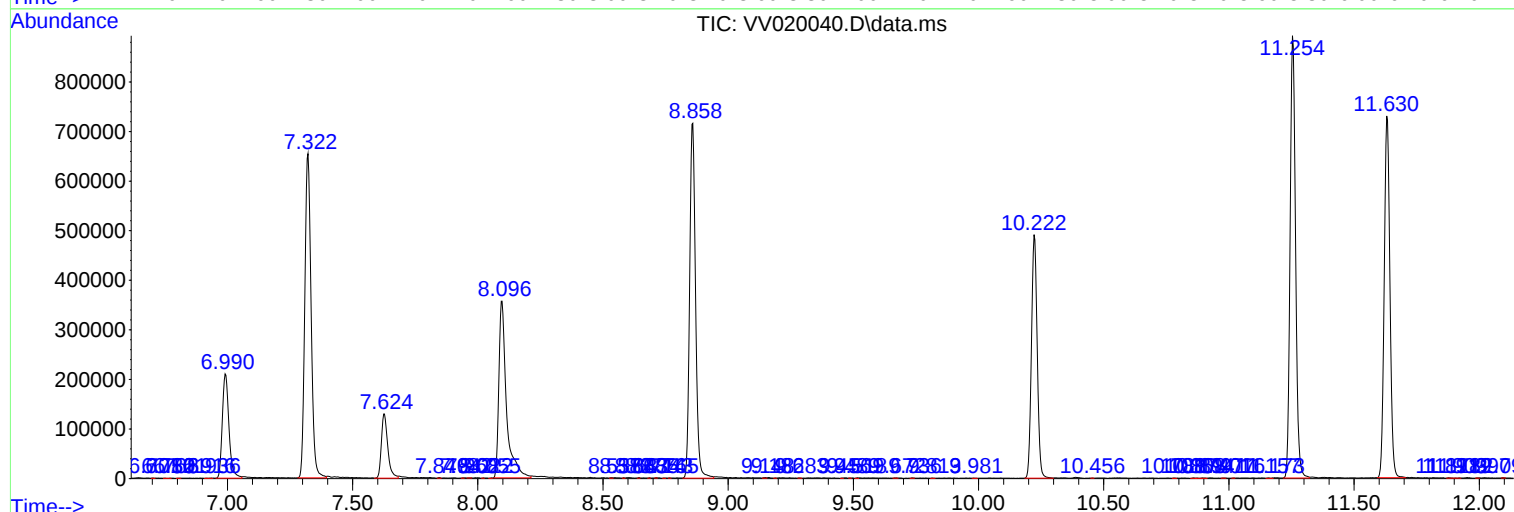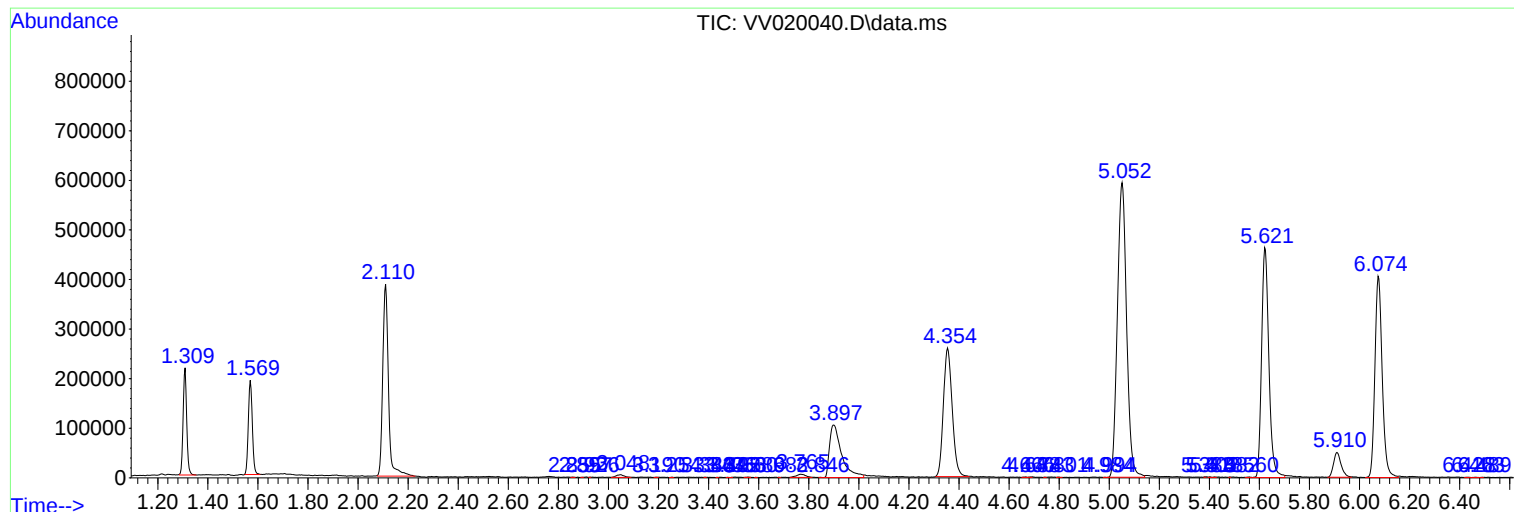

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020040.D
Acq On : 18 Jan 2021 13:34
Operator : SY/MD
Sample : M1147-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020040.D
Acq On : 18 Jan 2021 13:34
Operator : SY/MD
Sample : M1147-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------