

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020042.D
 Acq On : 18 Jan 2021 14:21
 Operator : SY/MD
 Sample : M1147-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	83	rVB	209178	212867	14.11%	1.696%
2	1.569	142	149	161	rVB	188591	211910	14.05%	1.688%
3	2.110	307	317	346	rVB	352007	535268	35.49%	4.263%
4	2.360	393	395	399	rBV2	241	207	0.01%	0.002%
5	2.528	435	447	464	rVB2	4155	10969	0.73%	0.087%
6	2.614	470	474	475	rBV	590	435	0.03%	0.003%
7	2.656	484	487	489	rBV	190	140	0.01%	0.001%
8	2.762	507	520	534	rBV3	6911	13615	0.90%	0.108%
9	2.823	538	539	541	rBV	401	157	0.01%	0.001%
10	2.849	544	547	552	rVB	264	127	0.01%	0.001%
11	2.878	552	556	558	rBV	460	366	0.02%	0.003%
12	2.984	587	589	593	rVB2	592	334	0.02%	0.003%
13	3.042	593	607	626	rBV4	21374	46702	3.10%	0.372%
14	3.171	643	647	648	rBV3	493	320	0.02%	0.003%
15	3.312	689	691	694	rVB2	759	283	0.02%	0.002%
16	3.325	694	695	697	rBV2	528	220	0.01%	0.002%
17	3.344	699	701	703	rVB2	577	241	0.02%	0.002%
18	3.396	715	717	718	rVB2	722	222	0.01%	0.002%
19	3.486	742	745	748	rBV3	517	430	0.03%	0.003%
20	3.563	766	769	771	rBV2	461	214	0.01%	0.002%
21	3.643	790	794	798	rBV2	696	577	0.04%	0.005%
22	3.663	798	800	801	rBV2	596	269	0.02%	0.002%
23	3.769	821	833	850	rVB3	11986	32472	2.15%	0.259%
24	3.833	850	853	856	rBV3	566	432	0.03%	0.003%
25	3.849	856	858	861	rBV	427	215	0.01%	0.002%
26	3.897	861	873	915	rBV	114411	368072	24.40%	2.932%
27	4.354	998	1015	1040	rBV	255886	632534	41.94%	5.038%
28	4.740	1132	1135	1136	rBV2	767	449	0.03%	0.004%
29	4.801	1151	1154	1156	rBV2	667	420	0.03%	0.003%
30	4.817	1157	1159	1161	rVB2	643	324	0.02%	0.003%
31	4.884	1178	1180	1182	rBV2	723	335	0.02%	0.003%
32	4.897	1182	1184	1186	rVV3	686	353	0.02%	0.003%
33	5.052	1214	1232	1257	rBV2	587059	1508249	100.00%	12.013%
34	5.405	1338	1342	1345	rBV4	987	714	0.05%	0.006%
35	5.470	1359	1362	1364	rVB4	990	461	0.03%	0.004%
36	5.495	1364	1370	1373	rBV5	1312	1545	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011821\
 Data File : VW020042.D
 Acq On : 18 Jan 2021 14:21
 Operator : SY/MD
 Sample : M1147-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.621	1396	1409	1429	rBV	475428	953614	63.23%	7.596%
38	5.836	1474	1476	1479	rBV4	942	536	0.04%	0.004%
39	5.910	1487	1499	1512	rBV4	30507	64486	4.28%	0.514%
40	6.074	1536	1550	1578	rBV	345501	703778	46.66%	5.606%
41	6.698	1742	1744	1745	rVB2	684	187	0.01%	0.001%
42	6.727	1750	1753	1755	rBV3	610	403	0.03%	0.003%
43	6.775	1760	1768	1770	rBV5	1504	1528	0.10%	0.012%
44	6.871	1796	1798	1800	rBV3	314	175	0.01%	0.001%
45	6.904	1805	1808	1810	rBV2	435	270	0.02%	0.002%
46	6.990	1824	1835	1855	rBV	213084	387537	25.69%	3.087%
47	7.322	1926	1938	1960	rBV	657325	1134452	75.22%	9.036%
48	7.627	2023	2033	2057	rBV	126121	223829	14.84%	1.783%
49	7.958	2134	2136	2139	rVB3	857	375	0.02%	0.003%
50	8.093	2168	2178	2214	rBV2	390884	782532	51.88%	6.233%
51	8.518	2307	2310	2312	rBV3	873	640	0.04%	0.005%
52	8.714	2369	2371	2373	rBV3	628	281	0.02%	0.002%
53	8.858	2404	2416	2442	rBV	742728	1204229	79.84%	9.592%
54	9.264	2539	2542	2543	rBV	397	226	0.01%	0.002%
55	9.280	2545	2547	2548	rBV	519	182	0.01%	0.001%
56	9.309	2555	2556	2561	rVB3	607	400	0.03%	0.003%
57	9.334	2561	2564	2567	rBV2	741	533	0.04%	0.004%
58	9.379	2576	2578	2582	rBV3	414	319	0.02%	0.003%
59	9.444	2595	2598	2603	rVB3	513	368	0.02%	0.003%
60	9.466	2603	2605	2606	rBV	274	130	0.01%	0.001%
61	9.495	2612	2614	2620	rVB2	553	353	0.02%	0.003%
62	9.524	2620	2623	2626	rBV2	426	320	0.02%	0.003%
63	9.604	2644	2648	2654	rVB5	795	731	0.05%	0.006%
64	9.633	2654	2657	2658	rBV	419	218	0.01%	0.002%
65	9.678	2667	2671	2673	rBV2	475	387	0.03%	0.003%
66	9.746	2689	2692	2693	rBV2	393	208	0.01%	0.002%
67	9.891	2735	2737	2741	rBV3	370	193	0.01%	0.002%
68	9.913	2742	2744	2747	rBV3	434	198	0.01%	0.002%
69	9.997	2767	2770	2771	rBV	292	117	0.01%	0.001%
70	10.071	2790	2793	2796	rBV	645	509	0.03%	0.004%
71	10.090	2796	2799	2804	rVB3	1178	951	0.06%	0.008%
72	10.145	2813	2816	2818	rVB2	529	266	0.02%	0.002%
73	10.164	2818	2822	2823	rBV2	666	313	0.02%	0.002%
74	10.222	2828	2840	2860	rBV	506609	790008	52.38%	6.293%
75	10.389	2888	2892	2895	rBV3	688	578	0.04%	0.005%
76	10.453	2910	2912	2915	rBV3	595	413	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020042.D
 Acq On : 18 Jan 2021 14:21
 Operator : SY/MD
 Sample : M1147-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.614	2961	2962	2965	rVB	723	286	0.02%	0.002%
78	10.630	2965	2967	2970	rBV3	378	224	0.01%	0.002%
79	10.694	2984	2987	2991	rBV3	431	342	0.02%	0.003%
80	10.865	3036	3040	3043	rVB3	322	257	0.02%	0.002%
81	10.897	3048	3050	3052	rBV3	375	125	0.01%	0.001%
82	11.112	3115	3117	3120	rBV3	521	330	0.02%	0.003%
83	11.183	3137	3139	3140	rBV	464	143	0.01%	0.001%
84	11.254	3149	3161	3178	rBV	893373	1372056	90.97%	10.929%
85	11.460	3223	3225	3227	rBV2	781	379	0.03%	0.003%
86	11.479	3229	3231	3234	rBV2	600	312	0.02%	0.002%
87	11.514	3240	3242	3245	rBV3	493	244	0.02%	0.002%
88	11.633	3267	3279	3299	rBV	852260	1335315	88.53%	10.636%
89	11.993	3388	3391	3397	rBV4	792	692	0.05%	0.006%
90	12.087	3418	3420	3423	rBV2	400	218	0.01%	0.002%
91	12.321	3491	3493	3496	rBV2	434	272	0.02%	0.002%
92	12.472	3538	3540	3544	rVB2	531	312	0.02%	0.002%
93	12.653	3593	3596	3597	rBV2	1058	597	0.04%	0.005%
94	12.919	3676	3679	3681	rBV3	840	494	0.03%	0.004%
95	13.090	3730	3732	3734	rBV	383	228	0.02%	0.002%
96	13.353	3811	3814	3816	rBV	583	463	0.03%	0.004%
97	13.569	3879	3881	3882	rBV	539	146	0.01%	0.001%
98	14.112	4048	4050	4053	rBV2	713	488	0.03%	0.004%
99	14.450	4152	4155	4160	rBV4	851	750	0.05%	0.006%
100	14.697	4230	4232	4237	rVB3	1066	799	0.05%	0.006%




Sum of corrected areas: 12554693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020042.D
Acq On : 18 Jan 2021 14:21
Operator : SY/MD
Sample : M1147-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

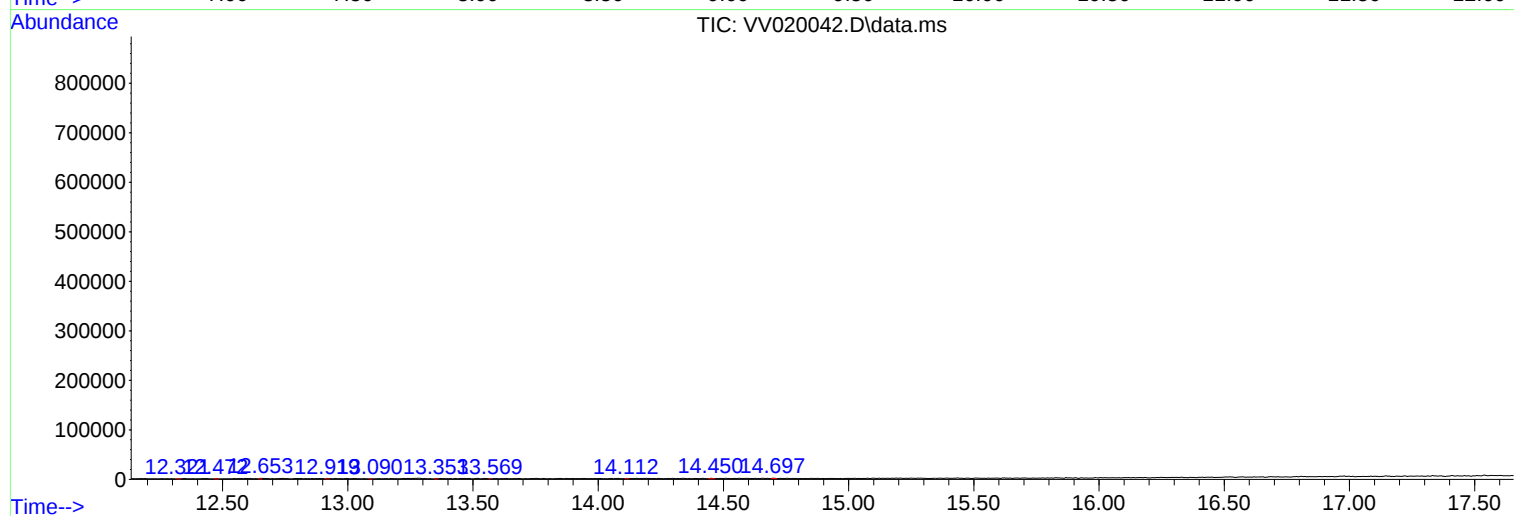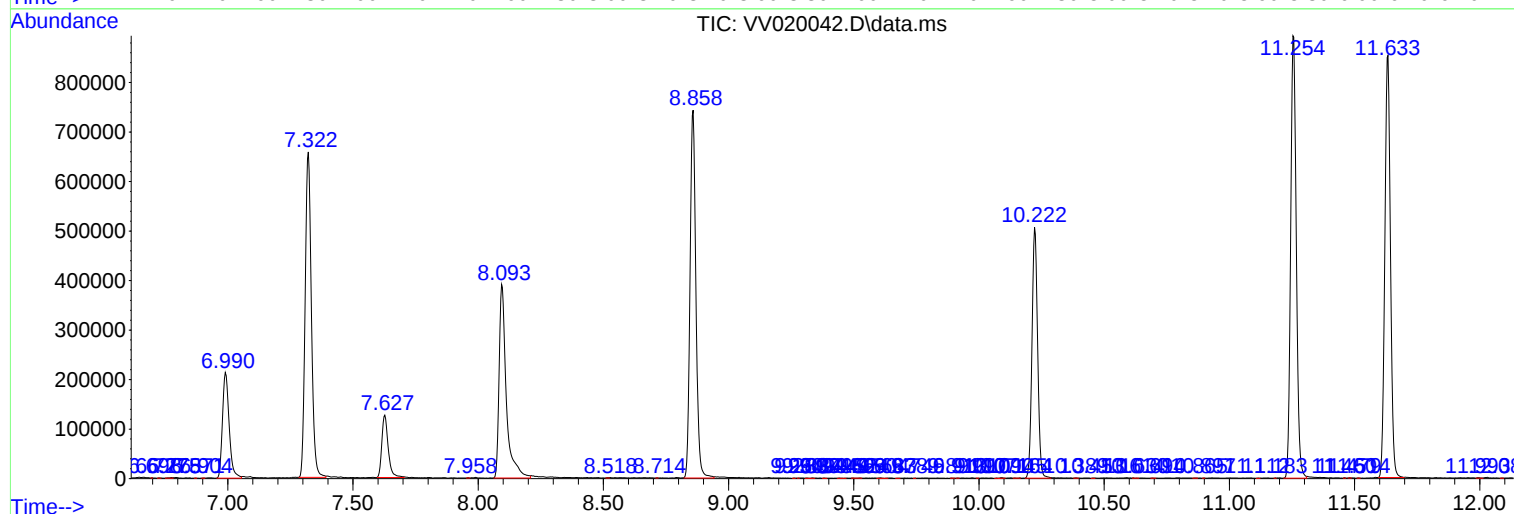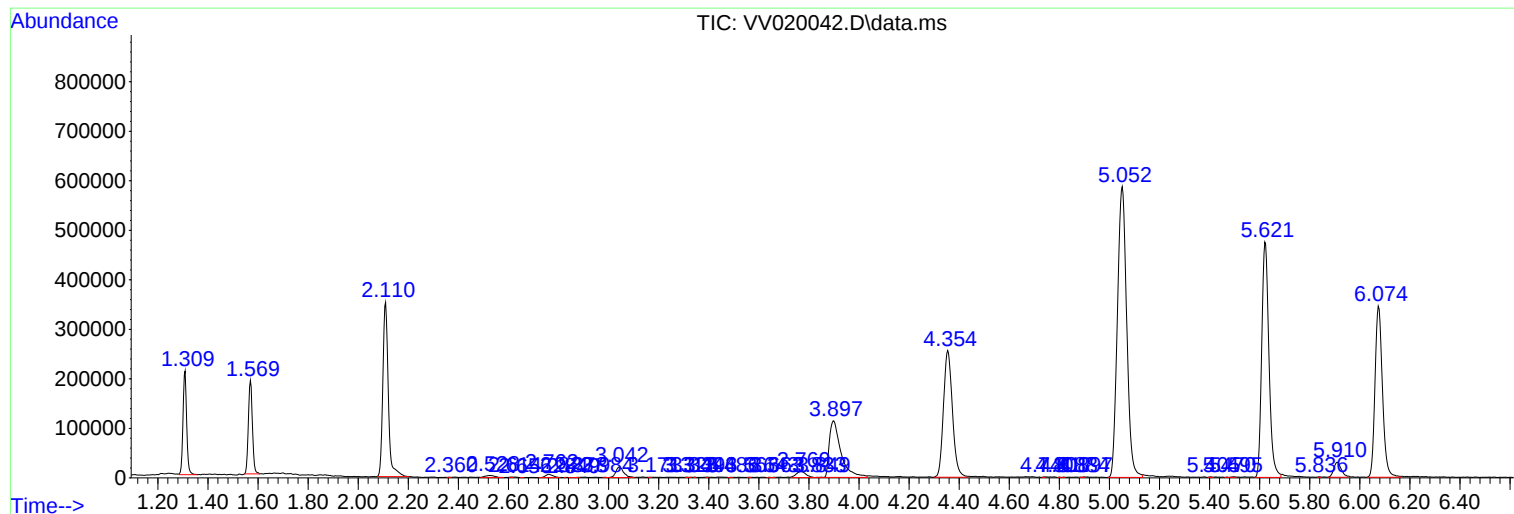

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020042.D
Acq On : 18 Jan 2021 14:21
Operator : SY/MD
Sample : M1147-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020042.D
Acq On : 18 Jan 2021 14:21
Operator : SY/MD
Sample : M1147-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
