

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020049.D
 Acq On : 18 Jan 2021 17:28
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	288209	285903	15.53%	1.837%
2	1.569	142	149	162	rVB	236592	266690	14.49%	1.714%
3	2.109	307	317	343	rVB	520751	780261	42.39%	5.014%
4	2.402	405	408	411	rBV5	650	431	0.02%	0.003%
5	2.441	416	420	426	rVB5	1069	976	0.05%	0.006%
6	2.486	431	434	436	rBV3	870	769	0.04%	0.005%
7	2.695	497	499	500	rBV	401	212	0.01%	0.001%
8	2.749	514	516	518	rBV2	825	362	0.02%	0.002%
9	2.810	533	535	539	rBV2	439	343	0.02%	0.002%
10	2.955	578	580	582	rBV	579	331	0.02%	0.002%
11	3.045	595	608	618	rBV8	3722	7810	0.42%	0.050%
12	3.109	625	628	632	rBV2	508	370	0.02%	0.002%
13	3.225	662	664	666	rBV	516	245	0.01%	0.002%
14	3.264	673	676	681	rVB2	354	288	0.02%	0.002%
15	3.306	685	689	693	rBV4	396	374	0.02%	0.002%
16	3.402	716	719	722	rBV5	510	366	0.02%	0.002%
17	3.444	729	732	734	rBV4	340	231	0.01%	0.001%
18	3.479	739	743	745	rBV2	407	314	0.02%	0.002%
19	3.502	745	750	753	rBV4	493	381	0.02%	0.002%
20	3.576	769	773	777	rBV4	575	470	0.03%	0.003%
21	3.611	781	784	788	rVB3	590	527	0.03%	0.003%
22	3.814	845	847	851	rVB2	441	210	0.01%	0.001%
23	3.852	855	859	862	rBV3	549	383	0.02%	0.002%
24	3.900	862	874	911	rBV2	119447	397139	21.58%	2.552%
25	4.354	999	1015	1041	rBV	302963	742276	40.33%	4.770%
26	4.579	1083	1085	1090	rBV3	551	367	0.02%	0.002%
27	4.614	1092	1096	1100	rBV6	998	912	0.05%	0.006%
28	4.836	1162	1165	1168	rBV3	500	446	0.02%	0.003%
29	4.875	1174	1177	1179	rBV	436	290	0.02%	0.002%
30	4.907	1184	1187	1189	rBV2	996	779	0.04%	0.005%
31	4.968	1204	1206	1208	rBV3	633	300	0.02%	0.002%
32	5.051	1215	1232	1259	rBV2	720169	1840676	100.00%	11.829%
33	5.479	1363	1365	1368	rBV2	797	474	0.03%	0.003%
34	5.621	1396	1409	1433	rVV	542970	1090099	59.22%	7.005%
35	5.865	1483	1485	1489	rBV4	573	337	0.02%	0.002%
36	5.910	1489	1499	1517	rBV2	24401	52431	2.85%	0.337%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011821\
 Data File : VW020049.D
 Acq On : 18 Jan 2021 17:28
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.074	1536	1550	1580	rBV	467881	945285	51.36%	6.075%
38	6.360	1637	1639	1642	rBV2	488	209	0.01%	0.001%
39	6.395	1647	1650	1653	rBV2	474	235	0.01%	0.002%
40	6.424	1657	1659	1665	rVB4	640	395	0.02%	0.003%
41	6.453	1665	1668	1669	rBV2	713	302	0.02%	0.002%
42	6.881	1798	1801	1803	rBV3	477	260	0.01%	0.002%
43	6.916	1806	1812	1813	rBV5	512	453	0.02%	0.003%
44	6.990	1823	1835	1857	rBV	263328	465293	25.28%	2.990%
45	7.321	1926	1938	1957	rBV	946520	1615878	87.79%	10.384%
46	7.627	2023	2033	2053	rBV2	163769	285449	15.51%	1.834%
47	7.987	2142	2145	2146	rVV	457	238	0.01%	0.002%
48	8.093	2168	2178	2211	rVV2	450178	863880	46.93%	5.552%
49	8.463	2291	2293	2299	rBV3	714	587	0.03%	0.004%
50	8.640	2346	2348	2351	rBV3	413	242	0.01%	0.002%
51	8.710	2368	2370	2371	rBV2	521	226	0.01%	0.001%
52	8.784	2389	2393	2397	rVB3	658	638	0.03%	0.004%
53	8.804	2397	2399	2403	rBV3	578	540	0.03%	0.003%
54	8.858	2403	2416	2452	rBV	946687	1536628	83.48%	9.875%
55	9.141	2500	2504	2505	rBV3	789	449	0.02%	0.003%
56	9.257	2537	2540	2543	rVB2	620	379	0.02%	0.002%
57	9.366	2570	2574	2578	rBV3	934	734	0.04%	0.005%
58	9.408	2585	2587	2591	rVB2	566	278	0.02%	0.002%
59	9.501	2613	2616	2618	rBV	437	285	0.02%	0.002%
60	9.543	2627	2629	2631	rBV2	791	420	0.02%	0.003%
61	9.672	2665	2669	2671	rBV	310	307	0.02%	0.002%
62	9.733	2686	2688	2690	rVV	523	289	0.02%	0.002%
63	9.781	2701	2703	2706	rBV	395	240	0.01%	0.002%
64	9.874	2730	2732	2736	rBV3	620	545	0.03%	0.004%
65	9.894	2736	2738	2742	rBV3	466	341	0.02%	0.002%
66	10.026	2776	2779	2782	rVB3	811	506	0.03%	0.003%
67	10.067	2788	2792	2794	rBV3	862	529	0.03%	0.003%
68	10.122	2807	2809	2813	rBV3	568	376	0.02%	0.002%
69	10.173	2823	2825	2828	rVB3	628	284	0.02%	0.002%
70	10.222	2828	2840	2862	rBV	516860	806058	43.79%	5.180%
71	10.376	2884	2888	2890	rBV2	826	535	0.03%	0.003%
72	10.389	2890	2892	2894	rVB	605	265	0.01%	0.002%
73	10.411	2894	2899	2901	rBV3	701	604	0.03%	0.004%
74	10.456	2908	2913	2914	rBV3	561	380	0.02%	0.002%
75	10.466	2914	2916	2920	rVB3	465	306	0.02%	0.002%
76	10.492	2920	2924	2926	rBV3	594	457	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020049.D
 Acq On : 18 Jan 2021 17:28
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.543	2937	2940	2941	rBV	456	297	0.02%	0.002%
78	10.698	2985	2988	2990	rBV	496	330	0.02%	0.002%
79	10.730	2994	2998	3000	rBV3	651	441	0.02%	0.003%
80	11.009	3082	3085	3086	rBV2	334	206	0.01%	0.001%
81	11.254	3150	3161	3182	rBV	1105856	1695304	92.10%	10.895%
82	11.553	3248	3254	3258	rBV5	6668	8763	0.48%	0.056%
83	11.630	3268	3278	3306	rVB	1065891	1689922	91.81%	10.860%
84	11.923	3360	3369	3373	rBV3	7201	11295	0.61%	0.073%
85	12.025	3394	3401	3409	rVB	13762	17640	0.96%	0.113%
86	12.421	3517	3524	3531	rBV3	9184	12280	0.67%	0.079%
87	12.472	3534	3540	3552	rVB	14551	22953	1.25%	0.148%
88	12.800	3638	3642	3645	rBV2	2698	2524	0.14%	0.016%
89	12.861	3652	3661	3665	rBV6	4271	7873	0.43%	0.051%
90	13.009	3701	3707	3719	rVB4	3862	6200	0.34%	0.040%
91	13.177	3752	3759	3767	rBV7	5018	6845	0.37%	0.044%
92	13.228	3767	3775	3782	rBV5	7655	11939	0.65%	0.077%
93	13.279	3785	3791	3798	rBV4	13245	19015	1.03%	0.122%
94	13.505	3859	3861	3862	rBV4	645	256	0.01%	0.002%
95	13.617	3894	3896	3900	rBV4	1209	715	0.04%	0.005%
96	13.730	3923	3931	3939	rBV4	3762	6283	0.34%	0.040%
97	13.919	3983	3990	4001	rBV4	8472	12889	0.70%	0.083%
98	14.099	4038	4046	4061	rVB7	7676	15493	0.84%	0.100%
99	14.154	4061	4063	4067	rBV3	922	578	0.03%	0.004%
100	14.247	4085	4092	4100	rVB4	3253	4637	0.25%	0.030%


Sum of corrected areas: 15560756

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020049.D
Acq On : 18 Jan 2021 17:28
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

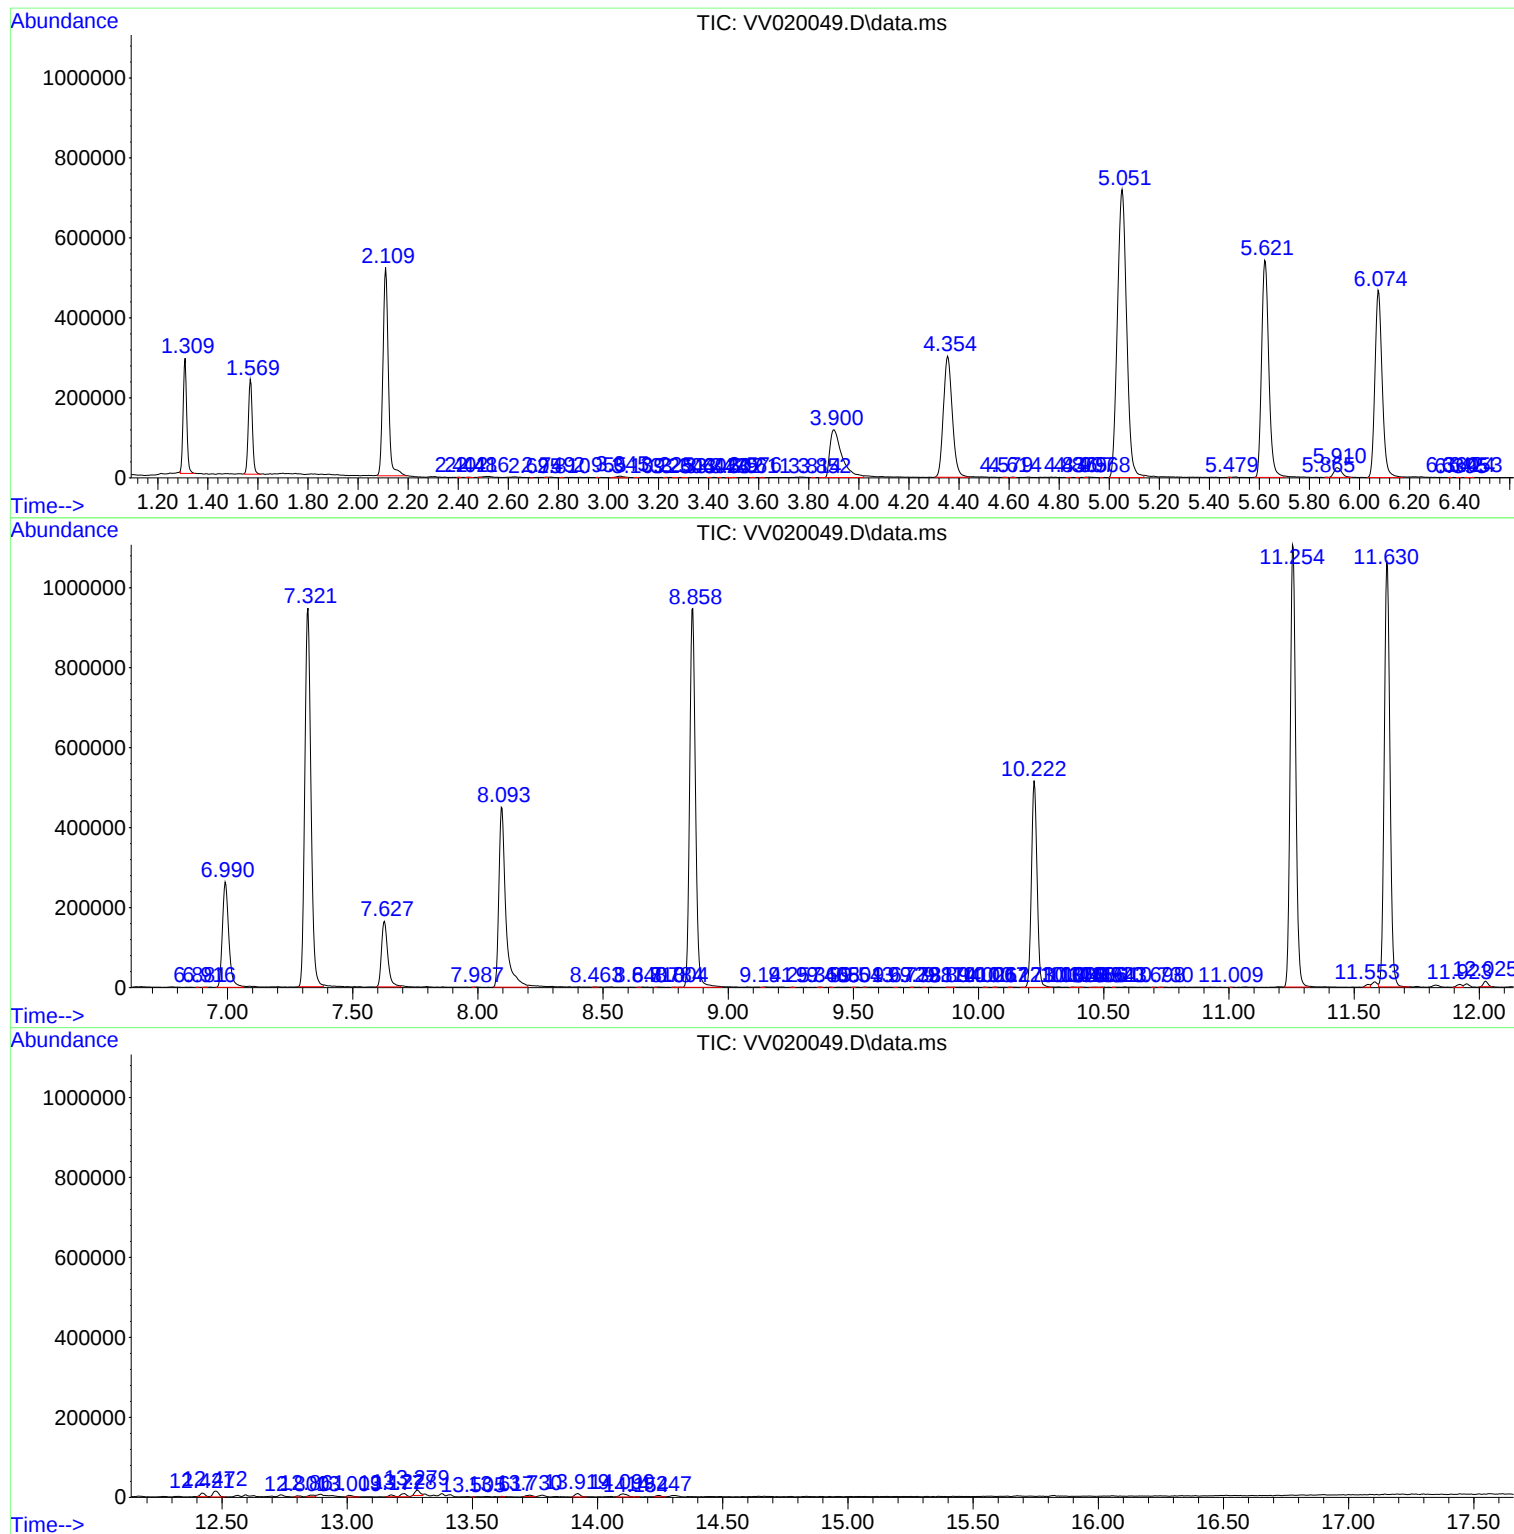

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020049.D
Acq On : 18 Jan 2021 17:28
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
Data File : VV020049.D
Acq On : 18 Jan 2021 17:28
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
