
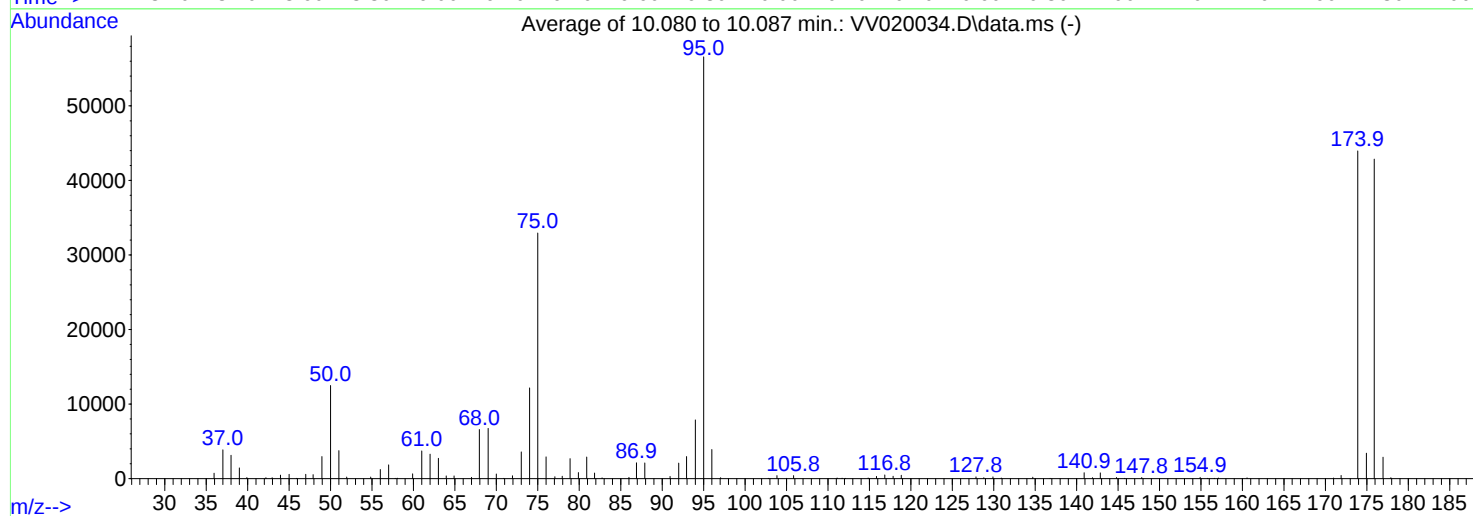


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011821\
 Data File : VV020034.D
 Acq On : 18 Jan 2021 09:39
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 20 01:05:37 2021

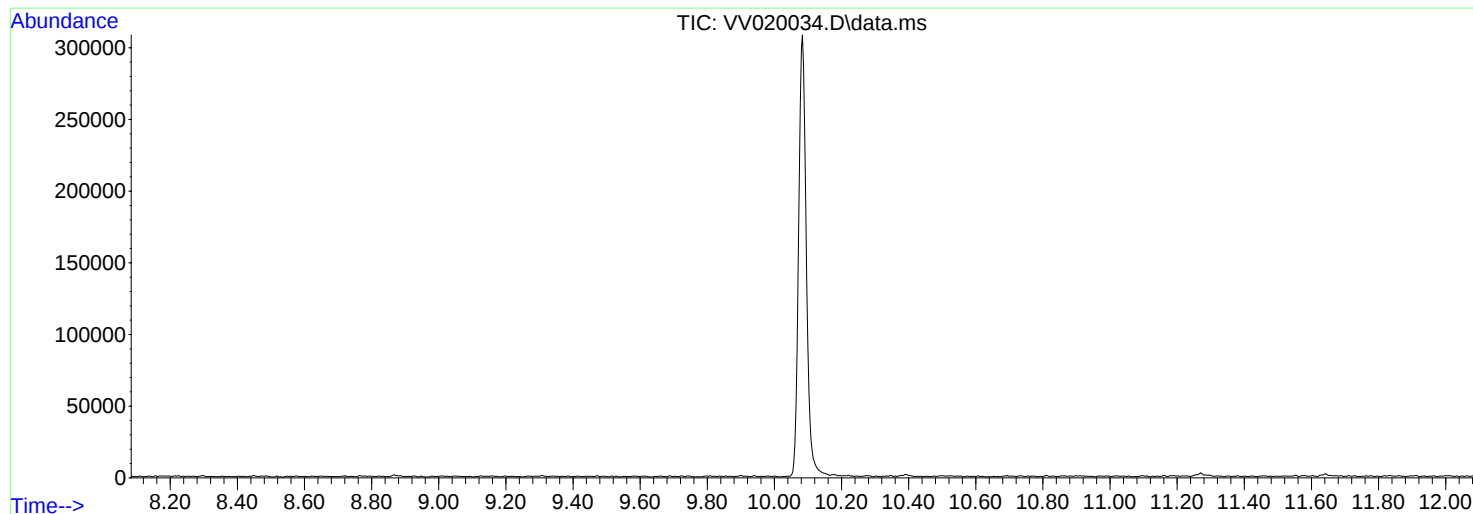

AutoFind: Scans 2796, 2797, 2798; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	12502	PASS
75	95	30	80	58.2	32955	PASS
95	95	100	100	100.0	56579	PASS
96	95	5	9	6.9	3905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.7	43947	PASS
175	174	5	9	7.8	3408	PASS
176	174	95	101	97.5	42856	PASS
177	176	5	9	6.7	2876	PASS

m/z	Abundance
35.70	132.0
38.40	103.0
39.80	232.0
41.10	136.0
44.00	548.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	772.0
37.00	4049.0
38.00	3320.0
39.00	1492.0
40.00	356.0
42.20	122.0
43.10	161.0
44.00	989.0
45.00	594.0
47.00	549.0
47.90	527.0
49.00	3128.0
50.00	12596.0
51.00	3953.0
52.00	221.0
54.90	232.0
56.00	1355.0
57.00	1823.0
57.80	118.0
59.90	701.0
61.00	3656.0
62.00	3375.0
63.00	2725.0
64.10	267.0
64.90	375.0
67.00	182.0
68.00	6637.0
69.00	6545.0
70.00	671.0
71.90	442.0
73.00	3627.0
74.00	12437.0
75.00	33104.0
76.00	3052.0
77.00	265.0
78.00	309.0
78.90	2714.0
79.90	807.0
80.90	3033.0
81.90	819.0
82.70	112.0
86.00	237.0
86.90	2022.0
87.90	1994.0
90.90	307.0
92.00	2135.0
93.00	2961.0
94.00	7721.0
95.00	57496.0
96.00	4079.0
97.10	127.0
103.90	420.0
105.00	101.0
105.80	415.0
111.10	144.0
111.70	102.0
115.80	326.0
116.90	510.0
117.90	321.0
118.80	413.0
127.80	229.0
128.80	101.0
129.90	258.0
134.70	133.0
140.90	755.0
141.90	127.0
142.90	749.0
144.80	155.0
145.80	105.0
147.90	160.0
154.90	222.0
156.60	137.0
160.60	111.0
171.90	440.0
173.90	42848.0
174.90	3302.0
175.90	42608.0
177.00	2944.0
177.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	767.0
37.00	4050.0
38.00	3234.0
39.00	1512.0
40.00	391.0
42.20	135.0
42.90	125.0
43.90	1041.0
45.00	583.0
47.00	605.0
47.90	575.0
48.90	3094.0
50.00	12905.0
51.00	3851.0
52.00	240.0
54.80	223.0
56.00	1269.0
57.00	1906.0
58.10	111.0
59.90	665.0
61.00	3837.0
62.00	3414.0
63.00	2840.0
63.90	374.0
64.90	378.0
67.00	192.0
68.00	6831.0
69.00	7069.0
70.00	606.0
70.90	103.0
71.90	386.0
73.00	3769.0
74.00	12587.0
75.00	34304.0
76.00	3005.0
77.10	261.0
77.90	369.0
78.90	2779.0
79.90	838.0
80.90	2945.0
81.90	734.0
82.80	123.0
86.00	164.0
86.90	2165.0
87.90	2168.0
91.00	303.0
92.00	2133.0
92.90	3041.0
94.00	8216.0
95.00	58408.0
96.00	4015.0
97.10	138.0
103.80	416.0
105.80	422.0
111.10	118.0
111.70	108.0
114.90	121.0
115.80	316.0
116.80	489.0
117.80	327.0
118.80	490.0
127.80	257.0
128.80	144.0
129.90	248.0
130.90	114.0
134.70	204.0
140.90	826.0
141.90	129.0
142.80	794.0
144.80	144.0
147.90	151.0
154.90	191.0
157.10	137.0
160.50	125.0
171.10	119.0
171.90	454.0
173.90	45336.0
175.00	3571.0
175.90	44232.0
177.00	3016.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	671.0
37.00	3526.0
38.00	2842.0
39.00	1303.0
40.00	393.0
40.90	101.0
42.20	138.0
42.90	106.0
43.90	1009.0
45.00	562.0
45.90	115.0
47.00	608.0
47.90	507.0
48.90	2674.0
50.00	12005.0
51.00	3487.0
51.90	215.0
54.90	189.0
56.00	1046.0
57.00	1806.0
58.00	101.0
59.90	571.0
61.00	3671.0
62.00	3073.0
63.00	2629.0
63.90	441.0
64.90	352.0
67.00	153.0
67.90	6315.0
69.00	6589.0
70.00	570.0
72.00	306.0
73.00	3373.0
74.00	11513.0
75.00	31456.0
76.00	2708.0
77.00	255.0
77.90	313.0
78.90	2592.0
79.90	785.0
80.90	2693.0
81.80	682.0
82.80	105.0
86.00	102.0
86.90	2165.0
87.90	2166.0
91.00	281.0
92.00	1967.0
92.90	2899.0
94.00	7668.0
95.00	53832.0
96.00	3622.0
97.00	135.0
102.80	129.0
103.80	395.0
105.90	398.0
112.10	110.0
114.80	129.0
115.90	265.0
116.80	462.0
117.80	294.0
118.90	464.0
127.90	247.0
128.80	143.0
129.90	209.0
130.90	122.0
134.70	234.0
136.80	126.0
140.90	799.0
141.90	111.0
142.80	793.0
144.80	130.0
147.80	125.0
154.90	126.0
155.80	121.0
157.10	130.0
160.50	119.0
170.90	108.0
171.90	404.0
173.90	43656.0
175.00	3350.0
175.90	41728.0
176.90	2668.0
178.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82