


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011823\
Data File : VV029888.D
Acq On : 18 Jan 2023 09:53
Operator : SY/MD
Sample : BFB361
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB361

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011823WMA.M
Title : VOC Analysis
Last Update : Thu Jan 19 00:40:29 2023

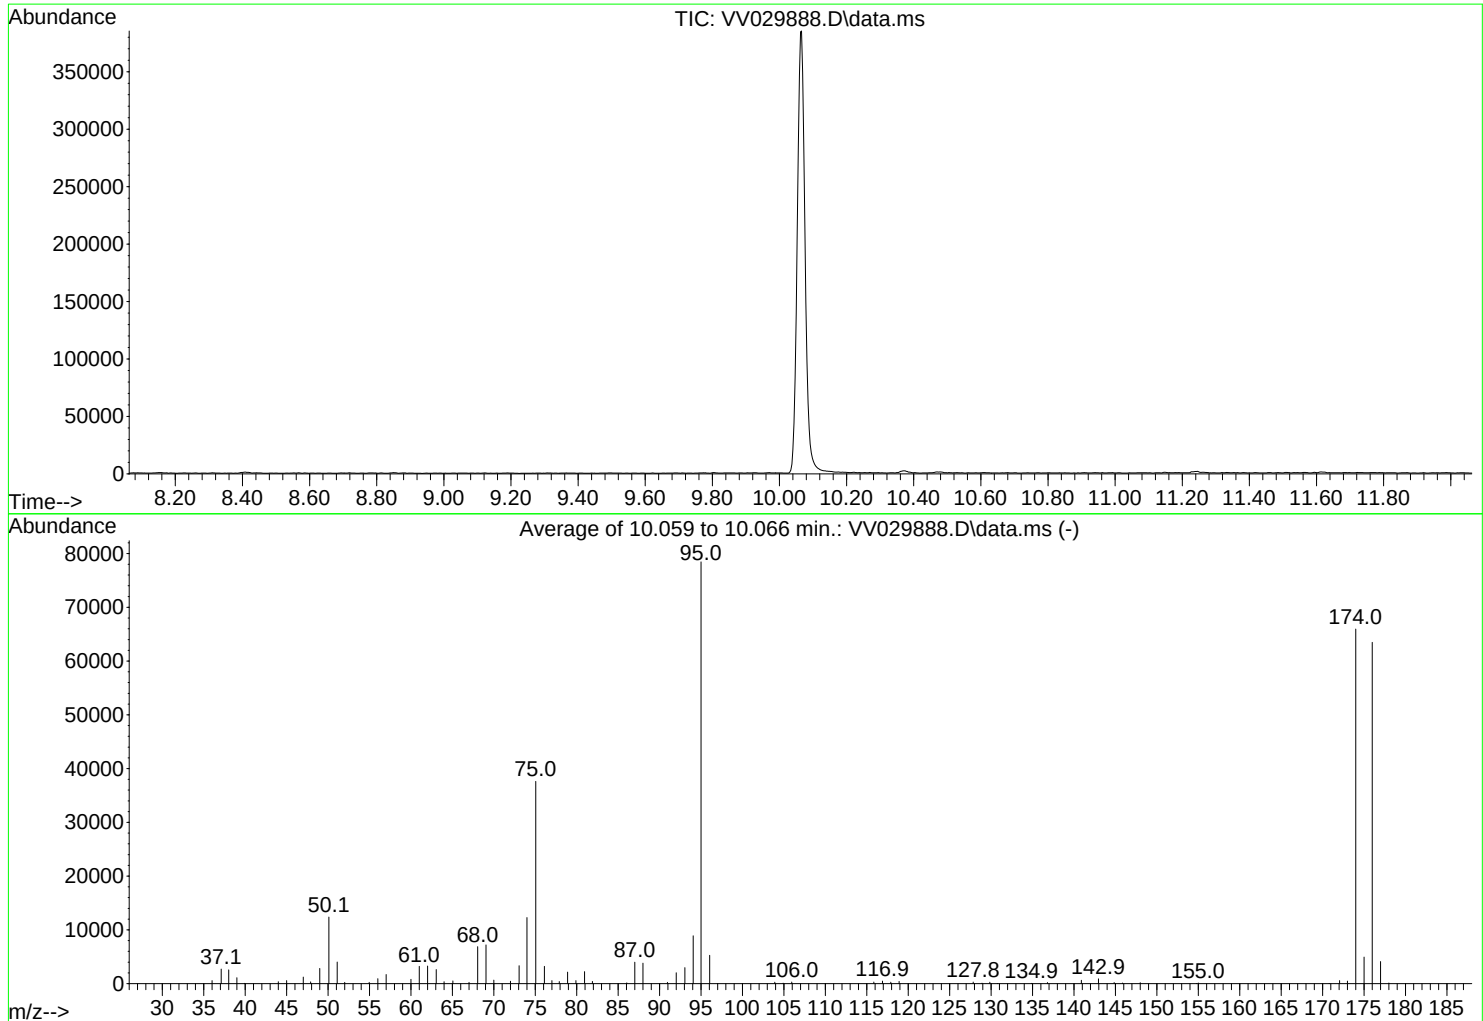

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	12377	PASS
75	95	30	80	48.0	37635	PASS
95	95	100	100	100.0	78453	PASS
96	95	5	9	6.7	5261	PASS
173	174	0.00	2	0.7	465	PASS
174	95	50	120	84.1	65944	PASS
175	174	5	9	7.5	4953	PASS
176	174	95	105	96.3	63488	PASS
177	176	5	10	6.5	4113	PASS

m/z	Abundance
40.00	309.0
44.00	422.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	582.0
37.10	2650.0
38.00	2545.0
39.00	1106.0
39.90	362.0
44.00	738.0
45.00	602.0
47.00	1171.0
47.90	329.0
49.00	2730.0
50.10	11806.0
51.10	3970.0
52.00	213.0
54.90	255.0
56.00	811.0
57.00	1627.0
60.00	769.0
61.00	3106.0
62.00	3130.0
63.10	2579.0
64.00	331.0
65.10	475.0
67.00	223.0
68.10	6524.0
69.00	6931.0
70.00	590.0
72.00	393.0
73.10	3248.0
74.00	11753.0
75.00	35128.0
76.10	3002.0
77.00	574.0
77.90	365.0
78.90	2079.0
79.90	480.0
80.90	2213.0
81.90	433.0
86.00	171.0
87.00	3807.0
88.00	3481.0
91.00	236.0
92.00	1861.0
93.00	2889.0
94.10	8331.0
95.00	73632.0
96.10	5145.0
103.90	241.0
105.90	300.0
115.90	272.0
116.90	472.0
117.90	224.0
118.90	353.0
127.80	279.0
129.90	264.0
136.80	178.0
140.80	521.0
142.90	882.0
144.80	204.0
145.90	101.0
148.00	167.0
154.80	121.0
172.00	544.0
173.00	660.0
174.00	60208.0
175.00	4540.0
176.00	57048.0
177.00	3865.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	602.0
37.10	2773.0
38.00	2611.0
39.00	1126.0
39.90	398.0
44.00	799.0
45.00	603.0
47.00	1274.0
47.90	341.0
49.00	2937.0
50.10	12823.0
51.10	4164.0
52.00	258.0
55.00	239.0
56.00	968.0
57.00	1725.0
60.00	836.0
61.00	3285.0
62.00	3367.0
63.10	2711.0
64.00	367.0
65.00	505.0
67.00	254.0
68.00	7060.0
69.10	7477.0
70.00	681.0
72.00	441.0
73.10	3489.0
74.00	12726.0
75.00	38960.0
76.10	3307.0
77.00	583.0
77.90	392.0
78.90	2222.0
79.90	622.0
80.90	2302.0
81.90	455.0
86.00	160.0
87.00	4109.0
88.00	3963.0
90.90	250.0
92.00	2059.0
93.10	3019.0
94.10	9264.0
95.00	81128.0
96.00	5403.0
103.90	285.0
104.90	123.0
106.00	317.0
115.80	306.0
116.90	495.0
117.90	280.0
118.90	429.0
127.80	304.0
128.90	110.0
129.80	276.0
134.90	106.0
136.80	216.0
140.90	614.0
142.90	975.0
144.90	224.0
145.80	138.0
148.00	185.0
155.00	151.0
172.10	600.0
173.00	736.0
174.00	67912.0
175.00	5122.0
176.00	65584.0
177.00	4186.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	548.0
37.10	2678.0
38.00	2511.0
39.00	1099.0
39.90	384.0
44.00	783.0
45.00	521.0
47.00	1181.0
47.90	339.0
49.00	2862.0
50.10	12502.0
51.10	3915.0
52.00	233.0
55.00	209.0
56.00	1014.0
57.00	1720.0
60.00	796.0
61.00	3254.0
62.00	3317.0
63.00	2546.0
64.00	389.0
65.00	500.0
67.00	265.0
68.00	7026.0
69.10	7188.0
70.00	685.0
72.00	485.0
73.00	3283.0
74.00	12414.0
75.10	38816.0
76.10	3323.0
77.00	561.0
77.90	391.0
78.90	2144.0
79.90	642.0
81.00	2191.0
81.90	417.0
86.10	144.0
87.00	4039.0
88.00	3999.0
90.90	276.0
92.00	2130.0
93.10	3004.0
94.00	9127.0
95.00	80600.0
96.00	5234.0
97.00	124.0
103.90	293.0
104.90	150.0
106.00	321.0
115.80	315.0
116.90	489.0
117.90	306.0
118.90	446.0
127.90	297.0
128.90	134.0
129.90	282.0
130.80	101.0
134.90	117.0
136.80	212.0
141.00	715.0
143.00	874.0
144.90	209.0
145.80	161.0
148.00	165.0
155.00	205.0
170.80	120.0
172.00	604.0
174.00	69712.0
175.00	5198.0
176.00	67832.0
177.00	4287.0
178.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361