

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011824\
 Data File : VV033732.D
 Acq On : 18 Jan 2024 11:44
 Operator : SY/MD
 Sample : P1121-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jan 19 00:09:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 19 00:08:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	110572	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	99686	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	49376	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	36999	6.119	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	122.400%
7) Chloroethane-d5	1.536	69	29804	5.558	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.200%
11) 1,1-Dichloroethene-d2	2.060	65	16434	6.031	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	120.600%
20) 2-Butanone-d5	3.838	46	45315	30.653	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	61.300%
24) Chloroform-d	4.253	84	61051	4.669	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	4.947	65	27584	4.705	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	4.960	84	128000	5.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.400%
36) 1,2-Dichloropropane-d6	5.989	67	35845	4.470	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.243	98	119027	5.543	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
43) trans-1,3-Dichloroprop...	7.561	79	12851	4.635	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.800%
46) 2-Hexanone-d5	8.034	63	37829	34.754	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.500%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	18716	3.994	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	36222	4.778	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	2571	0.280	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011824\
Data File : VV033732.D
Acq On : 18 Jan 2024 11:44
Operator : SY/MD
Sample : P1121-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jan 19 00:09:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 19 00:08:23 2024
Response via : Initial Calibration

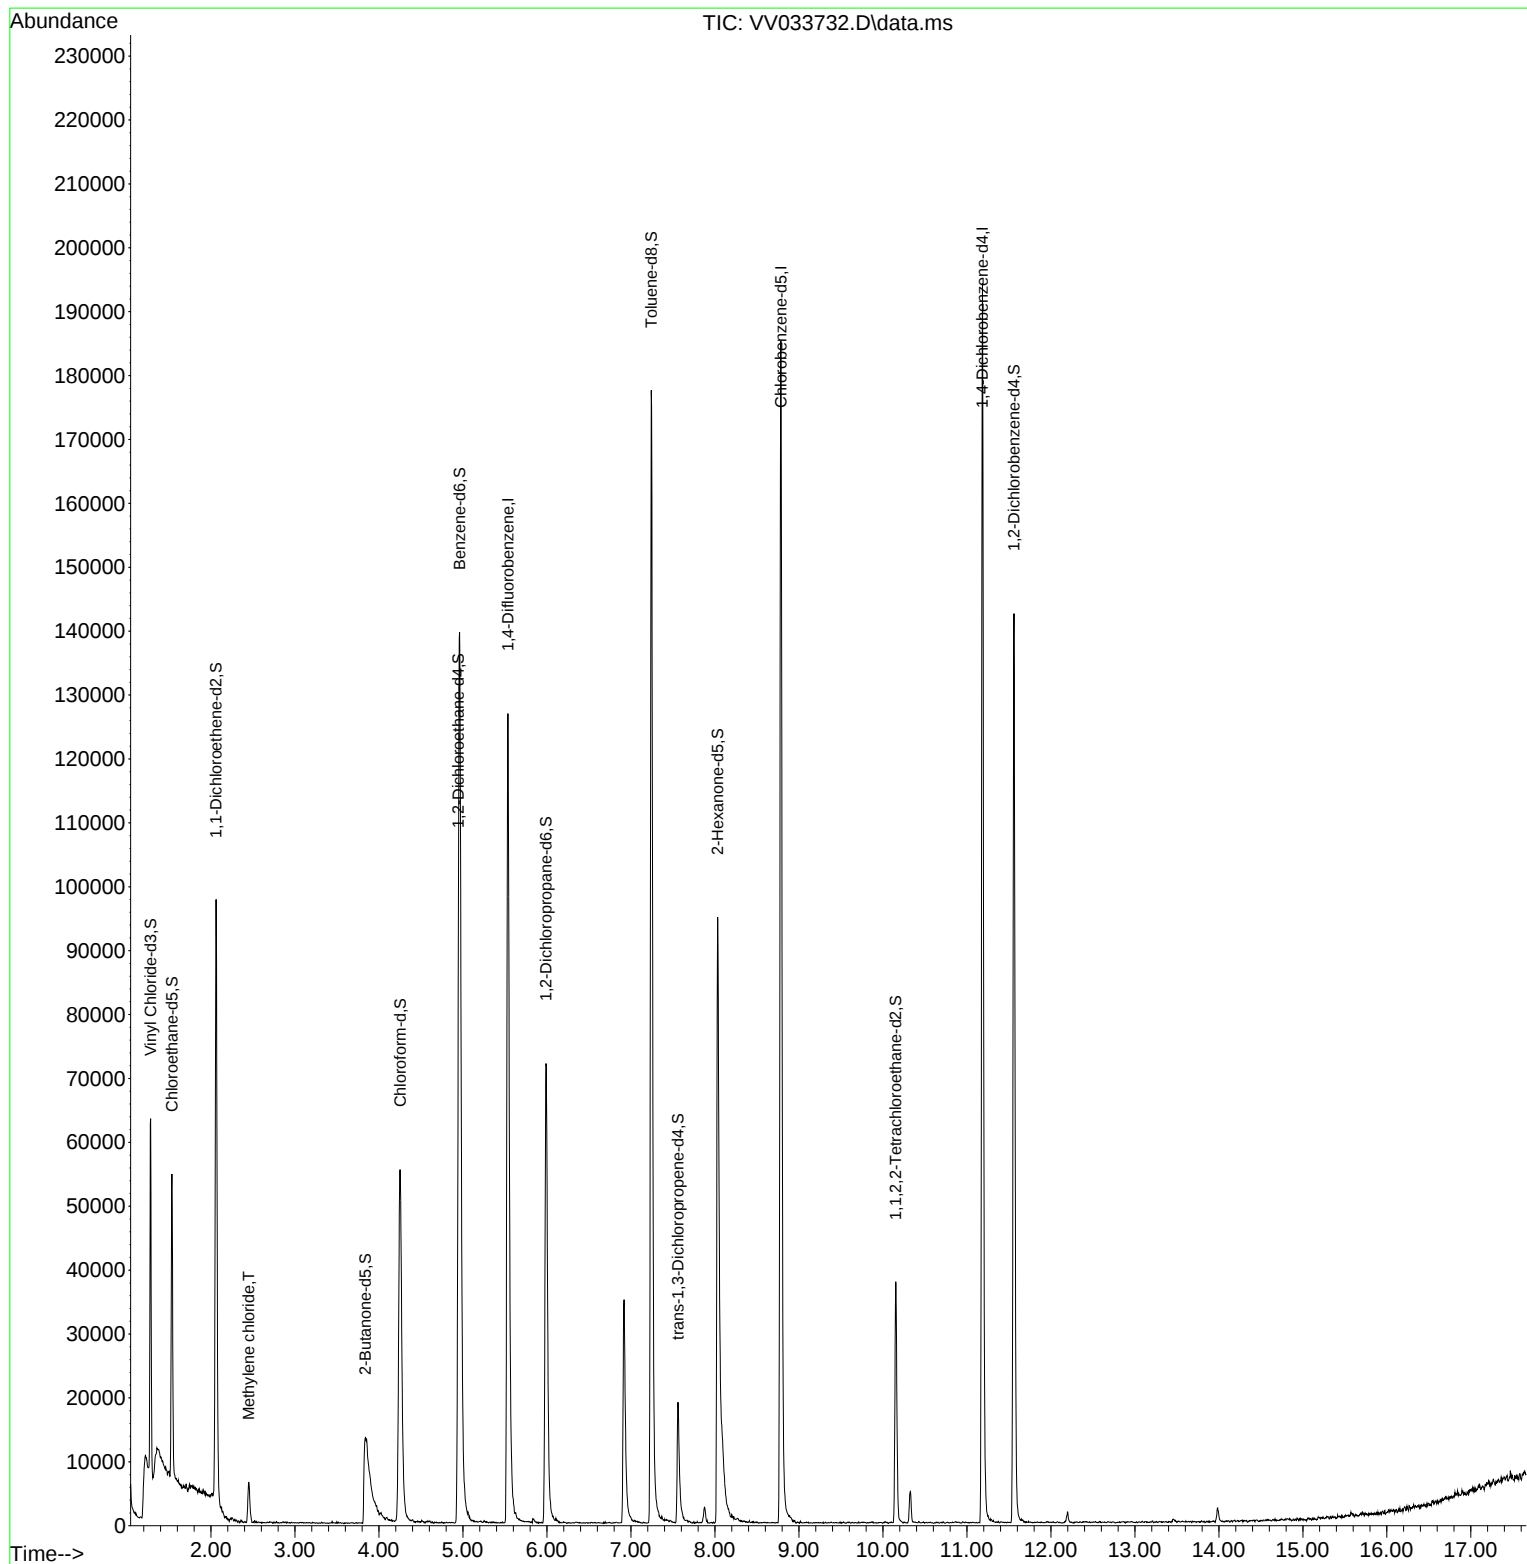

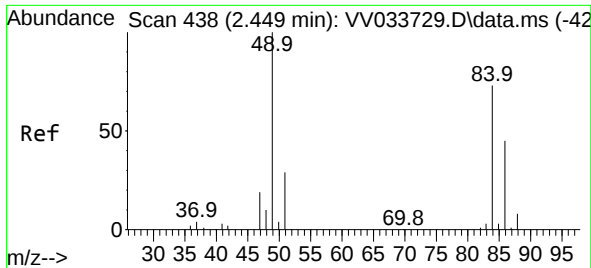

#16
Methylene chloride
Concen: 0.280 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV033732.D
Acq: 18 Jan 2024 11:44

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

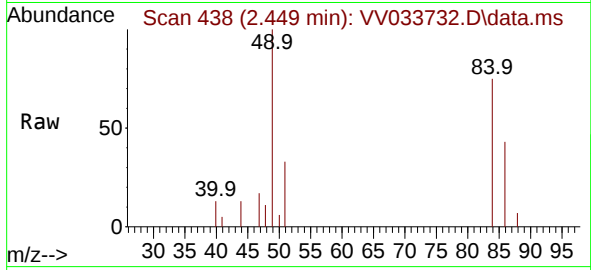

Tgt Ion:	84	Resp:	2571
Ion	Ratio	Lower	Upper
84	100		
86	57.4	45.5	84.5
49	133.0	100.3	186.3

