
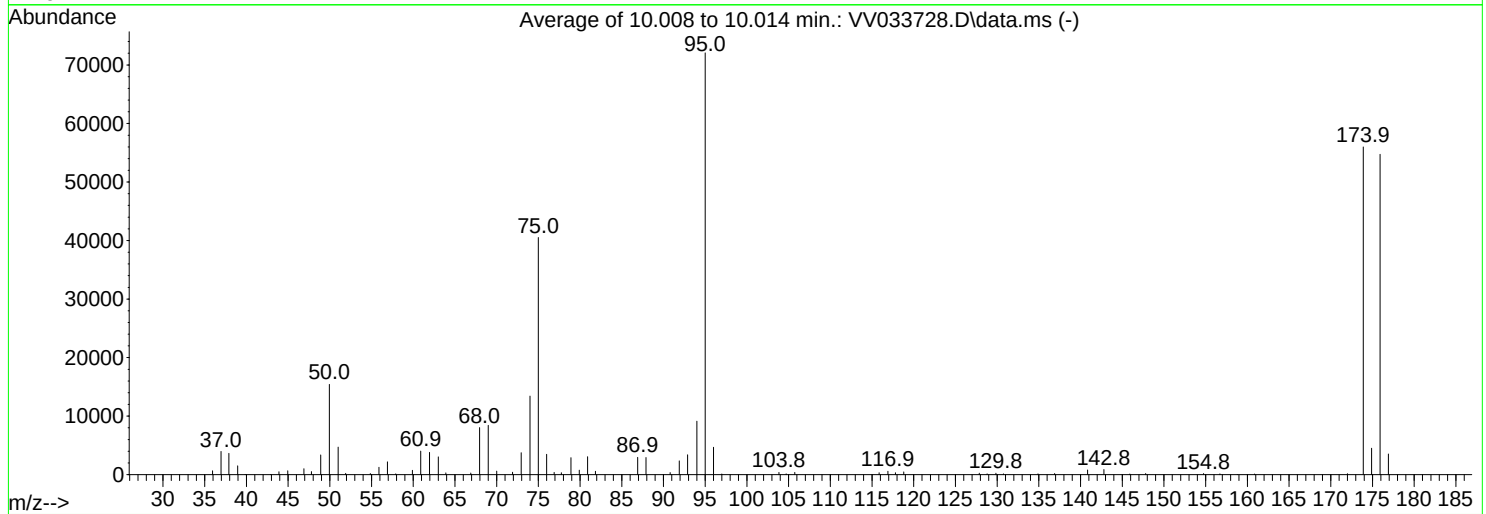


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011824\
Data File : VV033728.D
Acq On : 18 Jan 2024 09:22
Operator : SY/MD
Sample : BFB241
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB241

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 19 00:08:23 2024

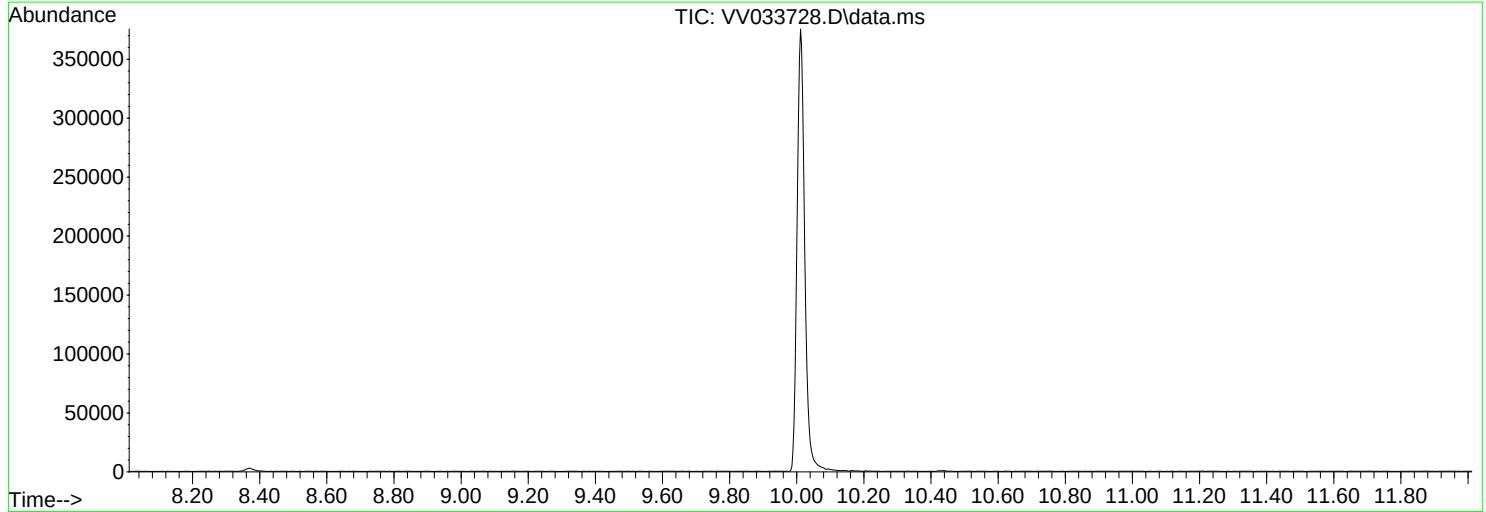

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	15433	PASS
75	95	30	80	56.2	40512	PASS
95	95	100	100	100.0	72072	PASS
96	95	5	9	6.5	4678	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.7	55981	PASS
175	174	5	9	8.1	4524	PASS
176	174	95	105	97.8	54728	PASS
177	176	5	10	6.4	3518	PASS

m/z	Abundance
39.90	323.0
43.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.90	693.0
37.00	3905.0
37.90	3631.0
38.90	1521.0
39.90	334.0
43.90	694.0
45.00	602.0
46.90	926.0
47.80	497.0
48.90	3527.0
50.00	15296.0
51.00	4747.0
51.90	204.0
54.80	184.0
55.90	1230.0
56.90	2149.0
57.90	124.0
59.90	760.0
60.90	3765.0
62.00	3640.0
63.00	3037.0
63.90	304.0
66.90	267.0
67.90	7804.0
69.00	8246.0
70.00	679.0
71.90	406.0
72.90	3621.0
74.00	13264.0
75.00	39360.0
76.00	3343.0
76.90	354.0
77.70	321.0
78.90	2731.0
79.90	772.0
80.90	2911.0
81.80	586.0
86.90	2990.0
87.90	2828.0
90.80	383.0
91.90	2253.0
92.90	3279.0
94.00	9073.0
95.00	69800.0
96.00	4747.0
97.00	128.0
103.80	426.0
104.70	110.0
105.70	373.0
115.80	310.0
116.90	573.0
117.80	354.0
118.80	476.0
127.90	236.0
128.80	116.0
129.80	244.0
130.70	125.0
134.90	130.0
136.90	169.0
140.90	731.0
142.80	815.0
145.90	106.0
147.80	180.0
154.70	204.0
156.70	149.0
160.90	116.0
173.90	52784.0
174.90	4429.0
175.90	51376.0
176.90	3385.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	662.0
37.00	4099.0
37.90	3769.0
38.90	1568.0
39.90	363.0
43.90	703.0
44.90	661.0
46.90	1041.0
47.80	544.0
48.90	3498.0
50.00	15972.0
51.00	4875.0
51.90	214.0
54.80	193.0
55.90	1347.0
56.90	2243.0
57.90	141.0
59.90	774.0
60.90	4150.0
62.00	3957.0
63.00	3129.0
63.90	321.0
66.90	290.0
67.90	8286.0
69.00	8779.0
70.00	613.0
71.90	438.0
73.00	3893.0
74.00	14044.0
75.00	41960.0
76.00	3619.0
76.90	405.0
77.80	354.0
78.90	3009.0
79.90	785.0
80.90	3184.0
81.90	621.0
86.90	3080.0
87.90	3042.0
90.80	382.0
91.90	2412.0
92.90	3522.0
94.00	9490.0
95.00	74560.0
96.00	4837.0
97.00	129.0
103.90	391.0
104.70	136.0
105.80	395.0
115.90	336.0
116.90	616.0
117.80	352.0
118.80	499.0
127.80	259.0
128.80	130.0
129.80	268.0
130.70	127.0
134.90	151.0
136.90	196.0
140.90	817.0
142.80	920.0
145.90	116.0
147.80	196.0
154.80	179.0
156.70	151.0
158.80	105.0
160.90	113.0
172.00	242.0
173.90	57984.0
174.90	4741.0
175.90	56640.0
176.90	3624.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.90	624.0
36.90	3880.0
37.90	3482.0
39.00	1420.0
39.80	375.0
42.90	104.0
43.90	658.0
44.90	698.0
46.90	1034.0
47.80	549.0
48.90	3105.0
49.90	15030.0
51.00	4526.0
51.90	210.0
54.90	170.0
55.90	1239.0
56.90	2147.0
57.90	133.0
59.90	705.0
60.90	4111.0
61.90	3818.0
63.00	2923.0
63.90	320.0
66.90	281.0
68.00	8035.0
69.00	8263.0
70.00	547.0
71.90	437.0
73.00	3697.0
74.00	13002.0
75.00	40216.0
76.00	3468.0
76.90	415.0
77.80	327.0
78.90	2977.0
79.90	779.0
80.90	3082.0
81.90	566.0
86.90	2827.0
87.90	2891.0
90.80	334.0
91.90	2356.0
92.90	3385.0
94.00	8855.0
95.00	71856.0
96.00	4451.0
97.00	112.0
103.90	364.0
104.70	141.0
105.80	405.0
115.90	314.0
116.90	548.0
117.80	292.0
118.80	425.0
127.80	276.0
128.80	145.0
129.90	267.0
130.80	119.0
134.90	170.0
136.90	192.0
140.80	852.0
142.80	917.0
145.90	124.0
147.80	187.0
154.80	162.0
156.70	132.0
160.80	113.0
172.00	241.0
173.90	57176.0
174.90	4402.0
175.90	56168.0
176.90	3545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241