
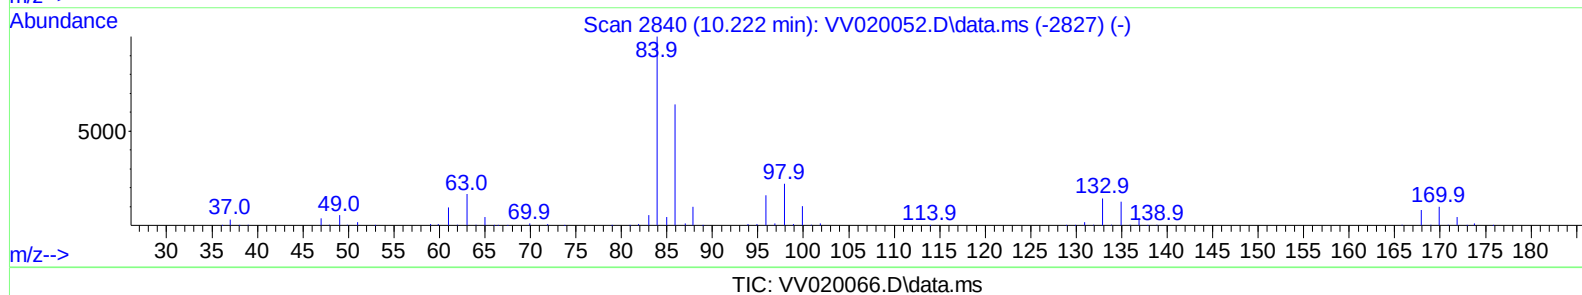
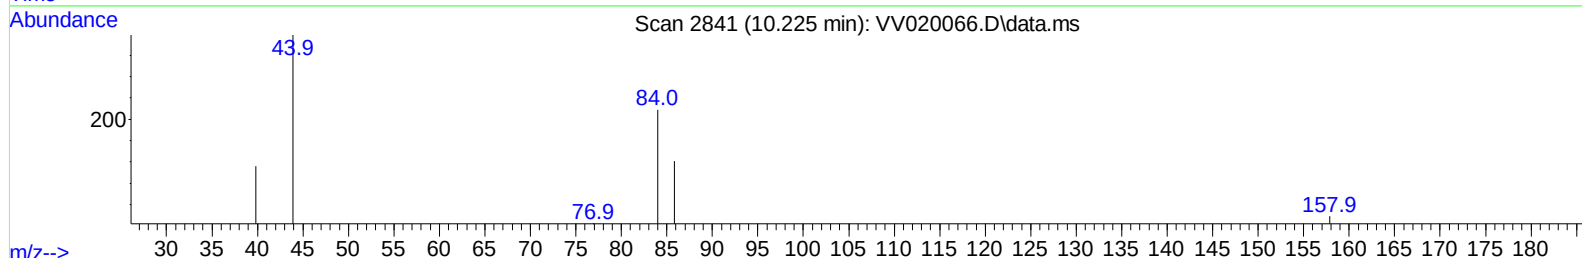


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020066.D
Acq On : 19 Jan 2021 21:51
Operator : SY/MD
Sample : M1173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jan 20 01:12:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 20 01:05:37 2021
Response via : Initial Calibration

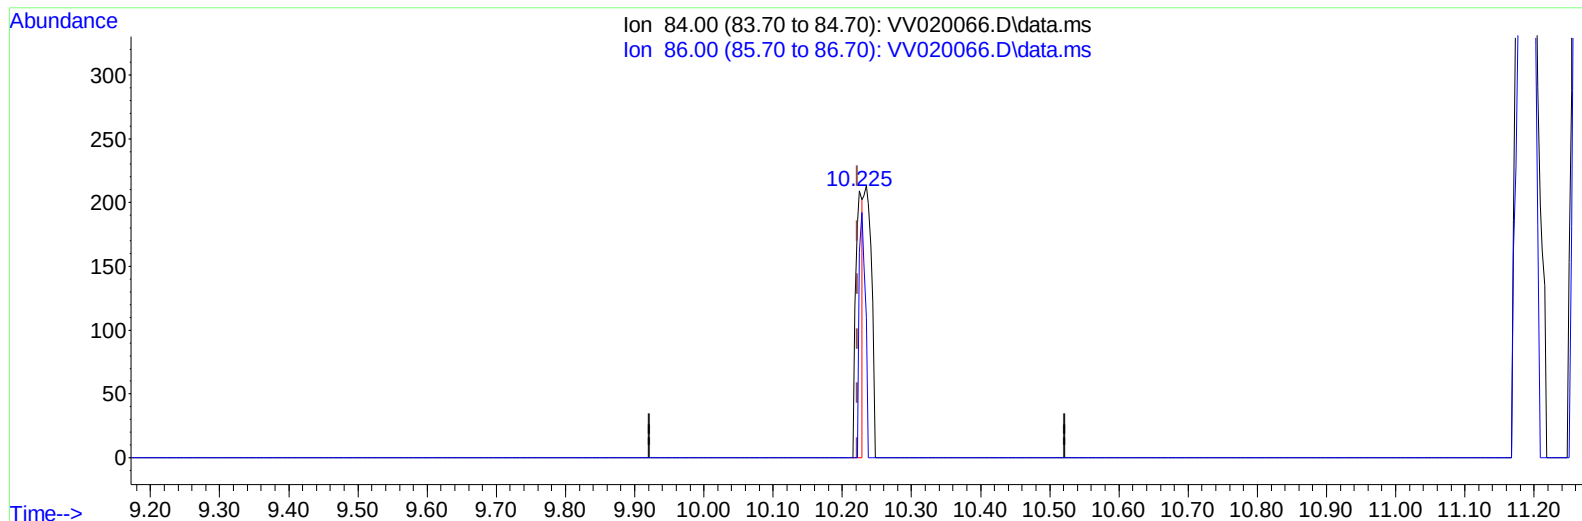

(57) 1,1,2,2-Tetrachloroethane-d2 (S)

10.225min (+ 0.003) 9.29 ug/L

response 138

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	86.23#
0.00	0.00	0.00
0.00	0.00	0.00