
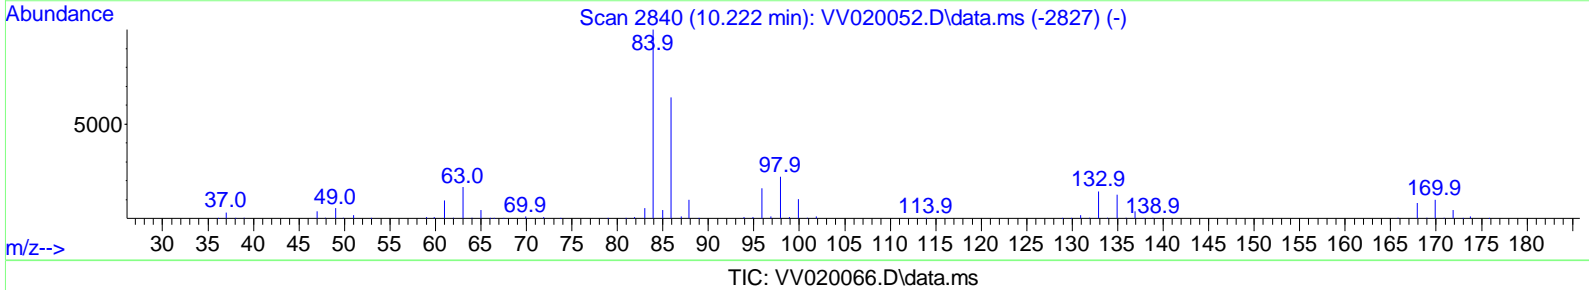
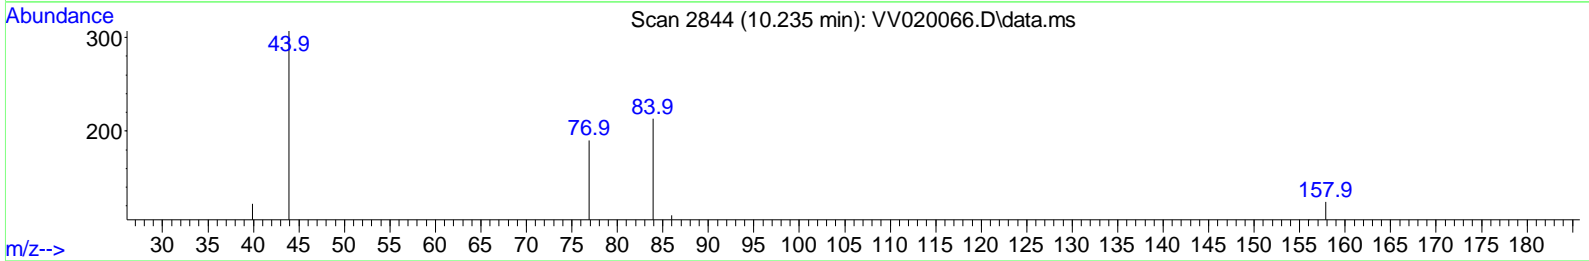


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020066.D
 Acq On : 19 Jan 2021 21:51
 Operator : SY/MD
 Sample : M1173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jan 20 01:12:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 20 01:05:37 2021
 Response via : Initial Calibration

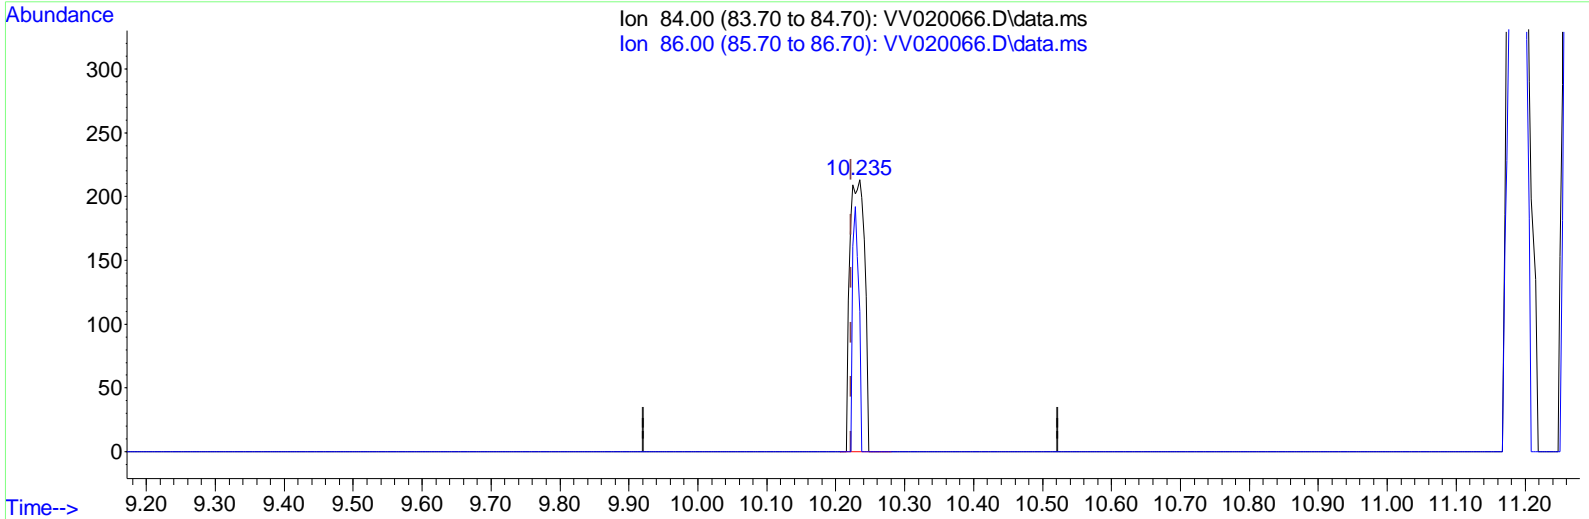

(57) 1,1,2,2-Tetrachloroethane-d2 (S)

10.235min (+ 0.013) 21.00 ug/L m

response 312

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.40	38.14#
0.00	0.00	0.00
0.00	0.00	0.00