

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020054.D
 Acq On : 19 Jan 2021 16:14
 Operator : SY/MD
 Sample : VV0119WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK82

Quant Time: Jan 20 01:10:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 20 01:05:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	381853	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	453986	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	220621	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	159350	49.47	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.94%	
7) Chloroethane-d5	1.570	69	131825	51.27	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.54%	
11) 1,1-Dichloroethene-d2	2.110	63	217209	34.24	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.48%	
21) 2-Butanone-d5	3.897	46	232718	111.38	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	111.38%	
24) Chloroform-d	4.354	84	278134	47.94	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.88%	
26) 1,2-Dichloroethane-d4	5.036	65	202648	51.38	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.76%	
32) Benzene-d6	5.055	84	525668	41.03	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.06%	
36) 1,2-Dichloropropane-d6	6.074	67	165851	41.46	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	82.92%	
41) Toluene-d8	7.322	98	512994	44.17	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.34%	
43) trans-1,3-Dichloroprop...	7.624	79	77767	37.46	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	74.92%	
47) 2-Hexanone-d5	8.093	63	139231	86.81	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.81%	
57) 1,1,2,2-Tetrachloroeth...	10.222	84	224138	41.44	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	82.88%	
64) 1,2-Dichlorobenzene-d4	11.630	152	219286	51.46	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.92%	
Target Compounds						
48) 2-Hexanone	8.148	43	12985	3.14	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020054.D
Acq On : 19 Jan 2021 16:14
Operator : SY/MD
Sample : VV0119WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK82

Quant Time: Jan 20 01:10:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 20 01:05:37 2021
Response via : Initial Calibration

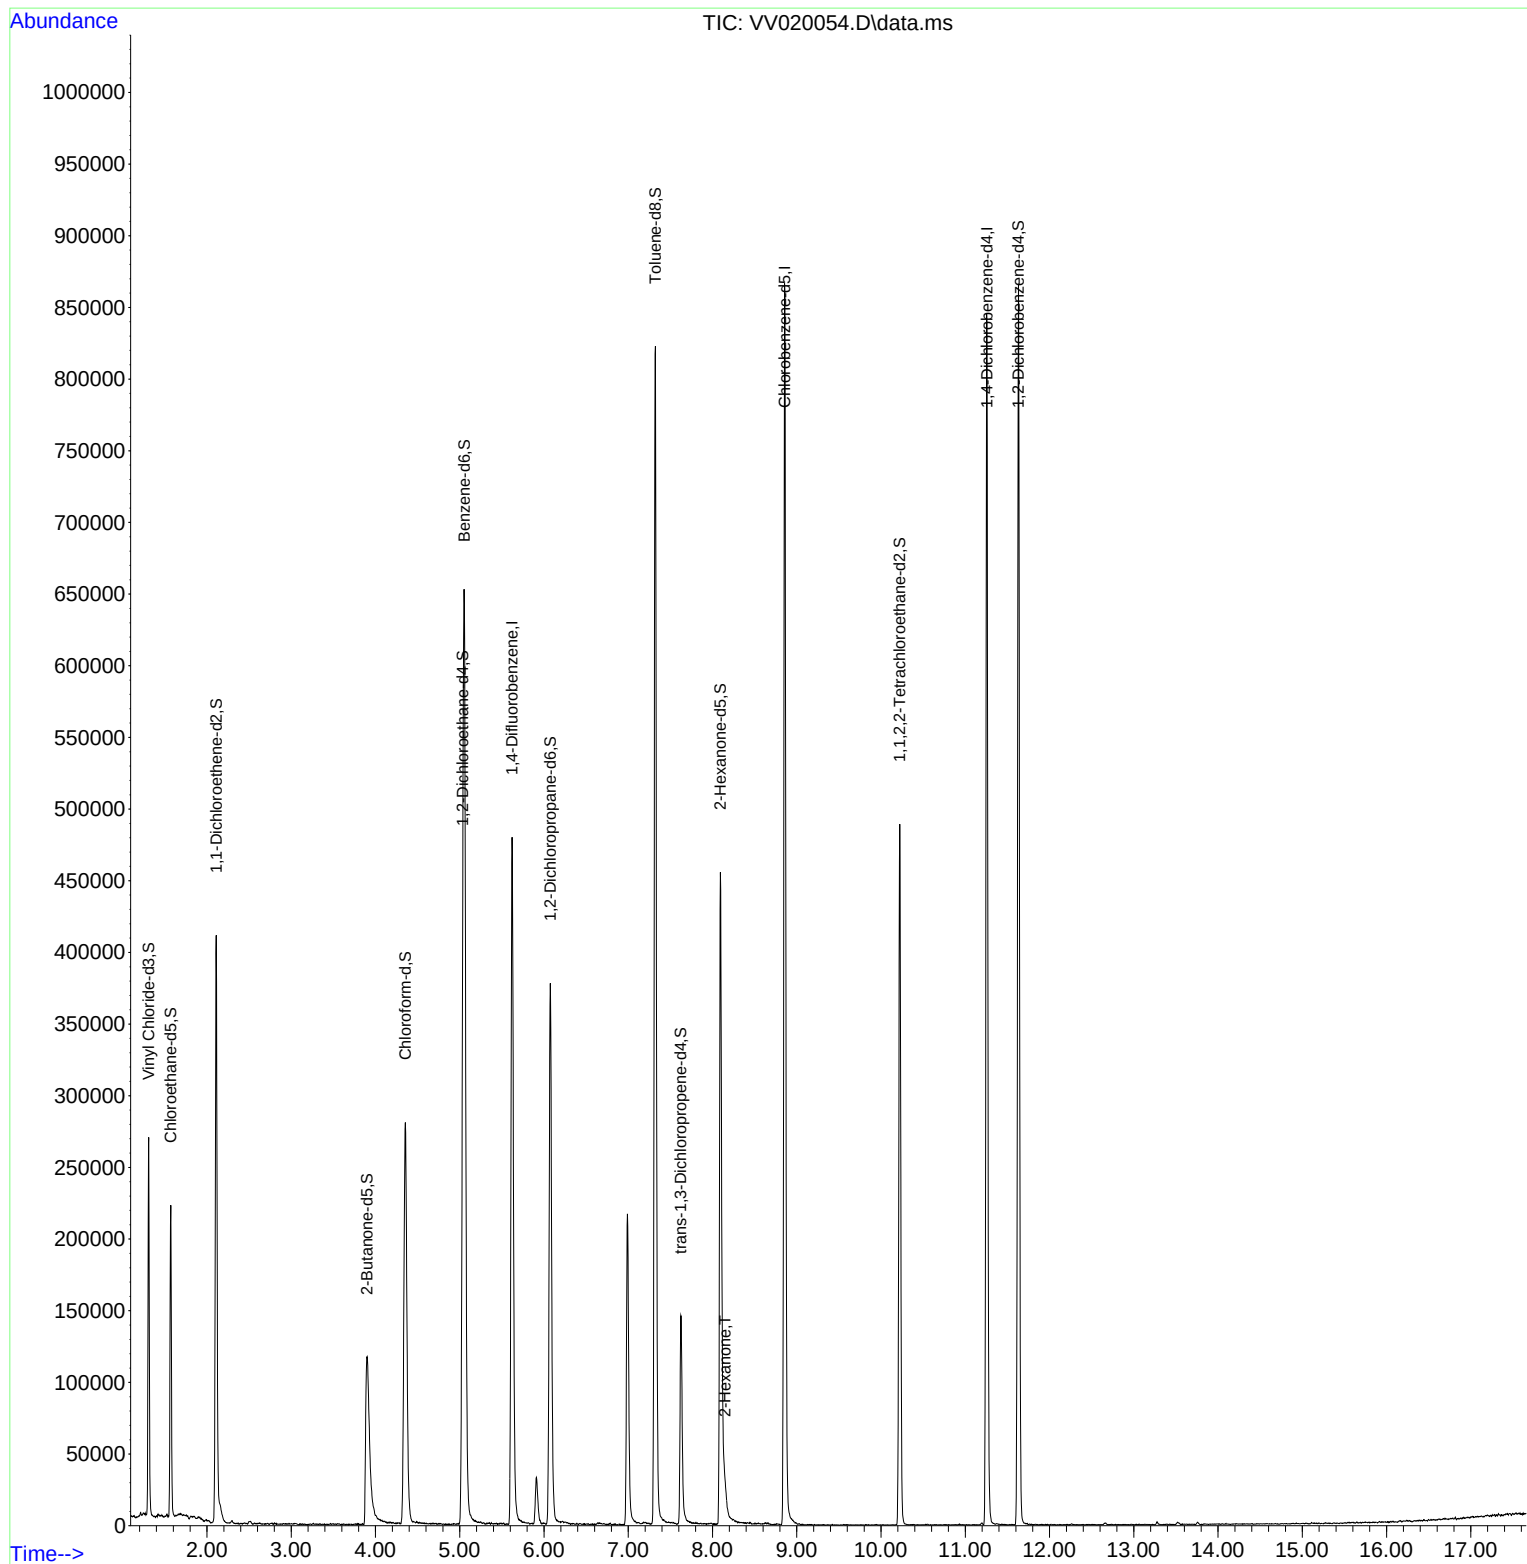

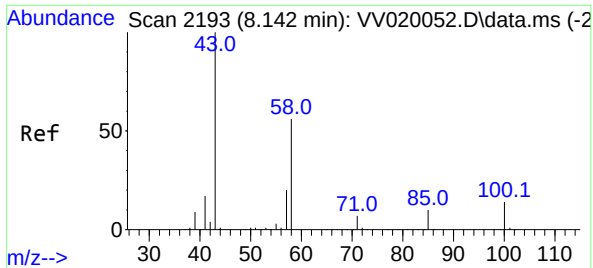

#48
2-Hexanone
Concen: 3.14 ug/L
RT: 8.148 min Scan# 2195
Delta R.T. 0.006 min
Lab File: VV020054.D
Acq: 19 Jan 2021 16:14

Instrument :
MSVOA_V
ClientSampleId :
VBLK82

Tgt Ion: 43 Resp: 12985

Ion	Ratio	Lower	Upper
43	100		
58	49.3	41.8	62.6
57	1.2	15.0	22.4#
100	4.4	8.9	13.3#

