

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011921\
 Data File : VW020066.D
 Acq On : 19 Jan 2021 21:51
 Operator : SY/MD
 Sample : M1173-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY1

Manual Integrations
 APPROVED

MMDadoda
 1/21/2021 10:40:05 AM

Quant Time: Jan 20 01:12:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 20 01:05:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.634	114	356	50.00	ug/L	# 0.02
28) Chlorobenzene-d5	8.865	117	1247	50.00	ug/L	# 0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	2296	50.00	ug/L	# 0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	190	63.27	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	126.54%	
7) Chloroethane-d5	1.569	69	79	32.96	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	65.92%#	
11) 1,1-Dichloroethene-d2	2.110	63	398	67.29	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	134.58%#	
21) 2-Butanone-d5	3.920	46	949m	487.17	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	487.17%#	
24) Chloroform-d	0.000	84	0	0.00	ug/L	
Spiked Amount 50.000	Range 70	- 125	Recovery	=	0.00%#	
26) 1,2-Dichloroethane-d4	5.061	65	51	13.87	ug/L	0.03
Spiked Amount 50.000	Range 70	- 125	Recovery	=	27.74%#	
32) Benzene-d6	5.064	84	347	9.86	ug/L	0.01
Spiked Amount 50.000	Range 70	- 125	Recovery	=	19.72%#	
36) 1,2-Dichloropropane-d6	0.000	67	0	0.00	ug/L	
Spiked Amount 50.000	Range 70	- 120	Recovery	=	0.00%#	
41) Toluene-d8	7.338	98	661	20.72	ug/L	0.02
Spiked Amount 50.000	Range 80	- 120	Recovery	=	41.44%#	
43) trans-1,3-Dichloroprop...	7.650	79	41	7.19	ug/L	0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	14.38%#	
47) 2-Hexanone-d5	0.000	63	0	0.00	ug/L	
Spiked Amount 100.000	Range 45	- 130	Recovery	=	0.00%#	
57) 1,1,2,2-Tetrachloroeth...	10.235	84	312m	21.00	ug/L	0.01
Spiked Amount 50.000	Range 65	- 120	Recovery	=	42.00%#	
64) 1,2-Dichlorobenzene-d4	11.630	152	2104	47.44	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.88%	
Target Compounds					Qvalue	
13) Acetone	2.187	43	18915	10989.95	ug/L	97
33) Benzene	5.116	78	10320	285.08	ug/L	100
51) Chlorobenzene	8.887	112	252120	9874.31	ug/L	98
62) 1,3-Dichlorobenzene	11.190	146	44839	650.81	ug/L	98
63) 1,4-Dichlorobenzene	11.280	146	350098	4951.76	ug/L	97
65) 1,2-Dichlorobenzene	11.649	146	1239407	17856.37	ug/L	98
68) 1,2,4-trichlorobenzene	13.270	180	317677	6944.41	ug/L	97
70) 1,2,3-Trichlorobenzene	13.752	180	184695	4159.35	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020066.D
Acq On : 19 Jan 2021 21:51
Operator : SY/MD
Sample : M1173-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0FY1

Manual Integrations
APPROVED

MMDadoda
1/21/2021 10:40:05 AM

Quant Time: Jan 20 01:12:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 20 01:05:37 2021
Response via : Initial Calibration

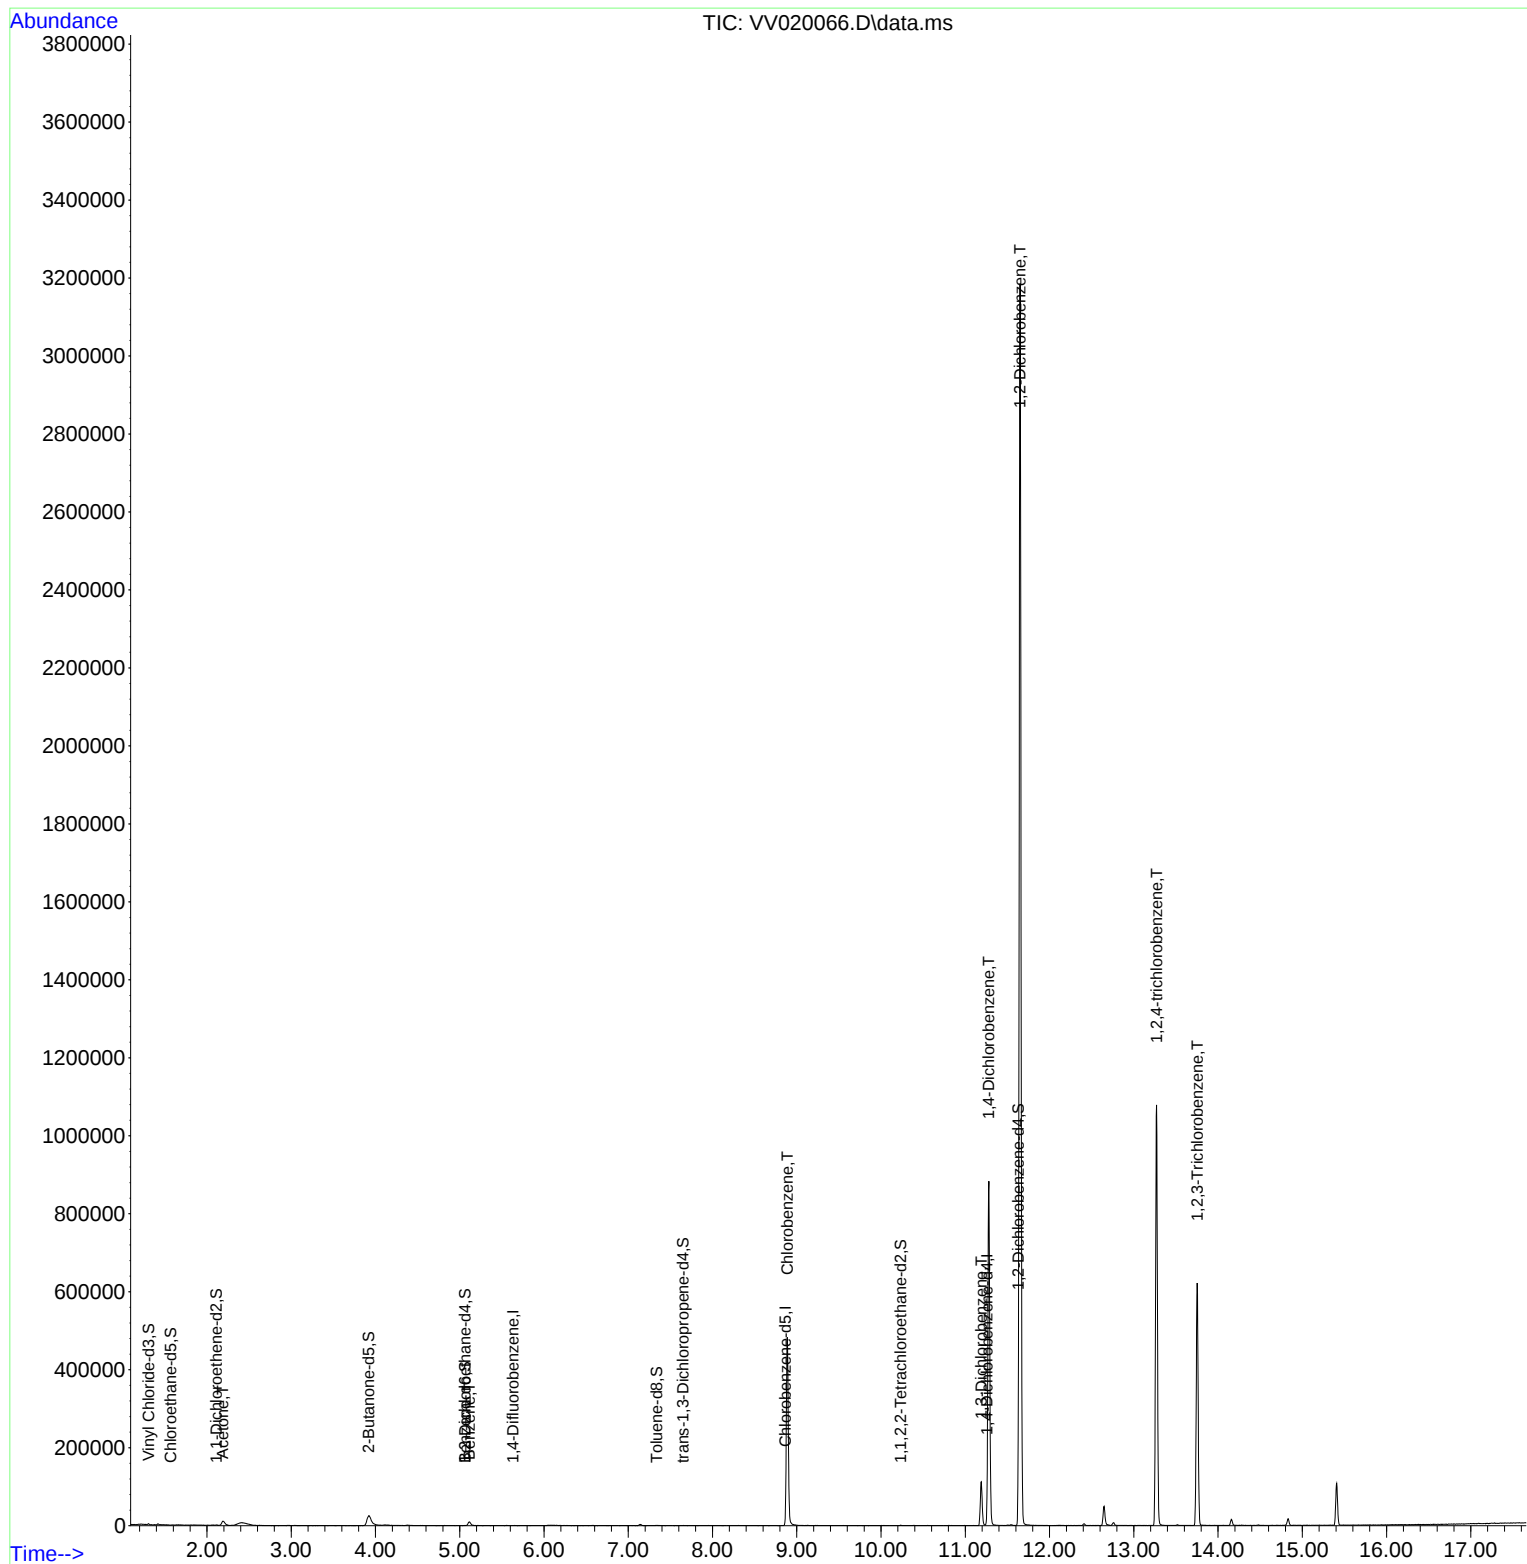

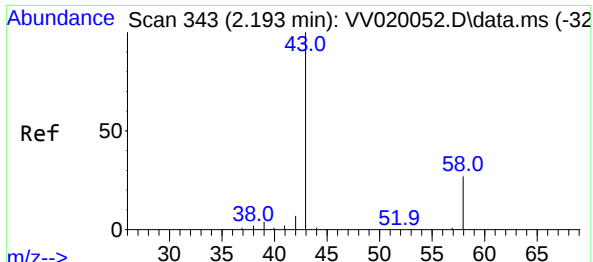





#13
Acetone
Concen: 10989.95 ug/L
RT: 2.187 min Scan# 341
Delta R.T. -0.007 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

Tgt Ion: 43 Resp: 18915
Ion Ratio Lower Upper
43 100
58 28.3 0.0 60.2

Instrument :
MSVOA_V
ClientSampled :
C0FY1




Manual Integrations
APPROVED


MMDadoda
1/21/2021 10:40:05 AM

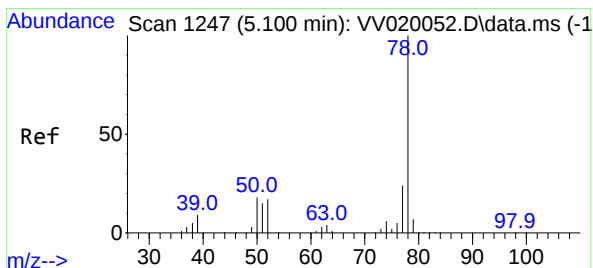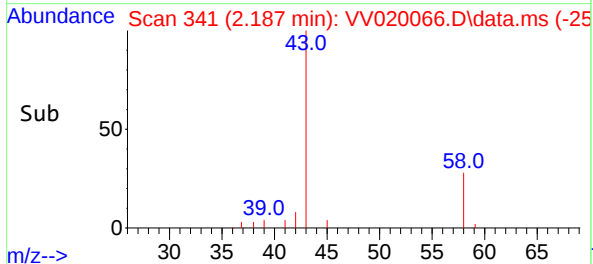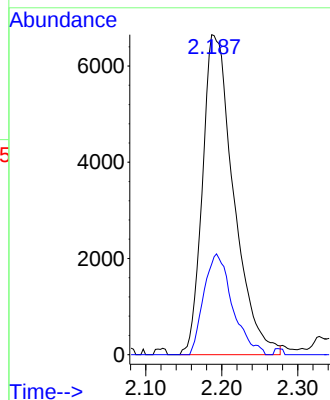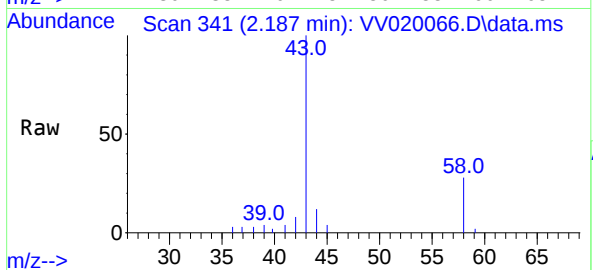

#33
Benzene
Concen: 285.08 ug/L
RT: 5.116 min Scan# 1252
Delta R.T. 0.016 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

Tgt Ion: 78 Resp: 10320

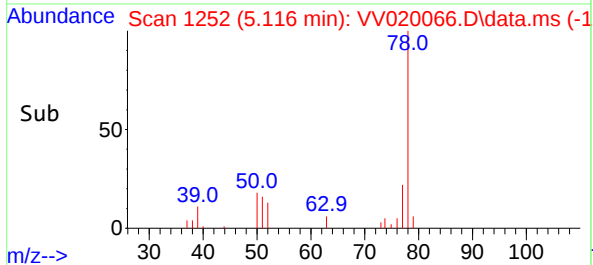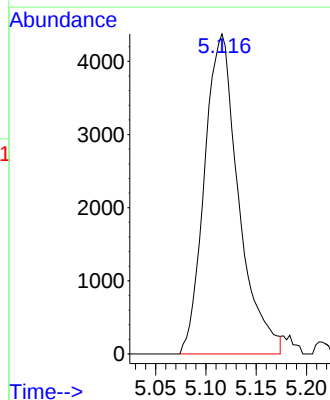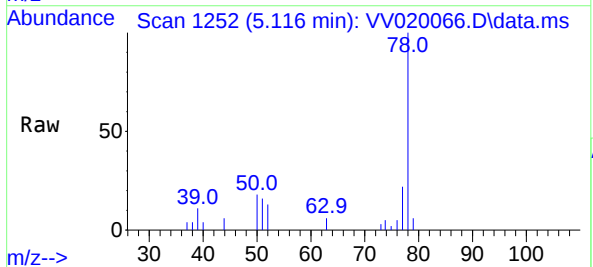

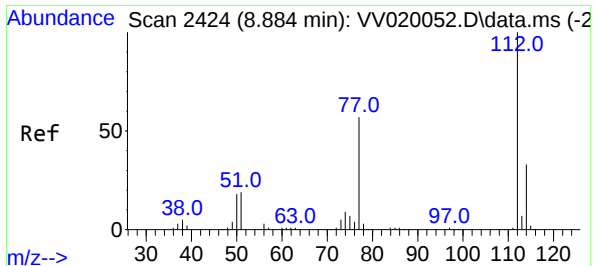





#51
Chlorobenzene
Concen: 9874.31 ug/L
RT: 8.887 min Scan# 2425
Delta R.T. 0.003 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

Tgt Ion:112 Resp: 252120
Ion Ratio Lower Upper
112 100
114 32.3 22.2 41.2
77 59.2 49.0 73.6

Instrument :
MSVOA_V
ClientSampled :
C0FY1




Manual Integrations
APPROVED


MMDadoda
1/21/2021 10:40:05 AM

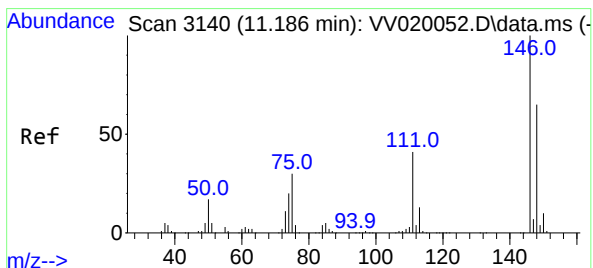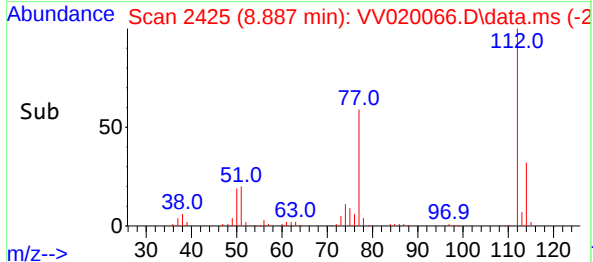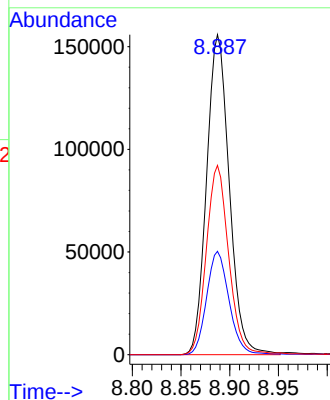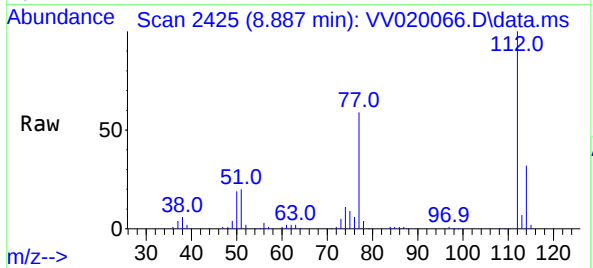


#62
1,3-Dichlorobenzene
Concen: 650.81 ug/L
RT: 11.190 min Scan# 3141
Delta R.T. 0.003 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

Tgt Ion:146 Resp: 44839
Ion Ratio Lower Upper
146 100
111 40.9 30.2 56.2
148 65.0 45.0 83.6

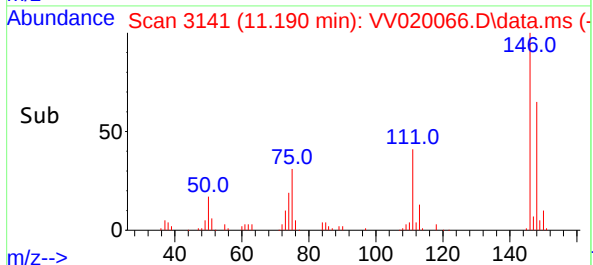
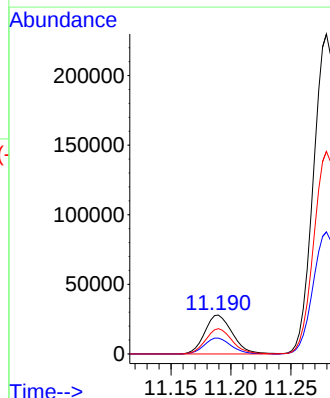
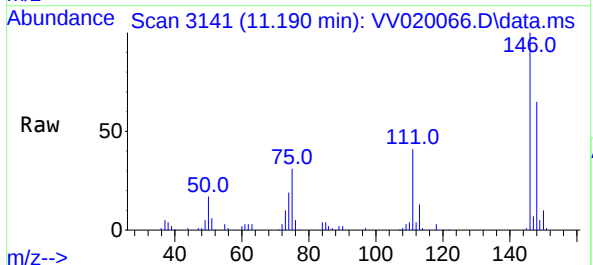


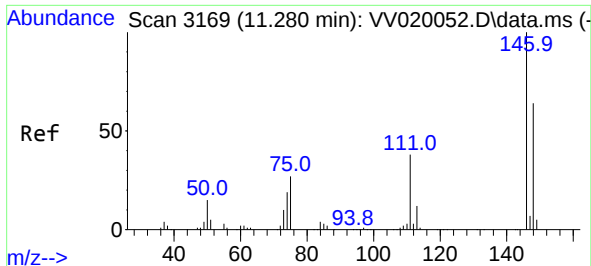


#63
1,4-Dichlorobenzene
Concen: 4951.76 ug/L
RT: 11.280 min Scan# 3169
Delta R.T. -0.000 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

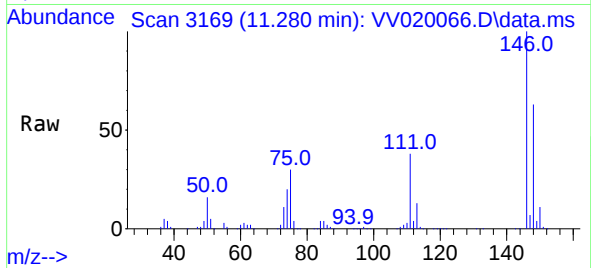



Tgt Ion:146 Resp: 350098
Ion Ratio Lower Upper
146 100
111 38.1 29.4 54.6
148 63.3 44.7 83.1

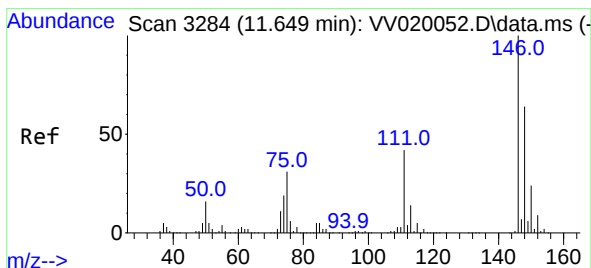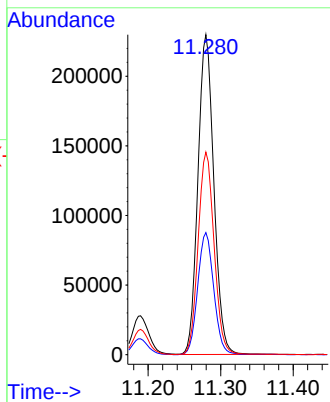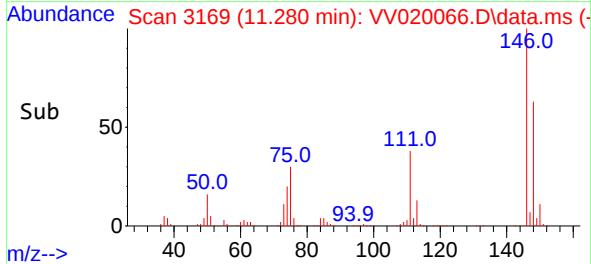

#65
1,2-Dichlorobenzene
Concen: 17856.37 ug/L
RT: 11.649 min Scan# 3284
Delta R.T. -0.000 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

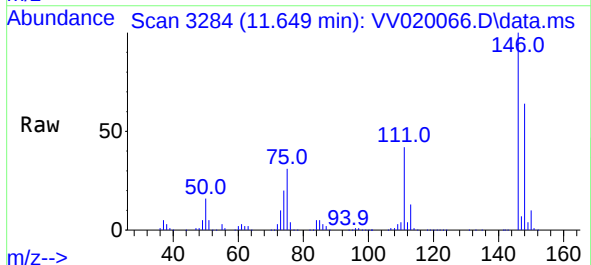


Tgt Ion:146 Resp: 1239407
Ion Ratio Lower Upper
146 100
111 42.3 36.3 54.5
148 64.1 51.7 77.5

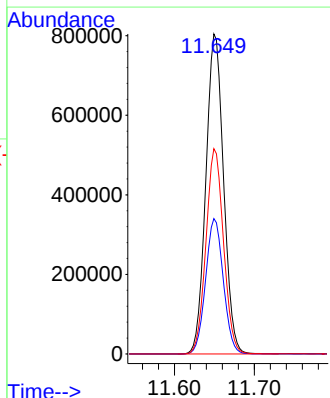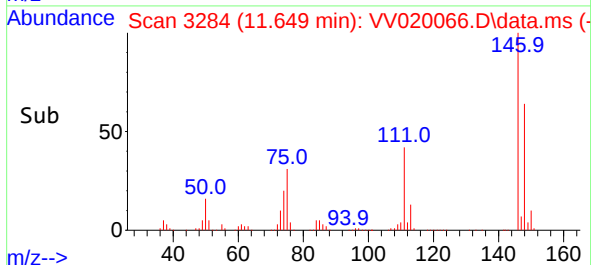

Instrument :
MSVOA_V
ClientSampled :
C0FY1


Manual Integrations
APPROVED

MMDadoda
1/21/2021 10:40:05 AM

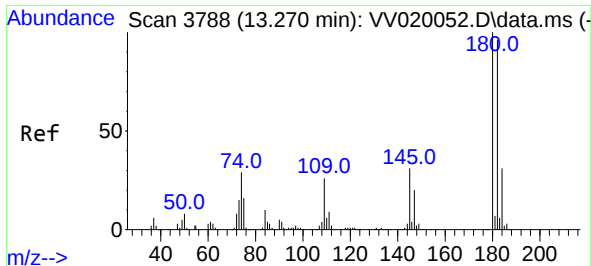

#68
1,2,4-trichlorobenzene
Concen: 6944.41 ug/L
RT: 13.270 min Scan# 3788
Delta R.T. -0.000 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51




Instrument :
MSVOA_V
ClientSampled :
C0FY1

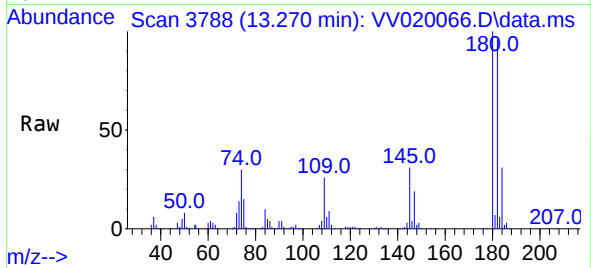


Tgt Ion:180 Resp: 317677
Ion Ratio Lower Upper
180 100
182 96.5 75.1 112.7
145 31.5 26.8 40.2

Manual Integrations
APPROVED

MMDadoda
1/21/2021 10:40:05 AM

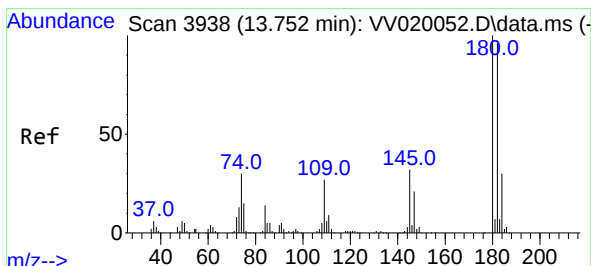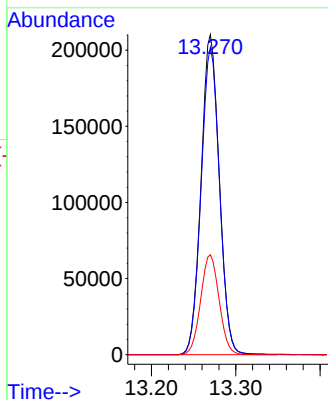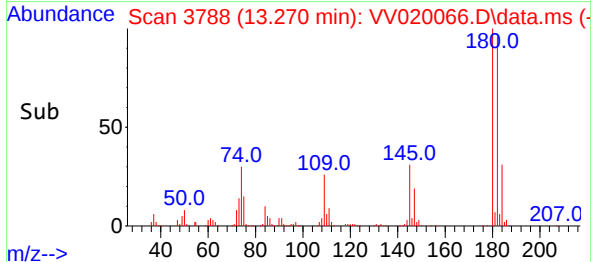

#70
1,2,3-Trichlorobenzene
Concen: 4159.35 ug/L
RT: 13.752 min Scan# 3938
Delta R.T. -0.000 min
Lab File: VV020066.D
Acq: 19 Jan 2021 21:51

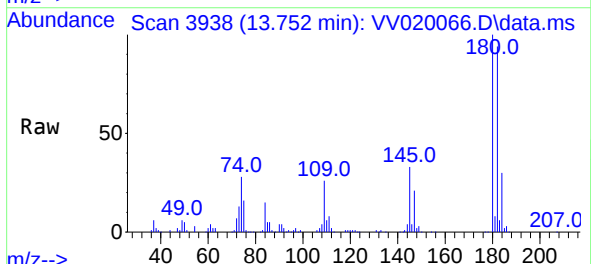

Tgt Ion:180 Resp: 184695
Ion Ratio Lower Upper
180 100
182 94.6 76.1 114.1
145 32.5 27.9 41.9

