

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020055.D
 Acq On : 19 Jan 2021 16:47
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	157054	161142	2.94%	0.770%
2	1.569	142	149	160	rVB	119528	129442	2.36%	0.619%
3	2.110	306	317	341	rVB	259039	390434	7.13%	1.866%
4	2.290	369	373	382	rVB2	1614	2369	0.04%	0.011%
5	2.611	469	473	474	rBV	221	113	0.00%	0.001%
6	2.643	480	483	485	rBV3	289	209	0.00%	0.001%
7	2.733	509	511	513	rBV	249	120	0.00%	0.001%
8	2.765	519	521	526	rBV2	235	147	0.00%	0.001%
9	2.923	563	570	576	rBV2	238	404	0.01%	0.002%
10	2.991	589	591	593	rBV2	156	97	0.00%	0.000%
11	3.026	600	602	603	rBV	173	55	0.00%	0.000%
12	3.155	632	642	647	rVB	329	538	0.01%	0.003%
13	3.187	647	652	654	rBV2	201	182	0.00%	0.001%
14	3.212	656	660	664	rVB	381	368	0.01%	0.002%
15	3.232	664	666	668	rVB	168	76	0.00%	0.000%
16	3.248	668	671	672	rBV	327	154	0.00%	0.001%
17	3.286	680	683	685	rBV2	398	213	0.00%	0.001%
18	3.338	698	699	700	rBV	141	34	0.00%	0.000%
19	3.402	715	719	721	rBV2	257	176	0.00%	0.001%
20	3.418	721	724	727	rVB2	267	179	0.00%	0.001%
21	3.434	727	729	730	rBV	98	48	0.00%	0.000%
22	3.447	731	733	735	rVB	193	58	0.00%	0.000%
23	3.460	735	737	742	rBV2	196	146	0.00%	0.001%
24	3.486	742	745	747	rBV2	126	94	0.00%	0.000%
25	3.540	755	762	766	rBV2	214	256	0.00%	0.001%
26	3.605	775	782	784	rBV2	278	283	0.01%	0.001%
27	3.669	799	802	804	rBV2	194	112	0.00%	0.001%
28	3.701	808	812	815	rBV	160	178	0.00%	0.001%
29	3.801	841	843	846	rVB3	186	102	0.00%	0.000%
30	3.891	858	871	911	rBV2	73514	222347	4.06%	1.063%
31	4.180	959	961	963	rBV2	436	232	0.00%	0.001%
32	4.351	998	1014	1043	rBV2	195971	488885	8.93%	2.336%
33	4.659	1108	1110	1112	rBV2	249	159	0.00%	0.001%
34	4.743	1134	1136	1138	rBV	158	106	0.00%	0.001%
35	4.836	1154	1165	1173	rBV5	1707	3481	0.06%	0.017%
36	4.900	1183	1185	1186	rBV5	164	76	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020055.D
 Acq On : 19 Jan 2021 16:47
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	4.936	1195	1196	1200	rVB	298	175	0.00%	0.001%
38	4.974	1207	1208	1209	rBV	250	89	0.00%	0.000%
39	5.048	1213	1231	1241	rBV2	485865	1237653	22.61%	5.914%
40	5.386	1334	1336	1339	rBV2	250	98	0.00%	0.000%
41	5.447	1353	1355	1357	rBV2	347	129	0.00%	0.001%
42	5.476	1363	1364	1365	rBV	235	82	0.00%	0.000%
43	5.527	1377	1380	1383	rBV2	282	180	0.00%	0.001%
44	5.617	1396	1408	1439	rBV	434785	878350	16.05%	4.197%
45	5.907	1488	1498	1517	rVB2	17201	36230	0.66%	0.173%
46	6.016	1529	1532	1533	rBV	251	115	0.00%	0.001%
47	6.071	1536	1549	1576	rBV	265655	543478	9.93%	2.597%
48	6.270	1609	1611	1615	rVB2	602	355	0.01%	0.002%
49	6.286	1615	1616	1617	rBV2	277	87	0.00%	0.000%
50	6.360	1636	1639	1640	rBV	181	99	0.00%	0.000%
51	6.376	1641	1644	1648	rVV2	387	308	0.01%	0.001%
52	6.412	1652	1655	1660	rBV2	285	252	0.00%	0.001%
53	6.547	1695	1697	1699	rBV2	212	140	0.00%	0.001%
54	6.637	1719	1725	1726	rBV	205	150	0.00%	0.001%
55	6.711	1747	1748	1749	rBV	145	42	0.00%	0.000%
56	6.791	1770	1773	1775	rBV	180	144	0.00%	0.001%
57	6.884	1800	1802	1805	rBV2	249	128	0.00%	0.001%
58	6.952	1821	1823	1824	rBV	219	112	0.00%	0.001%
59	6.990	1824	1835	1853	rBV2	149625	274639	5.02%	1.312%
60	7.318	1924	1937	1961	rBV	586618	1014136	18.53%	4.846%
61	7.624	2022	2032	2054	rBV2	103840	183167	3.35%	0.875%
62	7.797	2083	2086	2088	rVB	521	313	0.01%	0.001%
63	7.884	2111	2113	2116	rVB	262	112	0.00%	0.001%
64	8.026	2155	2157	2162	rVB2	315	195	0.00%	0.001%
65	8.055	2162	2166	2168	rBV2	271	267	0.00%	0.001%
66	8.093	2168	2178	2209	rBV	260071	497995	9.10%	2.380%
67	8.363	2259	2262	2263	rBV	467	310	0.01%	0.001%
68	8.662	2352	2355	2356	rBV	321	148	0.00%	0.001%
69	8.884	2403	2424	2465	rBV2	2764102	5473945	100.00%	26.159%
70	9.235	2530	2533	2535	rBV3	345	209	0.00%	0.001%
71	9.318	2557	2559	2561	rBV	249	103	0.00%	0.000%
72	9.453	2596	2601	2603	rBV	221	232	0.00%	0.001%
73	9.508	2616	2618	2619	rBV	225	90	0.00%	0.000%
74	9.550	2627	2631	2634	rBV2	503	471	0.01%	0.002%
75	9.736	2688	2689	2690	rBV2	205	60	0.00%	0.000%
76	10.064	2786	2791	2796	rBV3	451	543	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020055.D
 Acq On : 19 Jan 2021 16:47
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.109	2801	2805	2806	rBV	334	239	0.00%	0.001%
78	10.145	2814	2816	2820	rBV2	193	102	0.00%	0.000%
79	10.161	2820	2821	2822	rBV2	192	60	0.00%	0.000%
80	10.222	2828	2840	2862	rBV	349449	544321	9.94%	2.601%
81	10.537	2936	2938	2940	rBV2	298	150	0.00%	0.001%
82	10.887	3043	3047	3048	rBV2	243	201	0.00%	0.001%
83	11.186	3130	3140	3151	rBV	211945	327346	5.98%	1.564%
84	11.276	3151	3168	3194	rVB2	1648429	3652083	66.72%	17.452%
85	11.649	3266	3284	3304	rBV2	2097867	4039105	73.79%	19.302%
86	12.042	3402	3406	3410	rBV2	411	430	0.01%	0.002%
87	12.202	3452	3456	3459	rBV2	515	489	0.01%	0.002%
88	12.411	3515	3521	3529	rVB4	2266	2902	0.05%	0.014%
89	12.656	3593	3597	3604	rVB5	1739	1982	0.04%	0.009%
90	13.270	3777	3788	3811	rBV	416298	643792	11.76%	3.077%
91	13.755	3928	3939	3954	rBV	106170	164502	3.01%	0.786%




Sum of corrected areas: 20926050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020055.D
Acq On : 19 Jan 2021 16:47
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

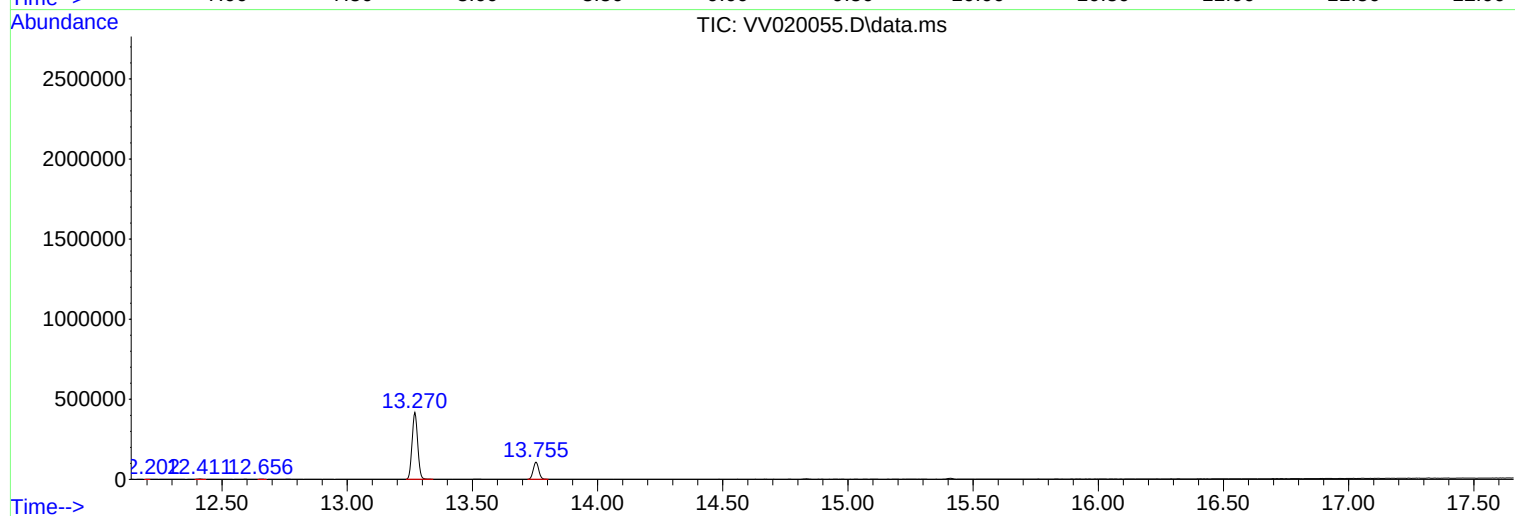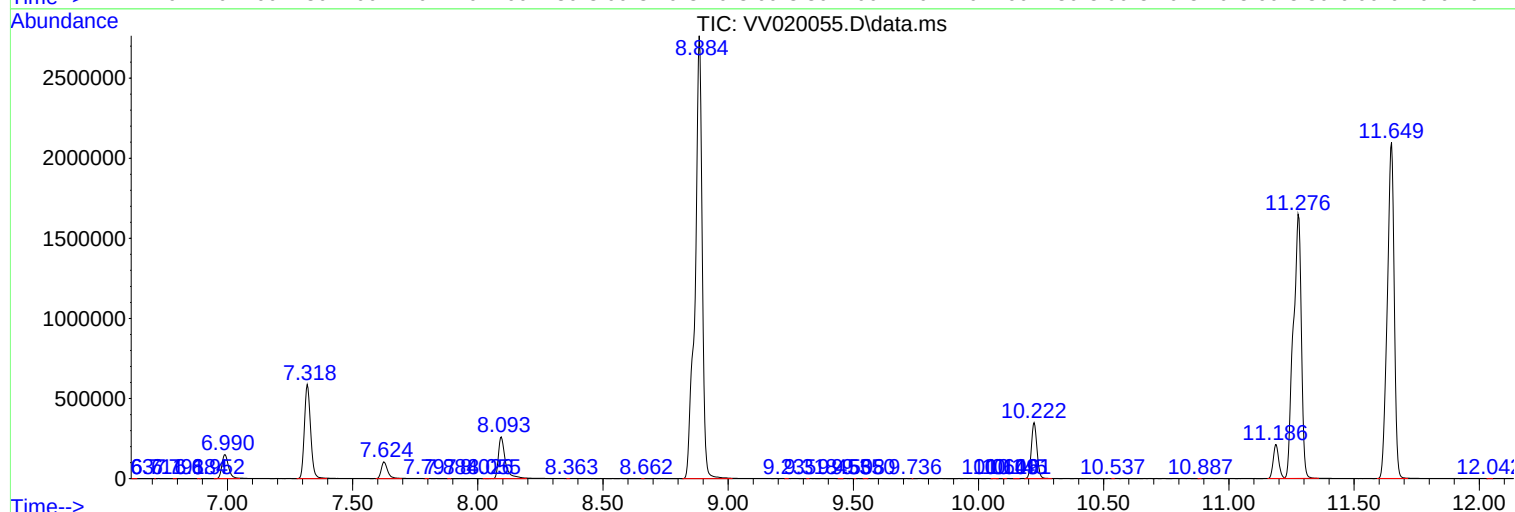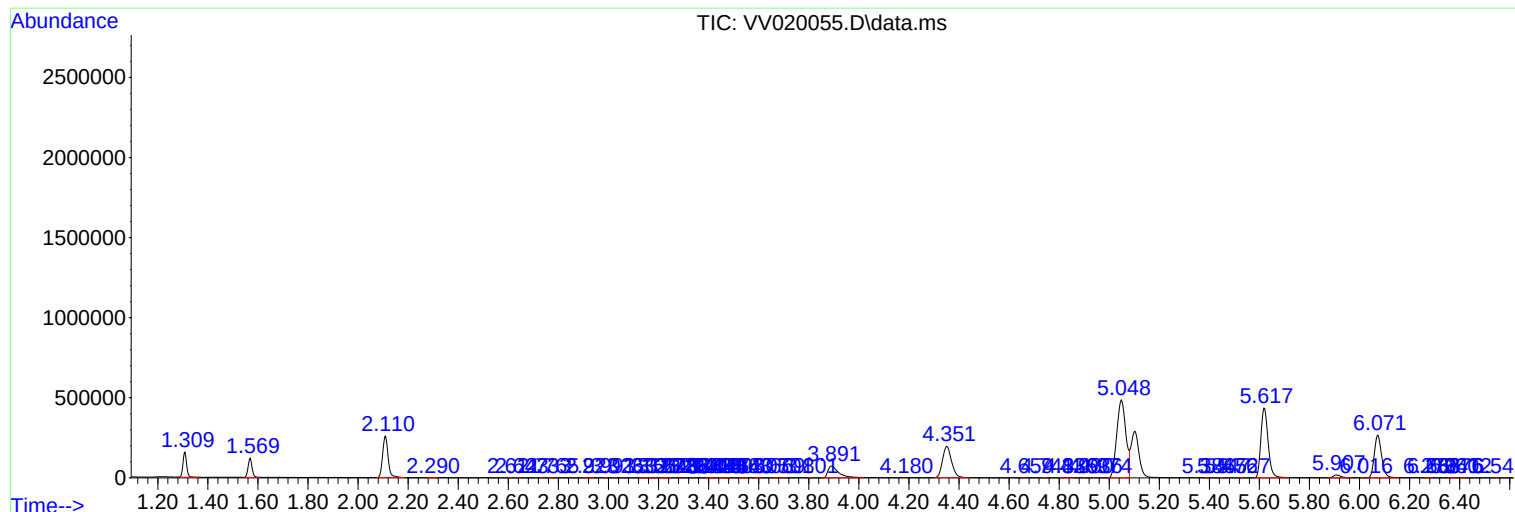

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020055.D
Acq On : 19 Jan 2021 16:47
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020055.D
Acq On : 19 Jan 2021 16:47
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
