

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020056.D
 Acq On : 19 Jan 2021 17:10
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	128282	132040	12.46%	1.580%
2	1.569	141	149	163	rVB	103394	116545	11.00%	1.395%
3	1.962	269	271	275	rBV2	447	343	0.03%	0.004%
4	2.110	306	317	347	rBV	223676	337614	31.86%	4.040%
5	2.277	365	369	371	rBV2	700	500	0.05%	0.006%
6	2.415	408	412	414	rBV2	541	381	0.04%	0.005%
7	2.450	419	423	427	rVV4	549	573	0.05%	0.007%
8	2.511	434	442	448	rVB4	1432	2095	0.20%	0.025%
9	2.614	468	474	477	rBV2	433	442	0.04%	0.005%
10	2.653	481	486	489	rVB2	381	279	0.03%	0.003%
11	2.672	489	492	495	rBV2	263	207	0.02%	0.002%
12	2.708	499	503	506	rBV3	381	393	0.04%	0.005%
13	2.756	515	518	521	rVV2	418	282	0.03%	0.003%
14	2.836	540	543	548	rBV2	294	271	0.03%	0.003%
15	2.891	556	560	565	rBV2	317	273	0.03%	0.003%
16	3.000	589	594	599	rVB2	470	435	0.04%	0.005%
17	3.023	599	601	603	rBV2	380	221	0.02%	0.003%
18	3.065	611	614	619	rVB2	327	244	0.02%	0.003%
19	3.190	649	653	657	rBV3	442	368	0.03%	0.004%
20	3.502	747	750	753	rBV2	275	213	0.02%	0.003%
21	3.669	795	802	804	rBV2	312	239	0.02%	0.003%
22	3.688	804	808	810	rVB2	260	189	0.02%	0.002%
23	3.900	864	874	913	rBV	64324	209309	19.75%	2.504%
24	4.235	976	978	983	rVB2	374	207	0.02%	0.002%
25	4.354	998	1015	1042	rBV	168414	419380	39.57%	5.018%
26	4.560	1076	1079	1083	rBV3	339	294	0.03%	0.004%
27	4.605	1090	1093	1096	rVB2	354	214	0.02%	0.003%
28	4.624	1096	1099	1103	rBV3	490	320	0.03%	0.004%
29	4.682	1113	1117	1124	rVB3	434	503	0.05%	0.006%
30	4.736	1131	1134	1137	rBV3	261	207	0.02%	0.002%
31	4.952	1197	1201	1207	rBV2	275	247	0.02%	0.003%
32	5.052	1207	1232	1267	rBV2	410826	1059831	100.00%	12.681%
33	5.277	1297	1302	1305	rBV3	557	411	0.04%	0.005%
34	5.405	1335	1342	1344	rBV3	272	305	0.03%	0.004%
35	5.621	1397	1409	1435	rBV	348655	701615	66.20%	8.395%
36	5.859	1481	1483	1488	rVB2	365	261	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020056.D
 Acq On : 19 Jan 2021 17:10
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.910	1488	1499	1517	rBV2	23165	47559	4.49%	0.569%
38	6.074	1537	1550	1576	rVV	227249	469463	44.30%	5.617%
39	6.212	1588	1593	1596	rBV4	438	452	0.04%	0.005%
40	6.579	1703	1707	1710	rBV	203	190	0.02%	0.002%
41	6.621	1716	1720	1725	rVV2	255	232	0.02%	0.003%
42	6.691	1738	1742	1744	rVV	319	206	0.02%	0.002%
43	6.740	1753	1757	1760	rBV2	281	239	0.02%	0.003%
44	6.788	1766	1772	1776	rBV2	280	304	0.03%	0.004%
45	6.926	1806	1815	1820	rBV2	387	564	0.05%	0.007%
46	6.990	1824	1835	1857	rBV	127271	231237	21.82%	2.767%
47	7.322	1925	1938	1963	rBV	485697	855075	80.68%	10.231%
48	7.553	2007	2010	2017	rVB2	362	324	0.03%	0.004%
49	7.627	2017	2033	2062	rBV	87108	157065	14.82%	1.879%
50	7.823	2092	2094	2097	rBV2	435	225	0.02%	0.003%
51	7.920	2118	2124	2126	rBV2	298	219	0.02%	0.003%
52	7.987	2140	2145	2150	rBV3	673	659	0.06%	0.008%
53	8.042	2159	2162	2165	rBV	284	237	0.02%	0.003%
54	8.096	2168	2179	2216	rBV2	225756	470506	44.39%	5.630%
55	8.322	2245	2249	2253	rVB2	382	385	0.04%	0.005%
56	8.447	2284	2288	2290	rBV2	510	311	0.03%	0.004%
57	8.540	2313	2317	2322	rVB3	267	225	0.02%	0.003%
58	8.582	2328	2330	2333	rVB2	389	215	0.02%	0.003%
59	8.621	2338	2342	2345	rBV3	322	250	0.02%	0.003%
60	8.698	2363	2366	2370	rBV2	375	314	0.03%	0.004%
61	8.723	2370	2374	2377	rVV	278	232	0.02%	0.003%
62	8.765	2385	2387	2392	rBV2	245	246	0.02%	0.003%
63	8.858	2404	2416	2447	rBV	529650	874179	82.48%	10.460%
64	9.026	2466	2468	2471	rBV3	376	233	0.02%	0.003%
65	9.161	2505	2510	2514	rBV2	321	345	0.03%	0.004%
66	9.244	2533	2536	2539	rBV	307	245	0.02%	0.003%
67	9.286	2544	2549	2557	rVV2	267	425	0.04%	0.005%
68	9.450	2595	2600	2603	rBV2	179	196	0.02%	0.002%
69	9.595	2641	2645	2649	rBV	339	301	0.03%	0.004%
70	9.797	2702	2708	2713	rBV2	189	278	0.03%	0.003%
71	10.177	2823	2826	2829	rBV2	230	185	0.02%	0.002%
72	10.222	2829	2840	2855	rBV	295740	462080	43.60%	5.529%
73	10.354	2878	2881	2887	rBV	169	188	0.02%	0.002%
74	10.505	2922	2928	2934	rBV	405	454	0.04%	0.005%
75	10.550	2939	2942	2948	rVV2	359	244	0.02%	0.003%
76	10.759	3003	3007	3009	rBV	390	303	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020056.D
 Acq On : 19 Jan 2021 17:10
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.862	3033	3039	3041	rBV2	354	379	0.04%	0.005%
78	10.932	3055	3061	3065	rBV3	330	425	0.04%	0.005%
79	11.003	3080	3083	3086	rBV	391	300	0.03%	0.004%
80	11.196	3137	3143	3150	rBV3	1171	1352	0.13%	0.016%
81	11.257	3150	3162	3185	rBV	580471	919018	86.71%	10.996%
82	11.492	3233	3235	3239	rVB	323	207	0.02%	0.002%
83	11.550	3249	3253	3259	rBV2	266	299	0.03%	0.004%
84	11.630	3265	3278	3296	rBV	540973	857962	80.95%	10.266%
85	11.813	3328	3335	3339	rBV3	343	435	0.04%	0.005%
86	12.122	3428	3431	3435	rBV2	474	379	0.04%	0.005%
87	12.257	3470	3473	3477	rBV2	288	197	0.02%	0.002%
88	12.386	3510	3513	3516	rBV2	310	224	0.02%	0.003%
89	12.804	3640	3643	3644	rBV	330	194	0.02%	0.002%
90	13.067	3723	3725	3731	rBV	229	213	0.02%	0.003%
91	13.238	3774	3778	3780	rBV2	428	372	0.04%	0.004%
92	13.273	3781	3789	3802	rVB3	4467	7123	0.67%	0.085%
93	13.411	3830	3832	3835	rBV	346	246	0.02%	0.003%
94	13.482	3852	3854	3858	rBV	288	183	0.02%	0.002%
95	13.505	3858	3861	3864	rBV2	645	532	0.05%	0.006%
96	13.701	3919	3922	3924	rBV2	322	214	0.02%	0.003%
97	13.755	3934	3939	3947	rBV4	1712	2212	0.21%	0.026%
98	14.122	4051	4053	4056	rBV	405	236	0.02%	0.003%
99	15.263	4406	4408	4413	rBV3	790	575	0.05%	0.007%
100	15.704	4543	4545	4547	rBV2	651	308	0.03%	0.004%


Sum of corrected areas: 8357426

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020056.D
Acq On : 19 Jan 2021 17:10
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

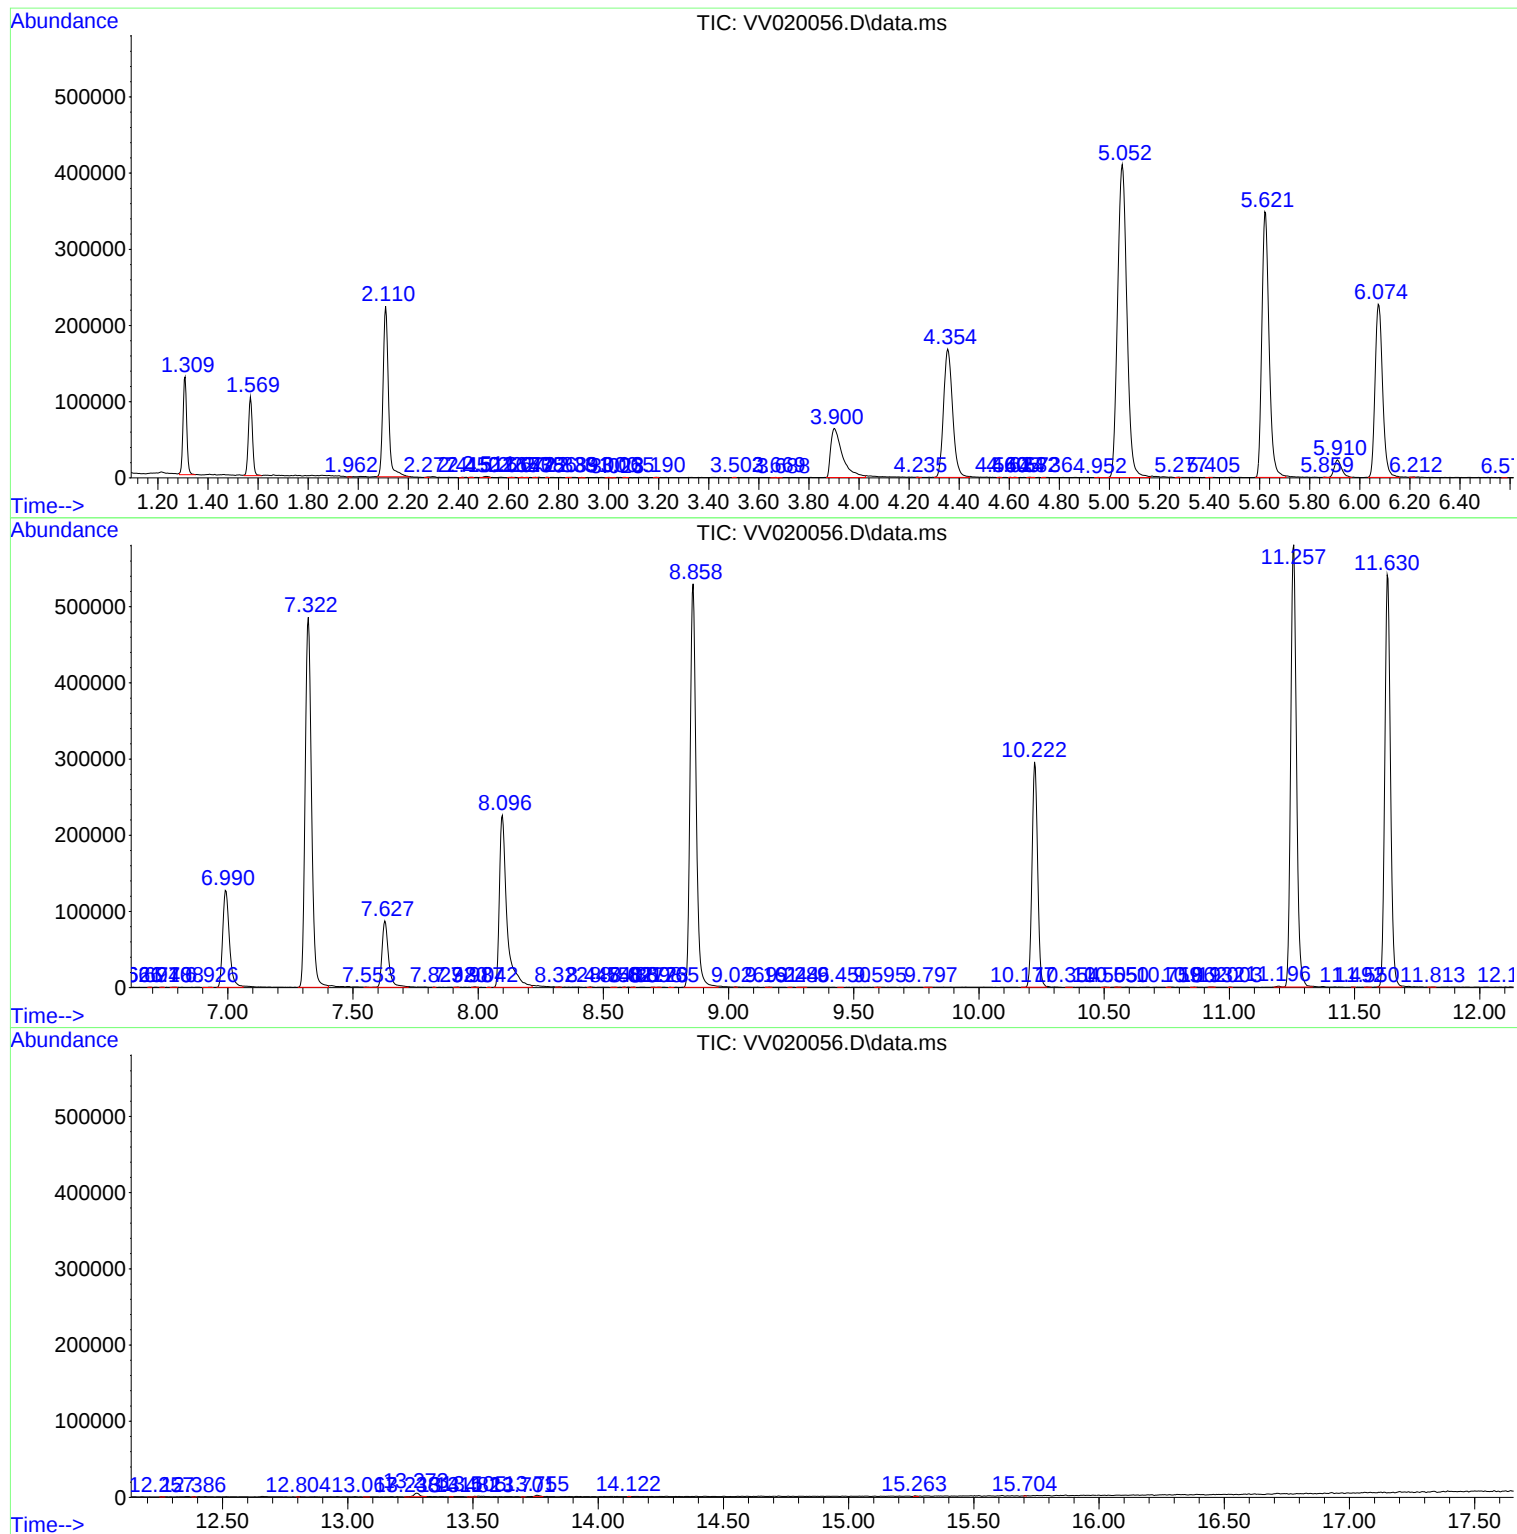

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020056.D
Acq On : 19 Jan 2021 17:10
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020056.D
Acq On : 19 Jan 2021 17:10
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
