

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020058.D
 Acq On : 19 Jan 2021 18:21
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	60	67	80	rVB	184905	185479	12.44%	1.634%
2	1.569	141	149	163	rVB	144611	160076	10.74%	1.410%
3	2.010	282	286	289	rBV4	769	605	0.04%	0.005%
4	2.110	303	317	348	rBV	308756	476713	31.97%	4.200%
5	2.296	371	375	378	rVV	805	828	0.06%	0.007%
6	2.386	400	403	405	rBV	252	170	0.01%	0.001%
7	2.508	435	441	446	rBV3	1210	1564	0.10%	0.014%
8	2.614	472	474	477	rVB2	366	182	0.01%	0.002%
9	2.724	505	508	510	rBV2	253	219	0.01%	0.002%
10	2.769	517	522	523	rVV4	596	503	0.03%	0.004%
11	2.926	565	571	574	rBV2	178	213	0.01%	0.002%
12	2.975	582	586	589	rVB2	234	178	0.01%	0.002%
13	3.052	599	610	617	rVV5	2148	4400	0.30%	0.039%
14	3.122	628	632	635	rVB2	267	191	0.01%	0.002%
15	3.161	639	644	648	rVB3	232	223	0.01%	0.002%
16	3.299	682	687	689	rBV	223	243	0.02%	0.002%
17	3.312	689	691	695	rVB2	497	250	0.02%	0.002%
18	3.376	706	711	714	rBV2	479	410	0.03%	0.004%
19	3.412	719	722	726	rVB2	225	194	0.01%	0.002%
20	3.534	756	760	764	rBV2	192	191	0.01%	0.002%
21	3.630	788	790	796	rVB	247	161	0.01%	0.001%
22	3.756	822	829	831	rBV3	800	558	0.04%	0.005%
23	3.897	862	873	912	rBV2	92875	301143	20.20%	2.653%
24	4.277	989	991	995	rVB2	357	199	0.01%	0.002%
25	4.354	995	1015	1041	rBV	238000	587584	39.41%	5.177%
26	4.592	1087	1089	1092	rBV2	305	239	0.02%	0.002%
27	4.637	1100	1103	1106	rBV3	289	170	0.01%	0.001%
28	4.714	1125	1127	1131	rVB	346	209	0.01%	0.002%
29	4.759	1138	1141	1145	rVB2	288	255	0.02%	0.002%
30	4.782	1145	1148	1153	rVB2	305	210	0.01%	0.002%
31	4.814	1153	1158	1159	rBV2	283	223	0.01%	0.002%
32	4.913	1184	1189	1191	rVV	243	164	0.01%	0.001%
33	4.926	1191	1193	1198	rVB2	330	177	0.01%	0.002%
34	5.052	1214	1232	1269	rBV2	579688	1491009	100.00%	13.136%
35	5.286	1303	1305	1308	rVB3	349	162	0.01%	0.001%
36	5.309	1310	1312	1315	rVB3	346	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011921\
 Data File : VW020058.D
 Acq On : 19 Jan 2021 18:21
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.402	1337	1341	1345	rBV2	376	209	0.01%	0.002%
38	5.428	1347	1349	1352	rVB2	339	189	0.01%	0.002%
39	5.486	1364	1367	1371	rBV2	187	189	0.01%	0.002%
40	5.621	1396	1409	1431	rBV	442964	872895	58.54%	7.690%
41	5.910	1488	1499	1518	rBV3	28647	59990	4.02%	0.529%
42	6.074	1533	1550	1576	rBV	330644	669235	44.88%	5.896%
43	6.219	1588	1595	1600	rBV3	725	1050	0.07%	0.009%
44	6.267	1607	1610	1612	rVB4	525	260	0.02%	0.002%
45	6.386	1644	1647	1650	rVB2	315	249	0.02%	0.002%
46	6.412	1650	1655	1659	rVB2	295	342	0.02%	0.003%
47	6.441	1659	1664	1668	rBV	218	229	0.02%	0.002%
48	6.611	1715	1717	1723	rBV2	289	287	0.02%	0.003%
49	6.875	1796	1799	1802	rVB2	375	239	0.02%	0.002%
50	6.897	1802	1806	1810	rBV2	169	176	0.01%	0.002%
51	6.990	1823	1835	1860	rBV	179596	327635	21.97%	2.886%
52	7.148	1880	1884	1887	rBV3	345	281	0.02%	0.002%
53	7.241	1909	1913	1915	rBV2	331	241	0.02%	0.002%
54	7.322	1925	1938	1961	rBV	706018	1221041	81.89%	10.757%
55	7.627	2022	2033	2052	rBV	124061	216156	14.50%	1.904%
56	7.929	2124	2127	2130	rVB3	346	240	0.02%	0.002%
57	7.978	2139	2142	2148	rVV2	511	518	0.03%	0.005%
58	8.093	2167	2178	2211	rBV2	342592	678413	45.50%	5.977%
59	8.370	2261	2264	2265	rBV2	344	231	0.02%	0.002%
60	8.592	2331	2333	2336	rVB	383	163	0.01%	0.001%
61	8.704	2365	2368	2372	rBV2	375	347	0.02%	0.003%
62	8.785	2387	2393	2394	rBV2	275	241	0.02%	0.002%
63	8.859	2404	2416	2435	rBV	660732	1080908	72.50%	9.523%
64	9.061	2476	2479	2484	rVB2	237	198	0.01%	0.002%
65	9.347	2565	2568	2573	rBV2	212	230	0.02%	0.002%
66	9.505	2614	2617	2621	rVB3	279	185	0.01%	0.002%
67	9.559	2629	2634	2637	rBV2	339	309	0.02%	0.003%
68	9.656	2660	2664	2669	rVB3	412	457	0.03%	0.004%
69	9.820	2713	2715	2721	rVB2	215	166	0.01%	0.001%
70	9.910	2741	2743	2745	rBV2	315	160	0.01%	0.001%
71	9.949	2752	2755	2759	rBV2	638	504	0.03%	0.004%
72	10.161	2819	2821	2827	rVB2	249	196	0.01%	0.002%
73	10.222	2827	2840	2861	rBV	429694	666052	44.67%	5.868%
74	10.495	2922	2925	2927	rBV	241	158	0.01%	0.001%
75	10.608	2957	2960	2962	rBV2	328	253	0.02%	0.002%
76	10.797	3016	3019	3022	rBV2	316	267	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020058.D
 Acq On : 19 Jan 2021 18:21
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.923	3056	3058	3061	rVB	315	177	0.01%	0.002%
78	11.058	3094	3100	3101	rBV2	344	311	0.02%	0.003%
79	11.257	3150	3162	3182	rBV	728382	1132838	75.98%	9.980%
80	11.630	3265	3278	3302	rBV	752235	1193938	80.08%	10.519%
81	11.842	3342	3344	3348	rBV2	330	241	0.02%	0.002%
82	11.881	3354	3356	3359	rVB	350	177	0.01%	0.002%
83	12.093	3419	3422	3425	rVB2	340	174	0.01%	0.002%
84	12.411	3518	3521	3524	rBV2	370	277	0.02%	0.002%
85	12.620	3582	3586	3589	rBV	339	289	0.02%	0.003%
86	12.656	3594	3597	3601	rBV	504	471	0.03%	0.004%
87	12.714	3611	3615	3616	rBV	352	245	0.02%	0.002%
88	12.932	3680	3683	3684	rBV2	288	162	0.01%	0.001%
89	12.977	3694	3697	3701	rBV	251	210	0.01%	0.002%
90	13.061	3718	3723	3727	rBV2	437	525	0.04%	0.005%
91	13.080	3727	3729	3735	rVB3	396	322	0.02%	0.003%
92	13.273	3786	3789	3790	rBV2	658	350	0.02%	0.003%
93	13.357	3811	3815	3818	rVB2	386	275	0.02%	0.002%
94	13.376	3818	3821	3823	rBV	319	223	0.01%	0.002%
95	13.765	3936	3942	3944	rVB3	659	678	0.05%	0.006%
96	13.784	3944	3948	3951	rBV2	519	373	0.03%	0.003%
97	14.016	4014	4020	4022	rBV2	417	538	0.04%	0.005%
98	14.334	4117	4119	4125	rBV2	418	361	0.02%	0.003%
99	15.022	4329	4333	4336	rBV2	529	488	0.03%	0.004%
100	16.157	4684	4686	4689	rBV3	981	627	0.04%	0.006%




Sum of corrected areas: 11350820

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020058.D
Acq On : 19 Jan 2021 18:21
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

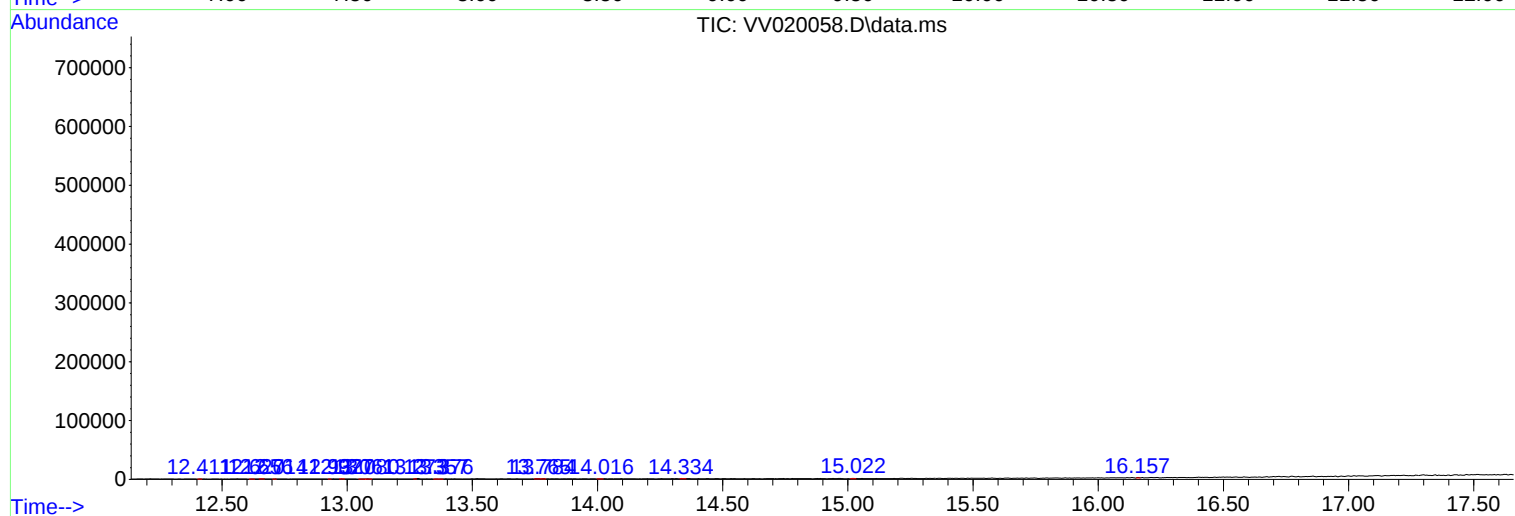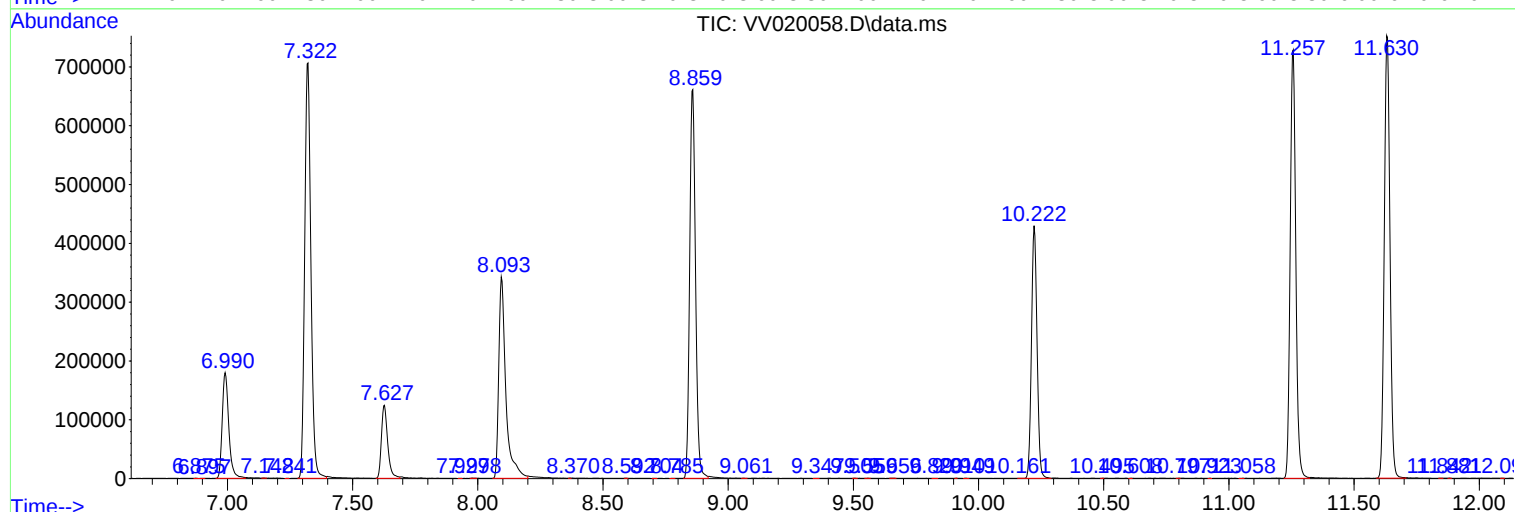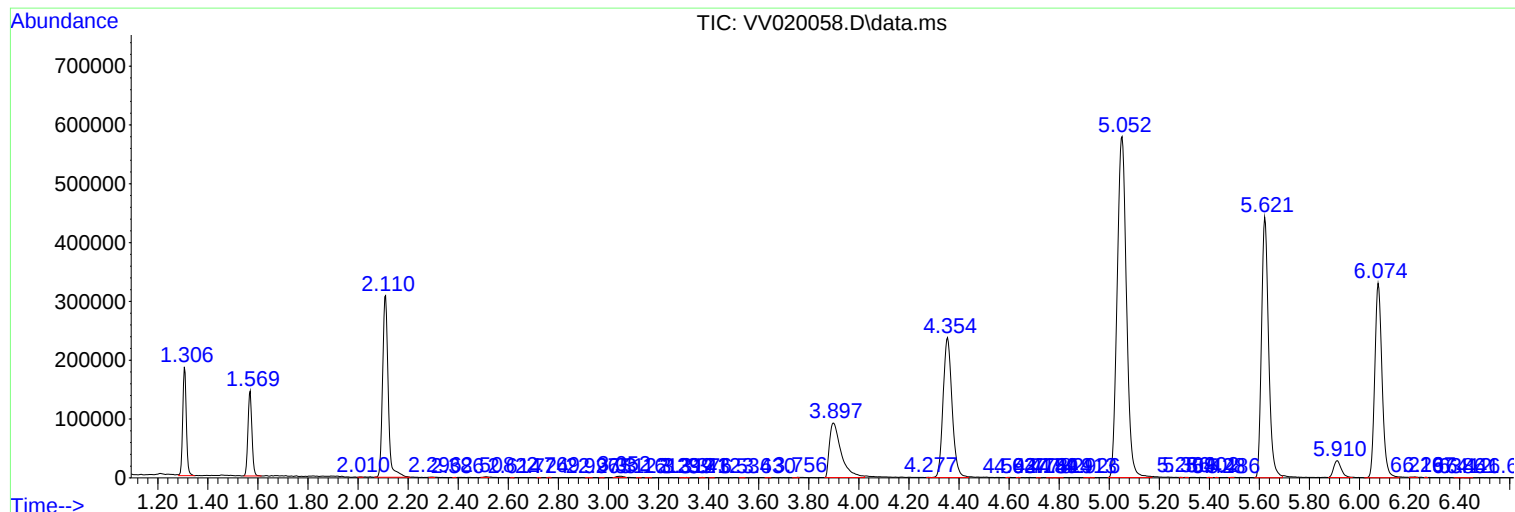

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020058.D
Acq On : 19 Jan 2021 18:21
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020058.D
Acq On : 19 Jan 2021 18:21
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
