

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020060.D
 Acq On : 19 Jan 2021 19:08
 Operator : SY/MD
 Sample : M1173-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	60	68	83	rVB	200312	199853	12.42%	1.619%
2	1.383	88	91	92	rBV	1319	770	0.05%	0.006%
3	1.569	140	149	163	rBV	147560	168348	10.46%	1.363%
4	1.827	228	229	233	rBV4	630	292	0.02%	0.002%
5	1.965	270	272	277	rBV4	623	484	0.03%	0.004%
6	2.110	306	317	335	rBV	339493	510740	31.73%	4.136%
7	2.296	372	375	378	rBV3	652	492	0.03%	0.004%
8	2.322	381	383	384	rBV	566	257	0.02%	0.002%
9	2.621	470	476	478	rBV3	410	461	0.03%	0.004%
10	2.730	507	510	517	rVB3	570	490	0.03%	0.004%
11	2.772	517	523	526	rVB2	408	359	0.02%	0.003%
12	2.885	552	558	559	rBV	322	300	0.02%	0.002%
13	2.920	566	569	574	rVB2	330	277	0.02%	0.002%
14	2.962	575	582	583	rBV	432	273	0.02%	0.002%
15	2.971	583	585	594	rVB2	357	405	0.03%	0.003%
16	3.036	601	605	607	rBV4	1120	923	0.06%	0.007%
17	3.177	643	649	652	rBV2	404	324	0.02%	0.003%
18	3.524	751	757	759	rBV2	207	224	0.01%	0.002%
19	3.647	789	795	799	rBV	329	399	0.02%	0.003%
20	3.775	830	835	841	rVB3	497	480	0.03%	0.004%
21	3.894	860	872	918	rBV	106742	327715	20.36%	2.654%
22	4.097	928	935	936	rBV4	3532	3688	0.23%	0.030%
23	4.254	982	984	989	rVB2	372	218	0.01%	0.002%
24	4.354	999	1015	1042	rBV	258485	635162	39.46%	5.144%
25	4.508	1061	1063	1067	rBV4	487	299	0.02%	0.002%
26	4.528	1067	1069	1074	rVB3	700	497	0.03%	0.004%
27	4.614	1092	1096	1099	rVB3	462	344	0.02%	0.003%
28	4.685	1115	1118	1124	rVB3	405	341	0.02%	0.003%
29	4.881	1177	1179	1184	rVB	329	239	0.01%	0.002%
30	5.052	1215	1232	1265	rBV2	624488	1609749	100.00%	13.037%
31	5.367	1327	1330	1334	rVB2	422	285	0.02%	0.002%
32	5.515	1374	1376	1381	rVB	380	272	0.02%	0.002%
33	5.540	1381	1384	1388	rBV2	397	345	0.02%	0.003%
34	5.621	1396	1409	1442	rBV	478143	964785	59.93%	7.813%
35	5.910	1487	1499	1520	rBV3	41931	85677	5.32%	0.694%
36	6.074	1535	1550	1577	rVV	355152	717532	44.57%	5.811%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020060.D
 Acq On : 19 Jan 2021 19:08
 Operator : SY/MD
 Sample : M1173-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.338	1625	1632	1637	rBV2	456	453	0.03%	0.004%
38	6.544	1691	1696	1703	rBV3	680	921	0.06%	0.007%
39	6.990	1821	1835	1859	rBV	199002	359001	22.30%	2.907%
40	7.135	1877	1880	1882	rBV2	671	493	0.03%	0.004%
41	7.196	1895	1899	1901	rVB3	381	258	0.02%	0.002%
42	7.322	1924	1938	1969	rBV	759638	1326398	82.40%	10.742%
43	7.470	1981	1984	1987	rBV2	447	289	0.02%	0.002%
44	7.627	2021	2033	2060	rVV	135567	238832	14.84%	1.934%
45	7.820	2090	2093	2095	rVB	453	285	0.02%	0.002%
46	7.949	2127	2133	2135	rBV2	411	474	0.03%	0.004%
47	7.987	2141	2145	2151	rBV4	850	849	0.05%	0.007%
48	8.093	2167	2178	2223	rBV2	346042	715403	44.44%	5.794%
49	8.331	2249	2252	2255	rBV2	322	283	0.02%	0.002%
50	8.360	2258	2261	2263	rVB3	545	269	0.02%	0.002%
51	8.453	2286	2290	2293	rVB2	354	229	0.01%	0.002%
52	8.495	2296	2303	2306	rBV3	415	469	0.03%	0.004%
53	8.515	2306	2309	2313	rVV	280	237	0.01%	0.002%
54	8.537	2313	2316	2320	rVB2	340	272	0.02%	0.002%
55	8.579	2325	2329	2331	rBV	449	278	0.02%	0.002%
56	8.598	2333	2335	2340	rBV2	437	243	0.02%	0.002%
57	8.743	2377	2380	2383	rVB	369	246	0.02%	0.002%
58	8.762	2383	2386	2390	rVB	553	336	0.02%	0.003%
59	8.801	2396	2398	2401	rBV2	343	254	0.02%	0.002%
60	8.859	2404	2416	2442	rBV	729558	1193897	74.17%	9.669%
61	9.084	2484	2486	2493	rVB2	319	247	0.02%	0.002%
62	9.151	2504	2507	2510	rBV2	558	356	0.02%	0.003%
63	9.296	2549	2552	2553	rBV	357	252	0.02%	0.002%
64	9.560	2631	2634	2639	rVB2	390	291	0.02%	0.002%
65	9.666	2661	2667	2672	rBV2	317	419	0.03%	0.003%
66	9.942	2749	2753	2761	rBV3	520	555	0.03%	0.004%
67	10.026	2774	2779	2780	rBV3	1912	1434	0.09%	0.012%
68	10.125	2804	2810	2813	rBV2	246	283	0.02%	0.002%
69	10.222	2828	2840	2861	rBV	433805	681396	42.33%	5.518%
70	10.392	2886	2893	2903	rVB4	1385	2144	0.13%	0.017%
71	10.547	2940	2941	2949	rVB2	419	433	0.03%	0.004%
72	10.588	2949	2954	2957	rBV4	475	457	0.03%	0.004%
73	10.794	3015	3018	3023	rBV2	211	256	0.02%	0.002%
74	10.932	3056	3061	3068	rVV2	429	487	0.03%	0.004%
75	11.196	3139	3143	3148	rVB3	591	541	0.03%	0.004%
76	11.254	3149	3161	3185	rBV	805141	1257481	78.12%	10.184%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020060.D
 Acq On : 19 Jan 2021 19:08
 Operator : SY/MD
 Sample : M1173-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	11.543	3243	3251	3264	rVV4	5997	10791	0.67%	0.087%
78	11.630	3264	3278	3299	rBV	825964	1307087	81.20%	10.585%
79	11.768	3319	3321	3328	rVB3	615	448	0.03%	0.004%
80	11.801	3328	3331	3337	rVB2	683	496	0.03%	0.004%
81	11.836	3340	3342	3346	rBV2	403	247	0.02%	0.002%
82	11.878	3352	3355	3358	rBV2	329	271	0.02%	0.002%
83	11.910	3361	3365	3370	rVB2	396	407	0.03%	0.003%
84	12.032	3399	3403	3404	rBV	386	225	0.01%	0.002%
85	12.360	3498	3505	3511	rBV4	1176	1683	0.10%	0.014%
86	12.431	3524	3527	3528	rBV	419	275	0.02%	0.002%
87	12.662	3597	3599	3602	rBV	436	269	0.02%	0.002%
88	12.759	3626	3629	3632	rBV	421	276	0.02%	0.002%
89	12.833	3648	3652	3655	rVB2	473	364	0.02%	0.003%
90	12.858	3655	3660	3662	rBV2	422	392	0.02%	0.003%
91	12.884	3665	3668	3673	rVV2	279	245	0.02%	0.002%
92	13.112	3737	3739	3744	rBV	372	271	0.02%	0.002%
93	13.180	3757	3760	3764	rBV2	328	297	0.02%	0.002%
94	13.559	3875	3878	3880	rBV2	326	234	0.01%	0.002%
95	13.707	3922	3924	3931	rVB2	490	393	0.02%	0.003%
96	13.759	3937	3940	3943	rBV3	782	615	0.04%	0.005%
97	14.106	4045	4048	4055	rBV4	431	645	0.04%	0.005%
98	14.476	4161	4163	4166	rBV	431	225	0.01%	0.002%
99	15.453	4463	4467	4471	rBV2	586	614	0.04%	0.005%
100	15.489	4476	4478	4480	rBV	509	231	0.01%	0.002%

Sum of corrected areas: 12348001




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020060.D
Acq On : 19 Jan 2021 19:08
Operator : SY/MD
Sample : M1173-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

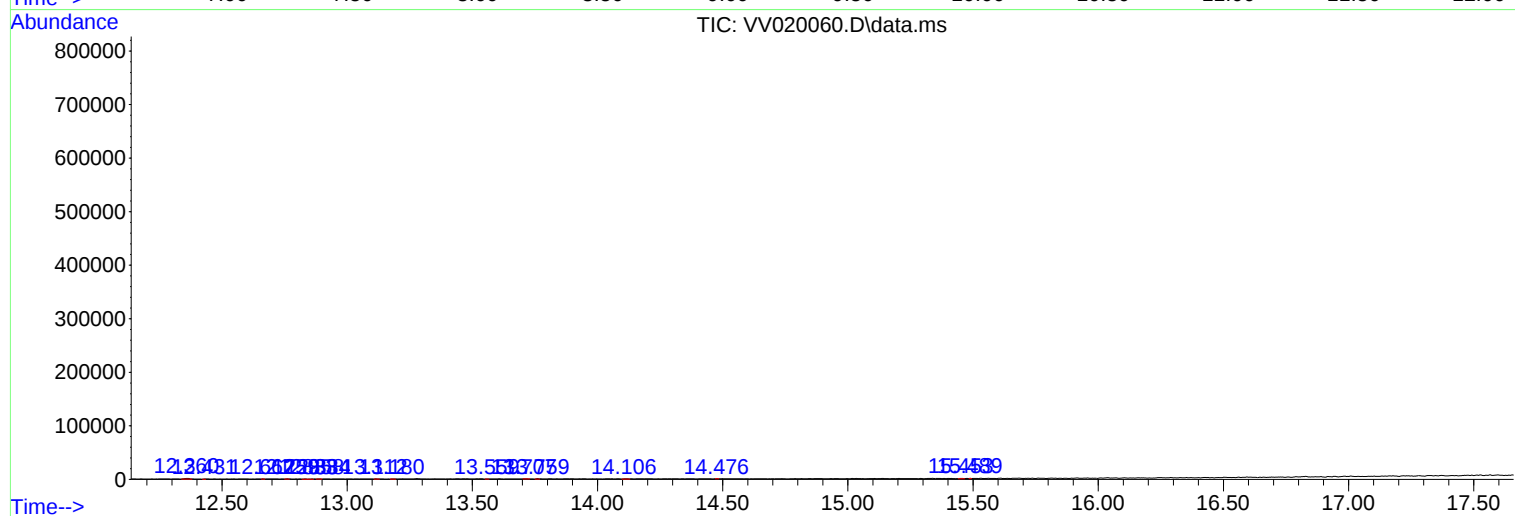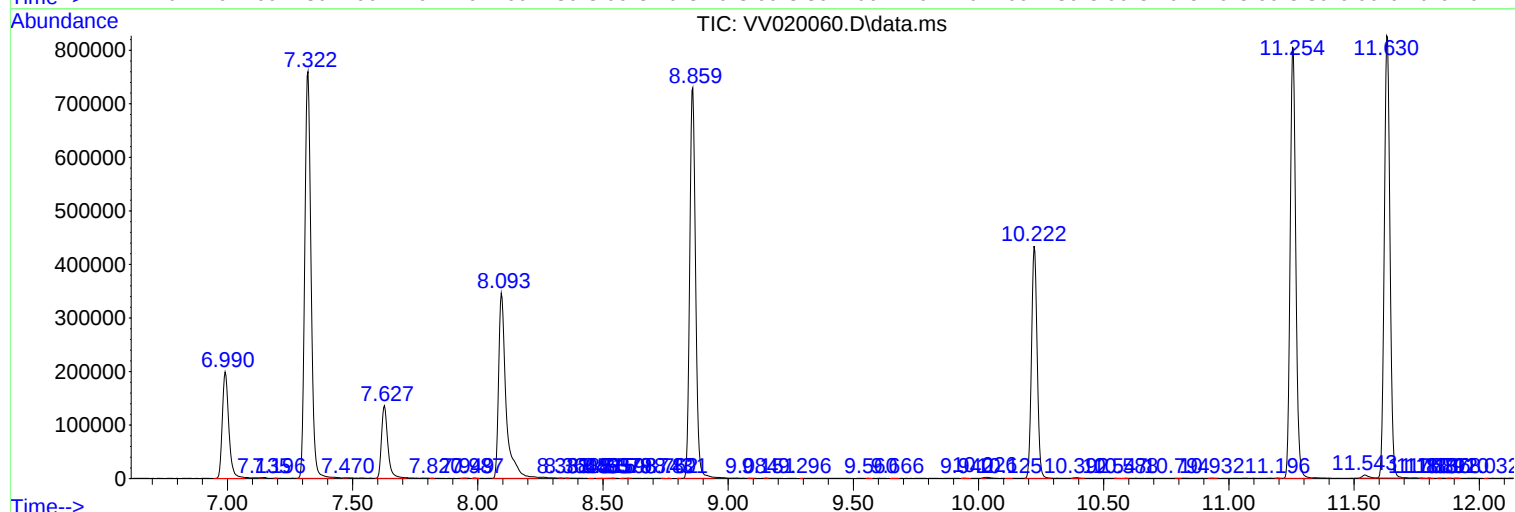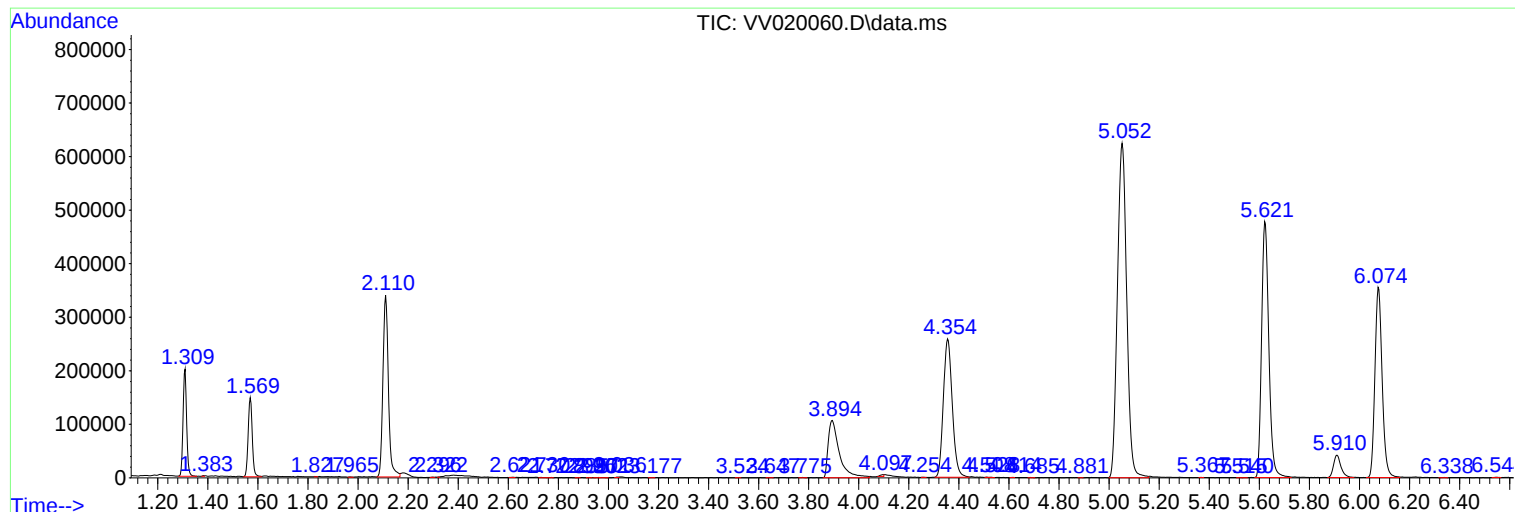

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020060.D
Acq On : 19 Jan 2021 19:08
Operator : SY/MD
Sample : M1173-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020060.D
Acq On : 19 Jan 2021 19:08
Operator : SY/MD
Sample : M1173-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
