

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020062.D
 Acq On : 19 Jan 2021 19:55
 Operator : SY/MD
 Sample : M1173-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	190207	188643	12.17%	1.576%
2	1.569	141	149	163	rBV	155521	170013	10.97%	1.421%
3	1.801	219	221	226	rVB4	980	767	0.05%	0.006%
4	1.975	272	275	280	rBV3	538	527	0.03%	0.004%
5	2.110	305	317	354	rBV	327973	501898	32.39%	4.194%
6	2.299	369	376	381	rBV3	809	1121	0.07%	0.009%
7	2.380	397	401	402	rBV2	1352	980	0.06%	0.008%
8	2.611	469	473	475	rBV3	1339	1225	0.08%	0.010%
9	2.624	475	477	486	rVB4	2951	3445	0.22%	0.029%
10	2.717	503	506	509	rVB2	367	252	0.02%	0.002%
11	2.862	543	551	553	rBV3	364	428	0.03%	0.004%
12	2.968	574	584	588	rBV3	1157	1650	0.11%	0.014%
13	3.049	602	609	614	rVV4	910	1145	0.07%	0.010%
14	3.434	727	729	734	rVB2	219	208	0.01%	0.002%
15	3.904	860	875	917	rBV2	100508	377634	24.37%	3.156%
16	4.094	926	934	960	rVB2	12371	33232	2.14%	0.278%
17	4.354	998	1015	1041	rBV	250342	616691	39.79%	5.154%
18	4.640	1101	1104	1110	rVB2	245	232	0.01%	0.002%
19	4.672	1111	1114	1117	rBV2	329	212	0.01%	0.002%
20	4.730	1127	1132	1135	rBV2	307	216	0.01%	0.002%
21	4.872	1171	1176	1179	rBV2	272	217	0.01%	0.002%
22	4.929	1189	1194	1198	rBV2	357	288	0.02%	0.002%
23	4.955	1198	1202	1205	rBV	227	209	0.01%	0.002%
24	5.052	1214	1232	1264	rBV2	610311	1549676	100.00%	12.950%
25	5.319	1313	1315	1319	rVB2	432	284	0.02%	0.002%
26	5.444	1351	1354	1356	rBV	314	202	0.01%	0.002%
27	5.524	1373	1379	1384	rBV2	268	256	0.02%	0.002%
28	5.550	1384	1387	1393	rBV4	365	483	0.03%	0.004%
29	5.621	1396	1409	1438	rBV	463920	920605	59.41%	7.693%
30	5.910	1488	1499	1516	rBV	38326	78566	5.07%	0.657%
31	6.074	1535	1550	1575	rBV	338543	692146	44.66%	5.784%
32	6.209	1590	1592	1596	rBV3	886	561	0.04%	0.005%
33	6.293	1616	1618	1621	rBV2	373	208	0.01%	0.002%
34	6.556	1696	1700	1702	rBV2	309	220	0.01%	0.002%
35	6.650	1727	1729	1734	rVB2	325	277	0.02%	0.002%
36	6.753	1759	1761	1765	rVB3	324	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020062.D
 Acq On : 19 Jan 2021 19:55
 Operator : SY/MD
 Sample : M1173-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.817	1778	1781	1786	rVB2	328	317	0.02%	0.003%
38	6.990	1824	1835	1862	rBV	191585	342954	22.13%	2.866%
39	7.142	1873	1882	1895	rVB5	5173	9938	0.64%	0.083%
40	7.203	1899	1901	1905	rVB	456	335	0.02%	0.003%
41	7.322	1924	1938	1967	rBV	735052	1269015	81.89%	10.605%
42	7.585	2017	2020	2022	rBV	350	281	0.02%	0.002%
43	7.627	2022	2033	2068	rVV	130706	231721	14.95%	1.936%
44	7.936	2126	2129	2131	rBV2	285	210	0.01%	0.002%
45	7.978	2137	2142	2145	rBV3	504	446	0.03%	0.004%
46	8.093	2168	2178	2219	rBV2	330779	675962	43.62%	5.649%
47	8.376	2263	2266	2271	rVB2	472	411	0.03%	0.003%
48	8.431	2277	2283	2284	rBV2	527	360	0.02%	0.003%
49	8.482	2296	2299	2303	rVV2	289	233	0.02%	0.002%
50	8.524	2309	2312	2315	rVB	382	258	0.02%	0.002%
51	8.550	2315	2320	2323	rBV3	424	379	0.02%	0.003%
52	8.720	2369	2373	2377	rVB	386	273	0.02%	0.002%
53	8.801	2395	2398	2402	rBV2	327	214	0.01%	0.002%
54	8.859	2404	2416	2444	rBV	698431	1134110	73.18%	9.477%
55	9.023	2464	2467	2473	rVB2	693	668	0.04%	0.006%
56	9.055	2473	2477	2479	rBV2	331	272	0.02%	0.002%
57	9.132	2499	2501	2505	rVB	452	255	0.02%	0.002%
58	9.183	2514	2517	2522	rVB3	340	274	0.02%	0.002%
59	9.267	2536	2543	2547	rVB2	233	291	0.02%	0.002%
60	9.293	2547	2551	2554	rBV2	264	249	0.02%	0.002%
61	9.344	2564	2567	2570	rVV2	247	192	0.01%	0.002%
62	9.469	2599	2606	2612	rBV2	274	409	0.03%	0.003%
63	9.502	2612	2616	2620	rBV	262	212	0.01%	0.002%
64	10.222	2824	2840	2861	rBV	424576	660751	42.64%	5.522%
65	10.527	2930	2935	2939	rBV	261	326	0.02%	0.003%
66	10.553	2940	2943	2947	rVV2	391	265	0.02%	0.002%
67	10.894	3042	3049	3051	rBV2	251	335	0.02%	0.003%
68	10.932	3054	3061	3063	rBV2	470	480	0.03%	0.004%
69	11.129	3118	3122	3127	rBV	264	278	0.02%	0.002%
70	11.190	3137	3141	3150	rVB3	639	836	0.05%	0.007%
71	11.254	3150	3161	3183	rBV	781823	1207145	77.90%	10.088%
72	11.421	3211	3213	3216	rVB2	382	203	0.01%	0.002%
73	11.547	3244	3252	3261	rBV5	2291	4285	0.28%	0.036%
74	11.633	3266	3279	3302	rBV	804456	1265662	81.67%	10.577%
75	11.887	3355	3358	3363	rBV3	354	397	0.03%	0.003%
76	12.010	3394	3396	3401	rVB2	274	205	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020062.D
 Acq On : 19 Jan 2021 19:55
 Operator : SY/MD
 Sample : M1173-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	12.035	3401	3404	3407	rBV	368	298	0.02%	0.002%
78	12.051	3407	3409	3413	rVB3	363	228	0.01%	0.002%
79	12.100	3420	3424	3427	rBV2	417	381	0.02%	0.003%
80	12.321	3489	3493	3499	rVB2	421	345	0.02%	0.003%
81	12.485	3536	3544	3545	rBV	377	454	0.03%	0.004%
82	12.579	3572	3573	3580	rVB2	282	248	0.02%	0.002%
83	12.614	3580	3584	3586	rBV	264	227	0.01%	0.002%
84	12.656	3593	3597	3598	rBV2	511	344	0.02%	0.003%
85	12.797	3635	3641	3643	rBV	396	416	0.03%	0.003%
86	12.913	3674	3677	3680	rBV	476	335	0.02%	0.003%
87	13.032	3711	3714	3717	rBV	381	239	0.02%	0.002%
88	13.112	3735	3739	3743	rBV	558	485	0.03%	0.004%
89	13.138	3743	3747	3750	rVB2	382	270	0.02%	0.002%
90	13.280	3784	3791	3793	rBV3	635	823	0.05%	0.007%
91	13.701	3918	3922	3927	rBV2	488	487	0.03%	0.004%
92	13.755	3936	3939	3943	rBV3	504	426	0.03%	0.004%
93	13.852	3966	3969	3971	rBV2	445	245	0.02%	0.002%
94	14.038	4024	4027	4034	rVB2	614	485	0.03%	0.004%
95	14.135	4054	4057	4061	rBV2	453	447	0.03%	0.004%
96	14.331	4115	4118	4120	rBV3	343	238	0.02%	0.002%
97	14.421	4142	4146	4148	rBV	595	426	0.03%	0.004%
98	14.913	4297	4299	4305	rVB3	380	275	0.02%	0.002%
99	15.556	4495	4499	4505	rBV4	793	1012	0.07%	0.008%
100	15.826	4578	4583	4586	rBV3	826	894	0.06%	0.007%




Sum of corrected areas: 11966364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020062.D
Acq On : 19 Jan 2021 19:55
Operator : SY/MD
Sample : M1173-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

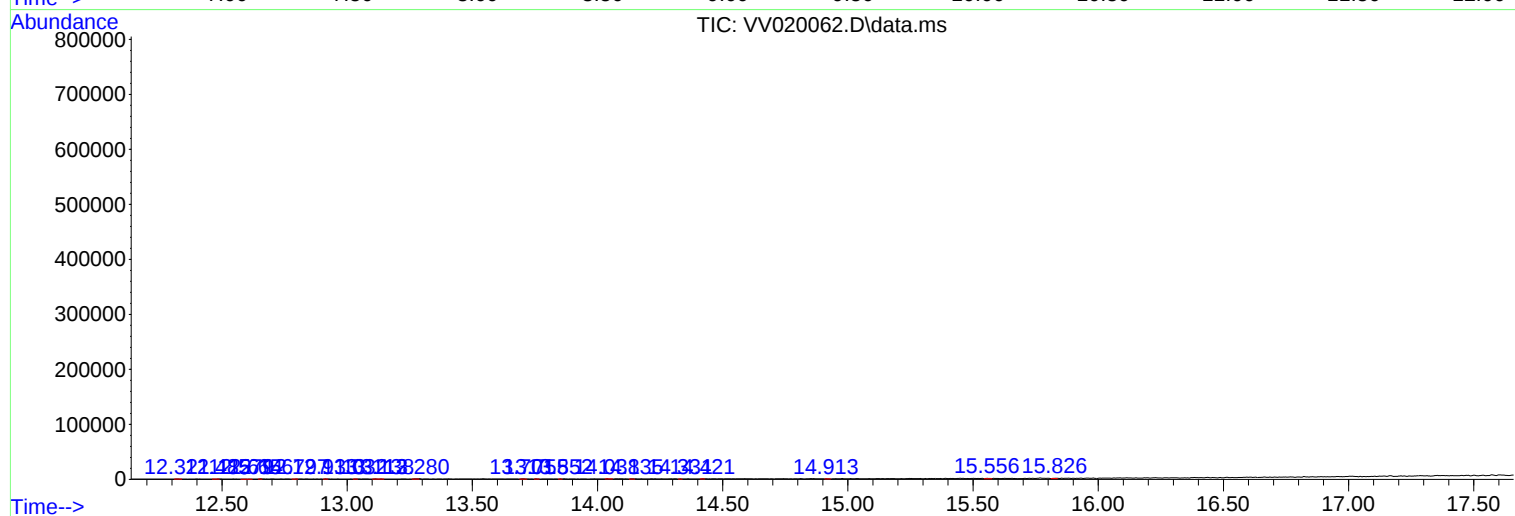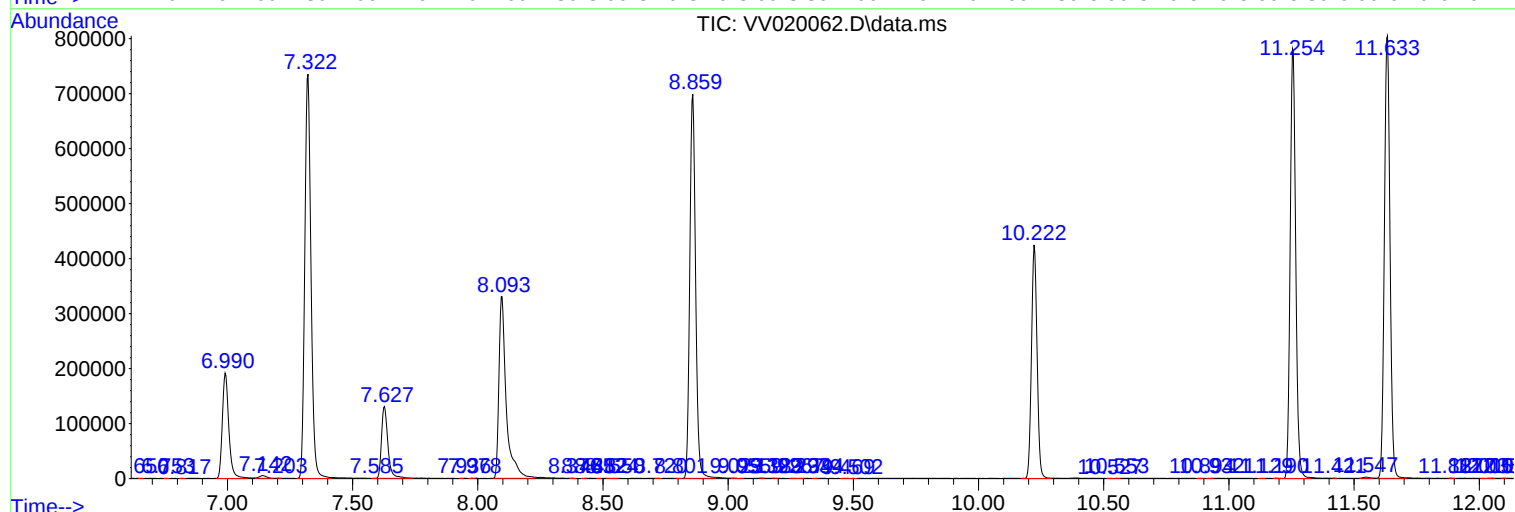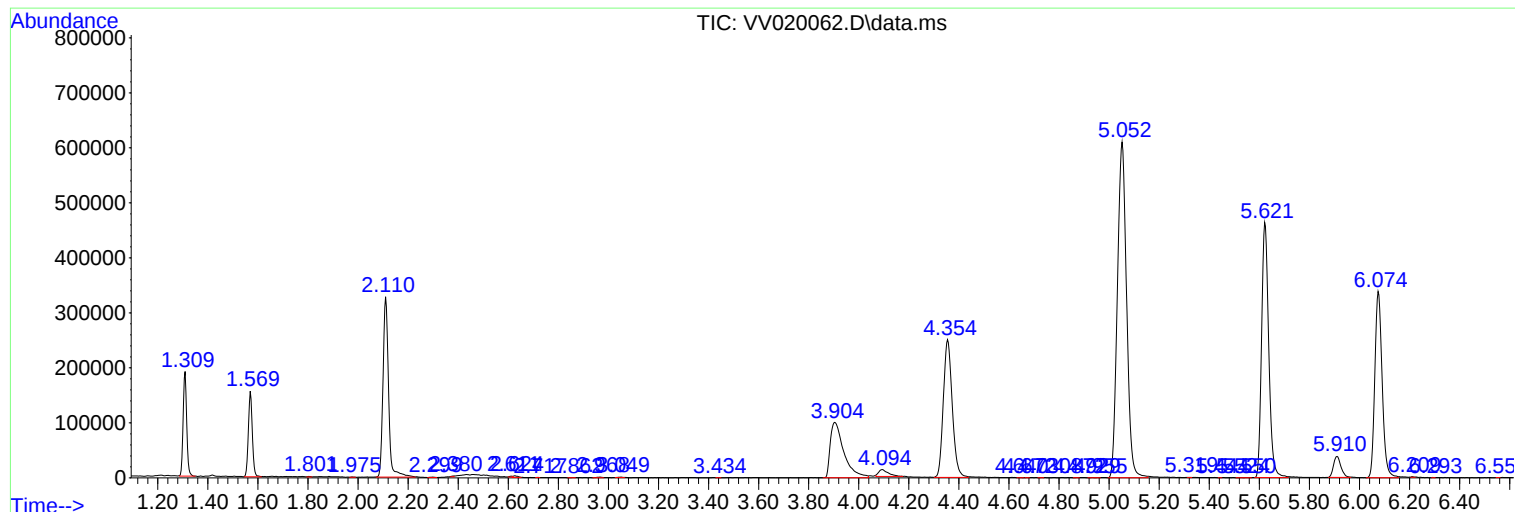

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020062.D
Acq On : 19 Jan 2021 19:55
Operator : SY/MD
Sample : M1173-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020062.D
Acq On : 19 Jan 2021 19:55
Operator : SY/MD
Sample : M1173-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
