

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020063.D
 Acq On : 19 Jan 2021 20:19
 Operator : SY/MD
 Sample : M1173-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	186968	185011	12.26%	1.593%
2	1.570	142	149	161	rVB	143039	159013	10.54%	1.369%
3	2.110	307	317	354	rVB	329280	499739	33.13%	4.302%
4	2.798	528	531	533	rBV2	305	212	0.01%	0.002%
5	2.849	545	547	553	rVB2	325	200	0.01%	0.002%
6	2.878	553	556	561	rBV2	173	174	0.01%	0.001%
7	2.946	574	577	580	rBV2	371	223	0.01%	0.002%
8	2.991	588	591	594	rBV2	230	151	0.01%	0.001%
9	3.013	594	598	601	rBV	257	241	0.02%	0.002%
10	3.052	602	610	616	rVV3	648	1031	0.07%	0.009%
11	3.123	628	632	633	rBV2	481	365	0.02%	0.003%
12	3.229	659	665	668	rBV2	328	373	0.02%	0.003%
13	3.312	687	691	695	rVB	328	279	0.02%	0.002%
14	3.328	695	696	697	rBV	135	37	0.00%	0.000%
15	3.344	697	701	703	rBV	164	120	0.01%	0.001%
16	3.457	735	736	740	rVB	158	110	0.01%	0.001%
17	3.483	740	744	750	rBV2	274	376	0.02%	0.003%
18	3.528	755	758	759	rBV	161	97	0.01%	0.001%
19	3.614	782	785	787	rBV	219	151	0.01%	0.001%
20	3.631	788	790	791	rBV	195	70	0.00%	0.001%
21	3.669	799	802	806	rVB2	188	112	0.01%	0.001%
22	3.743	819	825	828	rBV2	296	368	0.02%	0.003%
23	3.897	861	873	914	rBV2	113912	380068	25.19%	3.272%
24	4.354	998	1015	1041	rBV2	245918	604765	40.09%	5.206%
25	4.589	1086	1088	1092	rBV3	387	260	0.02%	0.002%
26	4.688	1116	1119	1120	rBV2	306	167	0.01%	0.001%
27	4.701	1120	1123	1126	rVB	280	134	0.01%	0.001%
28	4.721	1127	1129	1131	rVV2	295	107	0.01%	0.001%
29	4.733	1131	1133	1136	rVB	191	105	0.01%	0.001%
30	4.749	1136	1138	1140	rVB	253	102	0.01%	0.001%
31	4.766	1140	1143	1144	rBV	247	175	0.01%	0.002%
32	4.852	1166	1170	1172	rBV	147	139	0.01%	0.001%
33	4.885	1178	1180	1181	rBV	140	47	0.00%	0.000%
34	4.926	1189	1193	1200	rBV2	384	505	0.03%	0.004%
35	5.052	1214	1232	1274	rBV2	589976	1508550	100.00%	12.986%
36	5.338	1320	1321	1322	rBV2	268	90	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020063.D
 Acq On : 19 Jan 2021 20:19
 Operator : SY/MD
 Sample : M1173-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.418	1344	1346	1349	rVB2	414	173	0.01%	0.001%
38	5.473	1362	1363	1364	rBV	139	31	0.00%	0.000%
39	5.483	1364	1366	1369	rVV	267	193	0.01%	0.002%
40	5.505	1369	1373	1376	rVB2	286	184	0.01%	0.002%
41	5.563	1383	1391	1392	rBV2	451	538	0.04%	0.005%
42	5.621	1397	1409	1434	rBV	446996	888700	58.91%	7.650%
43	5.907	1487	1498	1518	rBV3	35454	74584	4.94%	0.642%
44	6.074	1536	1550	1575	rBV	328698	672468	44.58%	5.789%
45	6.360	1636	1639	1641	rBV2	271	222	0.01%	0.002%
46	6.386	1645	1647	1648	rBV2	359	159	0.01%	0.001%
47	6.444	1663	1665	1667	rVB	167	70	0.00%	0.001%
48	6.466	1667	1672	1677	rBV2	348	410	0.03%	0.004%
49	6.528	1688	1691	1693	rBV	302	168	0.01%	0.001%
50	6.582	1705	1708	1710	rBV2	302	243	0.02%	0.002%
51	6.782	1767	1770	1772	rVB2	206	101	0.01%	0.001%
52	6.830	1781	1785	1791	rBV3	250	265	0.02%	0.002%
53	6.888	1801	1803	1804	rBV	137	71	0.00%	0.001%
54	6.952	1819	1823	1824	rBV2	249	175	0.01%	0.002%
55	6.991	1824	1835	1859	rVV	186620	332916	22.07%	2.866%
56	7.216	1902	1905	1906	rBV	325	148	0.01%	0.001%
57	7.238	1911	1912	1915	rBV	195	97	0.01%	0.001%
58	7.251	1915	1916	1921	rBV3	357	253	0.02%	0.002%
59	7.322	1925	1938	1968	rBV	711879	1236081	81.94%	10.641%
60	7.627	2022	2033	2050	rBV	128153	223149	14.79%	1.921%
61	7.810	2087	2090	2097	rVB3	258	277	0.02%	0.002%
62	7.926	2119	2126	2127	rBV3	518	348	0.02%	0.003%
63	7.984	2138	2144	2146	rBV4	699	625	0.04%	0.005%
64	8.055	2159	2166	2168	rBV2	246	330	0.02%	0.003%
65	8.093	2168	2178	2213	rBV2	332403	670818	44.47%	5.775%
66	8.740	2376	2379	2381	rBV2	201	130	0.01%	0.001%
67	8.807	2396	2400	2402	rVB	233	161	0.01%	0.001%
68	8.859	2402	2416	2436	rBV	676408	1104417	73.21%	9.507%
69	9.566	2634	2636	2641	rBV2	163	170	0.01%	0.001%
70	9.592	2641	2644	2647	rVB2	241	174	0.01%	0.001%
71	9.614	2647	2651	2658	rBV2	358	565	0.04%	0.005%
72	9.749	2689	2693	2694	rBV2	257	151	0.01%	0.001%
73	9.875	2728	2732	2734	rBV	268	221	0.01%	0.002%
74	9.936	2747	2751	2752	rBV	348	246	0.02%	0.002%
75	10.103	2802	2803	2804	rBV	272	63	0.00%	0.001%
76	10.222	2828	2840	2861	rBV	423791	653904	43.35%	5.629%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020063.D
 Acq On : 19 Jan 2021 20:19
 Operator : SY/MD
 Sample : M1173-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.553	2941	2943	2948	rVB	267	219	0.01%	0.002%
78	10.598	2954	2957	2961	rBV	228	147	0.01%	0.001%
79	10.704	2986	2990	2993	rBV	397	354	0.02%	0.003%
80	10.862	3037	3039	3043	rBV	255	172	0.01%	0.001%
81	11.035	3091	3093	3095	rBV	191	116	0.01%	0.001%
82	11.187	3137	3140	3142	rBV	304	200	0.01%	0.002%
83	11.254	3150	3161	3191	rBV	766671	1176327	77.98%	10.127%
84	11.550	3246	3253	3257	rBV4	1934	2562	0.17%	0.022%
85	11.630	3266	3278	3298	rBV	780135	1227348	81.36%	10.566%
86	11.788	3323	3327	3331	rBV3	519	501	0.03%	0.004%
87	12.109	3425	3427	3429	rBV	190	100	0.01%	0.001%
88	12.649	3592	3595	3597	rBV	374	276	0.02%	0.002%
89	12.949	3686	3688	3693	rBV2	324	327	0.02%	0.003%




Sum of corrected areas: 11616315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020063.D
Acq On : 19 Jan 2021 20:19
Operator : SY/MD
Sample : M1173-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

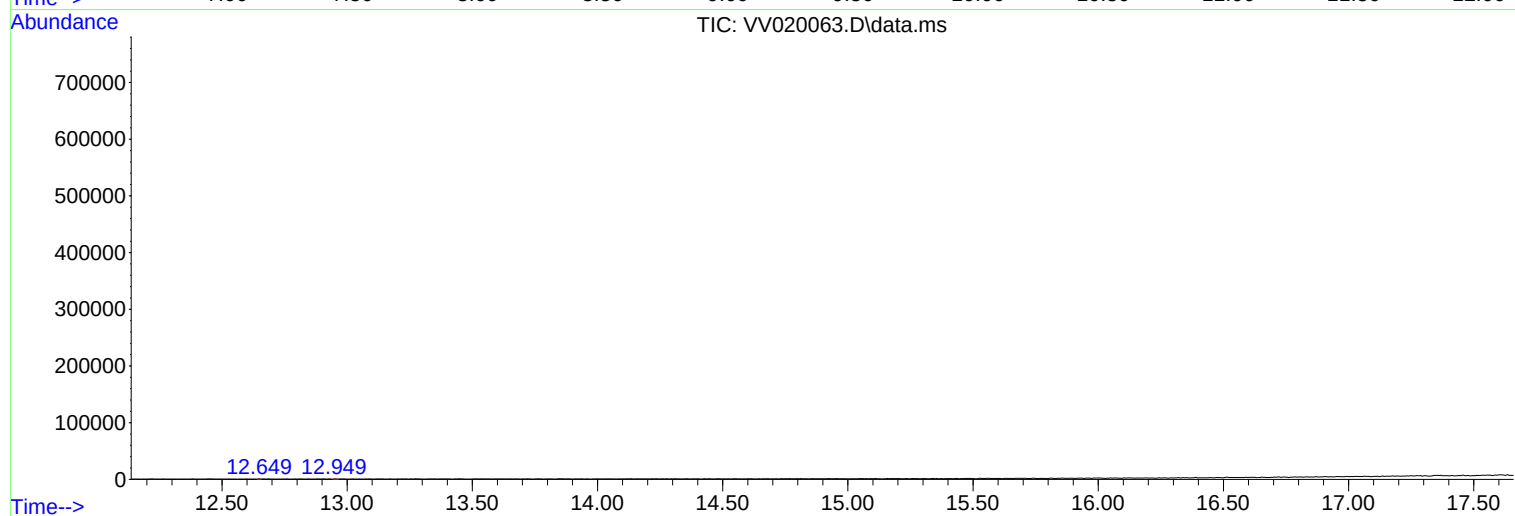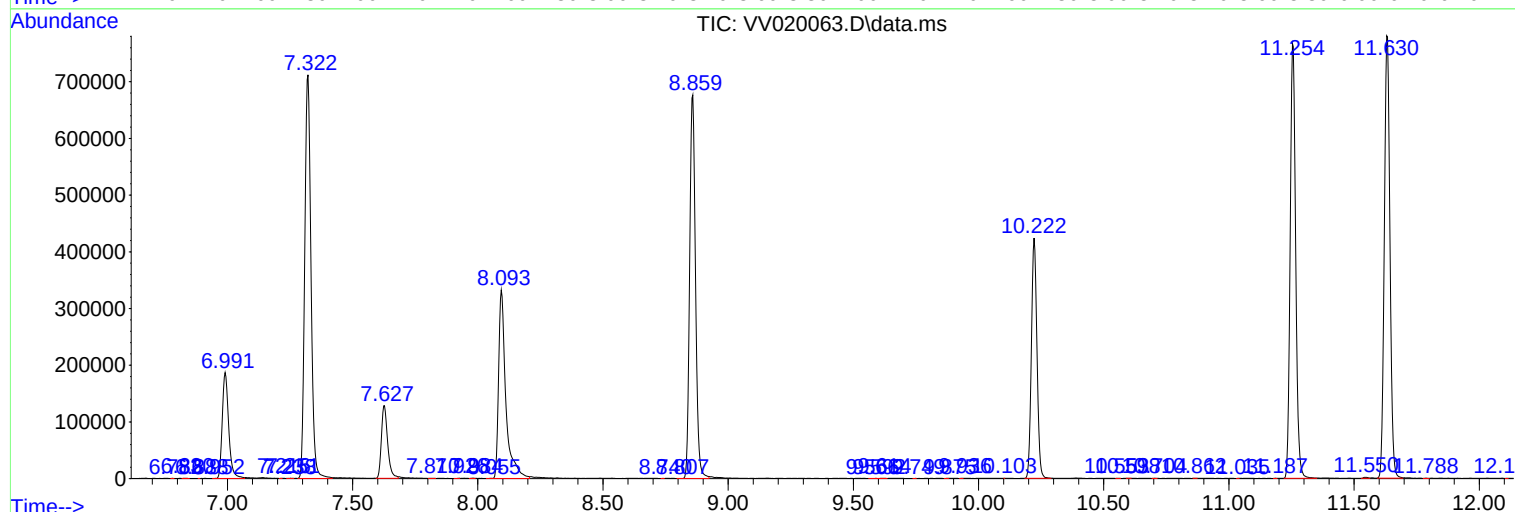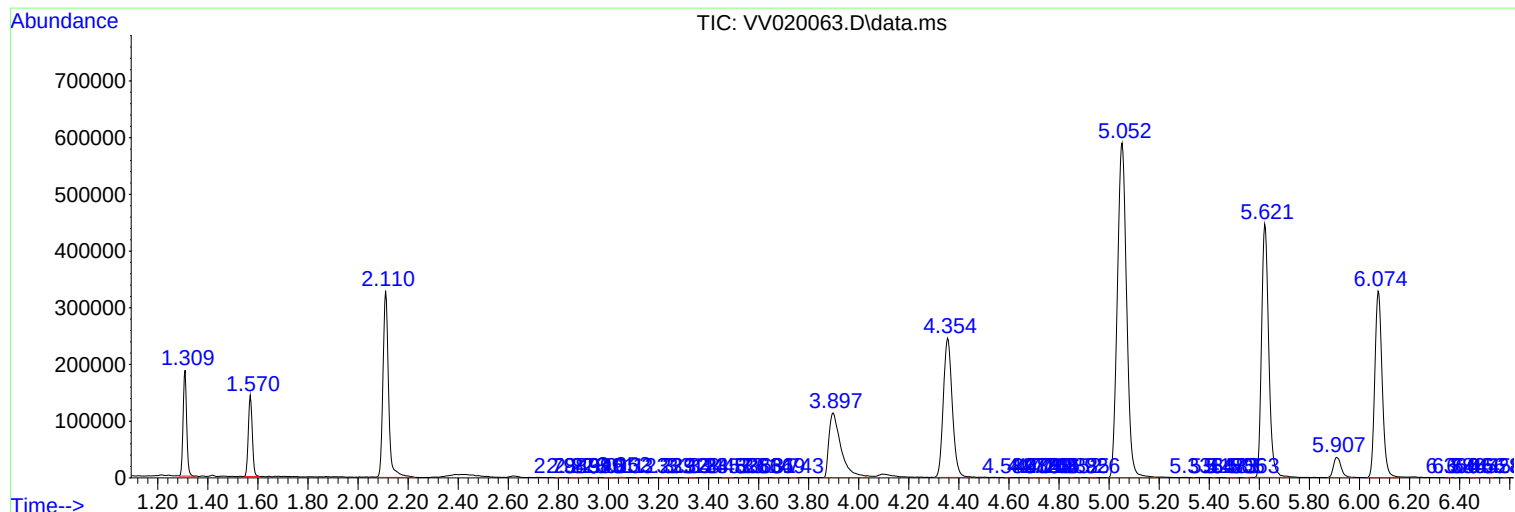

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020063.D
Acq On : 19 Jan 2021 20:19
Operator : SY/MD
Sample : M1173-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
Data File : VV020063.D
Acq On : 19 Jan 2021 20:19
Operator : SY/MD
Sample : M1173-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
