
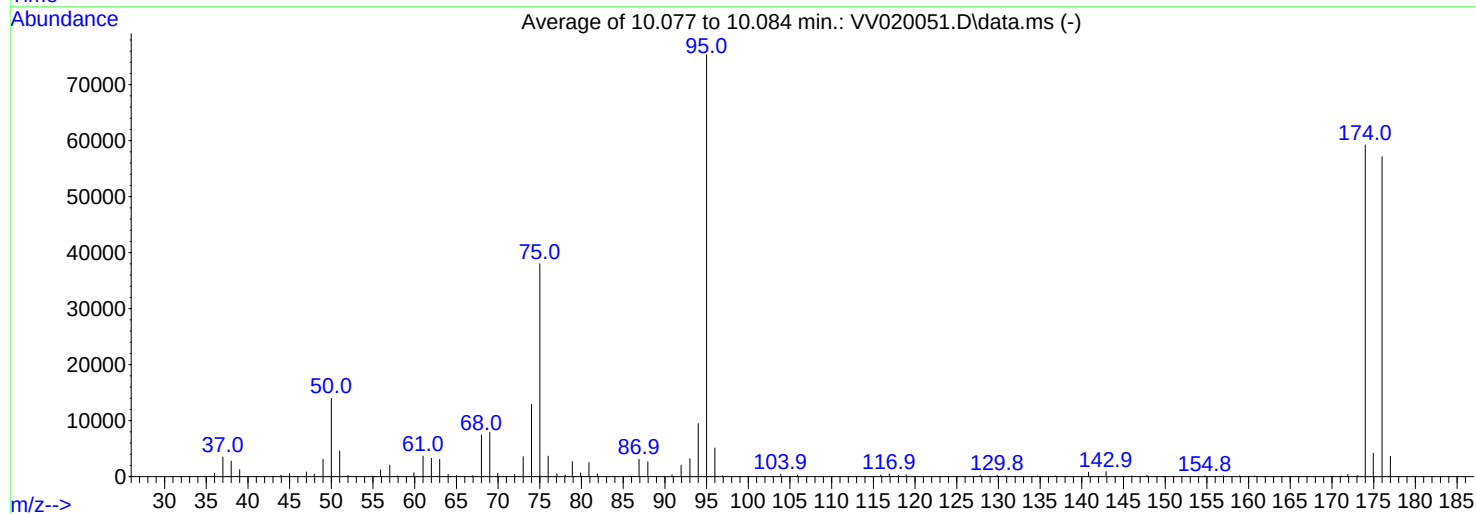


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011921\
 Data File : VV020051.D
 Acq On : 19 Jan 2021 12:50
 Operator : SY/MD
 Sample : BFB83
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 20 01:05:37 2021

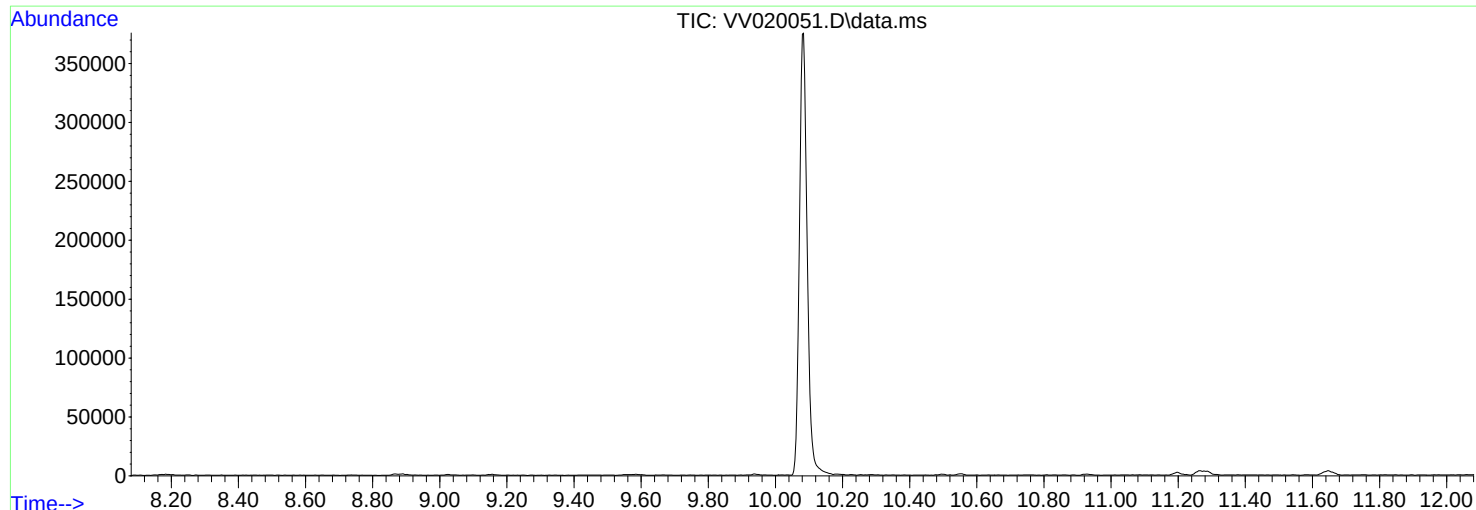

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	13976	PASS
75	95	30	80	50.5	38024	PASS
95	95	100	100	100.0	75333	PASS
96	95	5	9	6.8	5106	PASS
173	174	0.00	2	0.3	205	PASS
174	95	50	120	78.6	59248	PASS
175	174	5	9	7.1	4182	PASS
176	174	95	101	96.5	57155	PASS
177	176	5	9	6.4	3635	PASS

m/z	Abundance
39.90	153.0
44.00	497.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	579.0
37.00	3414.0
38.00	2653.0
39.00	1269.0
39.90	231.0
44.00	818.0
45.00	555.0
47.00	840.0
47.90	415.0
49.00	2987.0
50.00	13281.0
51.00	4539.0
52.00	237.0
55.90	1123.0
57.00	1799.0
57.90	129.0
59.90	650.0
61.00	3442.0
62.00	3064.0
63.00	2904.0
64.00	427.0
64.90	148.0
66.90	169.0
68.00	7050.0
69.00	7687.0
70.00	527.0
72.00	376.0
73.00	3205.0
74.00	11994.0
75.00	35496.0
76.00	3389.0
77.00	445.0
78.00	287.0
78.90	2581.0
79.90	564.0
80.90	2471.0
81.90	472.0
85.90	140.0
86.90	2809.0
88.00	2499.0
90.80	307.0
91.90	1829.0
93.00	3075.0
94.00	8605.0
95.00	70128.0
96.00	4924.0
96.90	148.0
103.90	404.0
105.90	334.0
115.90	206.0
117.00	380.0
118.00	286.0
119.00	361.0
127.80	269.0
128.90	120.0
129.80	292.0
130.90	137.0
134.70	116.0
136.80	145.0
140.80	743.0
142.90	794.0
144.90	101.0
146.00	142.0
147.80	233.0
154.70	176.0
156.90	138.0
158.90	140.0
160.70	171.0
171.10	127.0
171.90	344.0
173.10	614.0
174.00	53344.0
174.90	3780.0
176.00	52216.0
177.00	3376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	626.0
37.00	3697.0
38.00	2817.0
39.00	1256.0
39.90	220.0
43.00	127.0
43.90	758.0
45.00	545.0
47.00	873.0
48.00	465.0
49.00	3193.0
50.00	14464.0
51.00	4778.0
52.00	216.0
54.90	155.0
55.90	1240.0
57.00	2114.0
57.90	164.0
59.90	690.0
61.00	3828.0
62.00	3431.0
63.00	3220.0
64.00	441.0
65.00	195.0
66.90	167.0
68.00	7781.0
69.00	8195.0
69.90	638.0
72.00	423.0
73.00	3671.0
74.00	13395.0
75.00	39312.0
76.00	3807.0
77.10	547.0
78.10	295.0
78.90	2789.0
79.90	667.0
80.90	2601.0
81.90	517.0
85.90	122.0
86.90	3236.0
88.00	2809.0
90.90	346.0
92.00	2115.0
93.00	3329.0
94.00	9919.0
95.00	78136.0
96.00	5304.0
96.90	172.0
103.90	443.0
105.90	295.0
114.80	100.0
115.90	283.0
116.90	484.0
118.00	319.0
119.00	379.0
127.80	319.0
128.80	124.0
129.90	301.0
130.80	131.0
134.70	151.0
136.80	155.0
140.80	836.0
142.10	107.0
142.90	946.0
144.90	109.0
146.00	159.0
147.80	266.0
154.70	160.0
157.00	148.0
158.90	133.0
160.70	178.0
171.20	111.0
171.90	407.0
174.00	61232.0
175.00	4324.0
176.00	58808.0
177.00	3819.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	597.0
37.00	3456.0
38.00	2846.0
39.00	1159.0
39.90	227.0
43.00	139.0
43.90	696.0
45.00	483.0
47.00	778.0
48.00	498.0
49.00	3117.0
50.00	14183.0
51.00	4536.0
52.00	175.0
54.90	226.0
55.90	1181.0
57.00	2257.0
58.00	149.0
59.90	746.0
61.00	3680.0
62.00	3406.0
63.00	3145.0
64.00	358.0
65.10	223.0
66.90	186.0
68.00	7441.0
69.00	7869.0
69.90	654.0
72.00	426.0
73.00	3847.0
74.00	13316.0
75.00	39264.0
76.00	3829.0
77.10	598.0
78.10	293.0
78.90	2703.0
79.90	713.0
80.90	2486.0
81.90	583.0
85.90	109.0
86.90	3239.0
87.90	2707.0
90.90	327.0
92.00	2220.0
93.00	3199.0
94.00	9937.0
95.00	77736.0
96.00	5091.0
96.90	162.0
103.90	432.0
105.90	272.0
115.90	357.0
116.80	522.0
118.00	289.0
118.90	317.0
123.70	103.0
127.80	288.0
128.70	122.0
129.90	301.0
130.80	144.0
134.70	154.0
136.80	127.0
140.80	838.0
142.00	115.0
142.90	991.0
144.90	119.0
146.00	121.0
147.80	251.0
149.70	107.0
154.80	165.0
157.10	159.0
158.90	143.0
160.70	124.0
171.90	407.0
174.00	63168.0
175.00	4442.0
176.00	60440.0
177.00	3710.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83