

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033750.D
 Acq On : 19 Jan 2024 13:39
 Operator : SY/MD
 Sample : P1190-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rBV	114399	121505	13.79%	1.772%
2	1.529	145	152	172	rVB	100651	120610	13.69%	1.759%
3	2.059	307	317	350	rVB	209634	312628	35.47%	4.558%
4	2.252	374	377	381	rBV2	553	471	0.05%	0.007%
5	2.294	388	390	394	rVB3	285	185	0.02%	0.003%
6	2.368	411	413	416	rVB	320	118	0.01%	0.002%
7	2.400	420	423	424	rBV2	187	84	0.01%	0.001%
8	2.449	432	438	447	rBV5	1710	2455	0.28%	0.036%
9	2.516	457	459	465	rVB2	159	61	0.01%	0.001%
10	2.574	476	477	478	rVB	117	23	0.00%	0.000%
11	2.587	478	481	484	rBV2	145	106	0.01%	0.002%
12	2.773	536	539	541	rBV	83	54	0.01%	0.001%
13	2.902	576	579	582	rBV	155	100	0.01%	0.001%
14	2.915	582	583	584	rVB	208	40	0.00%	0.001%
15	2.931	584	588	592	rBV2	101	95	0.01%	0.001%
16	3.014	610	614	624	rVB2	174	254	0.03%	0.004%
17	3.056	624	627	628	rBV	60	30	0.00%	0.000%
18	3.166	658	661	666	rBV2	124	135	0.02%	0.002%
19	3.249	683	687	691	rBV2	170	143	0.02%	0.002%
20	3.272	691	694	698	rBV	85	64	0.01%	0.001%
21	3.378	721	727	729	rBV	111	116	0.01%	0.002%
22	3.407	733	736	739	rVB2	84	52	0.01%	0.001%
23	3.487	756	761	767	rBV2	165	251	0.03%	0.004%
24	3.542	775	778	780	rBV	89	57	0.01%	0.001%
25	3.629	802	805	808	rVB	114	68	0.01%	0.001%
26	3.648	808	811	819	rBV	97	76	0.01%	0.001%
27	3.703	826	828	832	rBV2	74	50	0.01%	0.001%
28	3.725	832	835	836	rBV2	163	74	0.01%	0.001%
29	3.786	844	854	897	rBV	58157	161549	18.33%	2.356%
30	4.249	980	998	1030	rBV	133144	343227	38.95%	5.005%
31	4.596	1102	1106	1108	rVB2	301	209	0.02%	0.003%
32	4.612	1108	1111	1112	rBV	199	101	0.01%	0.001%
33	4.632	1116	1117	1118	rBV	116	35	0.00%	0.001%
34	4.641	1118	1120	1122	rBV2	190	65	0.01%	0.001%
35	4.657	1122	1125	1126	rBV	268	91	0.01%	0.001%
36	4.683	1132	1133	1136	rBV	142	64	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033750.D
 Acq On : 19 Jan 2024 13:39
 Operator : SY/MD
 Sample : P1190-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	4.744	1149	1152	1156	rVB2	196	114	0.01%	0.002%
38	4.767	1156	1159	1161	rBV2	145	85	0.01%	0.001%
39	4.850	1183	1185	1189	rBV2	121	77	0.01%	0.001%
40	4.956	1201	1218	1251	rBV2	329968	881264	100.00%	12.850%
41	5.487	1381	1383	1386	rVB2	196	112	0.01%	0.002%
42	5.532	1386	1397	1423	rBV	285656	580850	65.91%	8.469%
43	5.834	1483	1491	1493	rBV5	2256	2978	0.34%	0.043%
44	5.989	1526	1539	1568	rBV	191152	392628	44.55%	5.725%
45	6.281	1628	1630	1636	rVB	298	267	0.03%	0.004%
46	6.310	1636	1639	1641	rBV2	254	178	0.02%	0.003%
47	6.336	1646	1647	1649	rVB	155	59	0.01%	0.001%
48	6.397	1663	1666	1668	rBV	55	28	0.00%	0.000%
49	6.477	1687	1691	1695	rBV2	207	185	0.02%	0.003%
50	6.529	1703	1707	1710	rBV2	164	157	0.02%	0.002%
51	6.593	1724	1727	1730	rBV2	283	226	0.03%	0.003%
52	6.683	1754	1755	1757	rVB	124	41	0.00%	0.001%
53	6.751	1774	1776	1780	rVB2	255	109	0.01%	0.002%
54	6.773	1780	1783	1785	rBV	111	77	0.01%	0.001%
55	6.911	1816	1826	1852	rBV	110370	208285	23.63%	3.037%
56	7.243	1918	1929	1964	rBV	400674	713871	81.01%	10.409%
57	7.522	2013	2016	2017	rBV	425	190	0.02%	0.003%
58	7.554	2017	2026	2044	rBV	76269	134669	15.28%	1.964%
59	7.757	2087	2089	2093	rVB3	224	149	0.02%	0.002%
60	7.776	2093	2095	2096	rBV2	179	91	0.01%	0.001%
61	7.828	2109	2111	2114	rBV	113	59	0.01%	0.001%
62	7.860	2118	2121	2124	rBV2	144	93	0.01%	0.001%
63	7.876	2124	2126	2127	rBV2	241	78	0.01%	0.001%
64	7.905	2133	2135	2137	rVB	144	39	0.00%	0.001%
65	8.024	2163	2172	2213	rBV	206058	408130	46.31%	5.951%
66	8.516	2322	2325	2329	rBV	190	146	0.02%	0.002%
67	8.587	2344	2347	2350	rBV2	111	74	0.01%	0.001%
68	8.648	2363	2366	2371	rVB	167	129	0.01%	0.002%
69	8.673	2371	2374	2380	rBV2	101	105	0.01%	0.002%
70	8.783	2397	2408	2445	rBV	430826	710150	80.58%	10.355%
71	9.021	2476	2482	2483	rBV2	173	202	0.02%	0.003%
72	9.040	2487	2488	2490	rVB2	162	40	0.00%	0.001%
73	9.091	2500	2504	2505	rBV2	220	172	0.02%	0.003%
74	9.468	2618	2621	2624	rBV	99	87	0.01%	0.001%
75	9.493	2624	2629	2633	rVB2	281	280	0.03%	0.004%
76	9.529	2636	2640	2641	rBV2	173	117	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033750.D
 Acq On : 19 Jan 2024 13:39
 Operator : SY/MD
 Sample : P1190-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	9.538	2641	2643	2645	rBV2	186	74	0.01%	0.001%
78	9.683	2682	2688	2690	rBV	134	143	0.02%	0.002%
79	9.763	2711	2713	2718	rBV2	136	145	0.02%	0.002%
80	9.943	2764	2769	2771	rBV2	159	140	0.02%	0.002%
81	10.024	2791	2794	2796	rBV	96	53	0.01%	0.001%
82	10.152	2822	2834	2858	rBV	245664	387033	43.92%	5.643%
83	10.313	2882	2884	2885	rBV	120	35	0.00%	0.001%
84	10.760	3021	3023	3026	rVB	136	71	0.01%	0.001%
85	11.127	3135	3137	3144	rVB3	371	320	0.04%	0.005%
86	11.185	3144	3155	3186	rBV	442936	703754	79.86%	10.262%
87	11.368	3210	3212	3214	rBV2	297	134	0.02%	0.002%
88	11.397	3219	3221	3222	rBV2	137	59	0.01%	0.001%
89	11.561	3260	3272	3298	rBV	418268	647952	73.53%	9.448%
90	11.776	3337	3339	3342	rVB2	184	62	0.01%	0.001%
91	12.432	3541	3543	3544	rBV	219	86	0.01%	0.001%
92	13.014	3721	3724	3726	rBV2	164	112	0.01%	0.002%
93	13.207	3781	3784	3793	rVB2	773	790	0.09%	0.012%
94	13.448	3850	3859	3876	rBV2	9164	15286	1.73%	0.223%
95	13.757	3952	3955	3956	rBV2	175	89	0.01%	0.001%




Sum of corrected areas: 6858175

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033750.D
Acq On : 19 Jan 2024 13:39
Operator : SY/MD
Sample : P1190-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

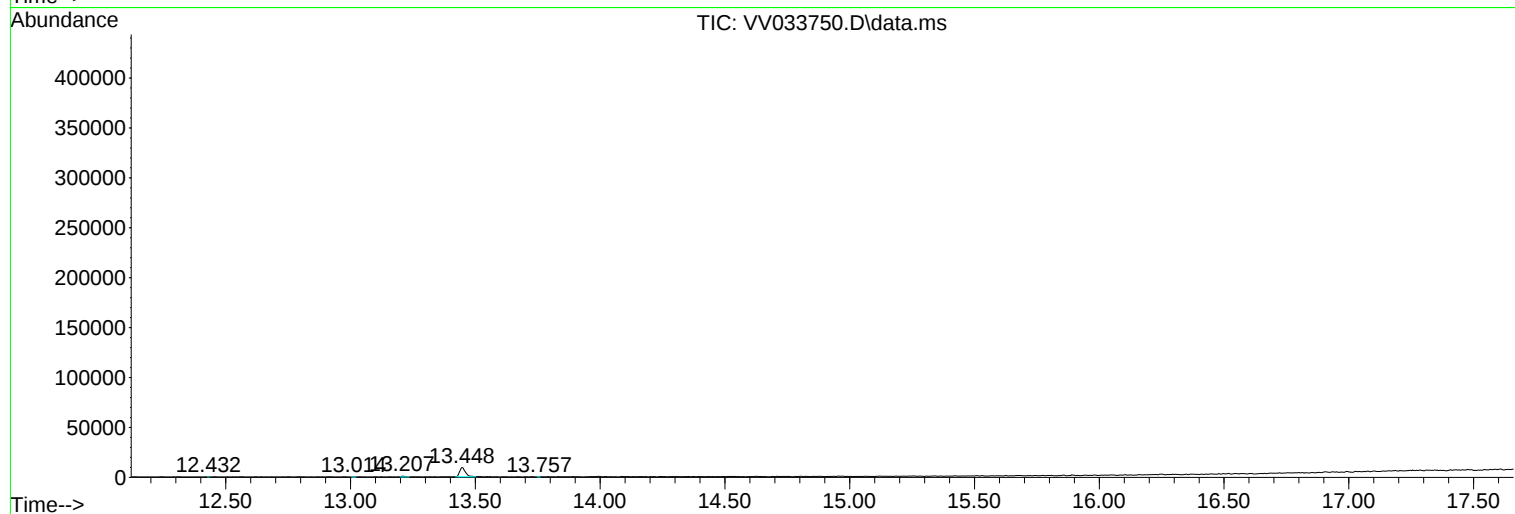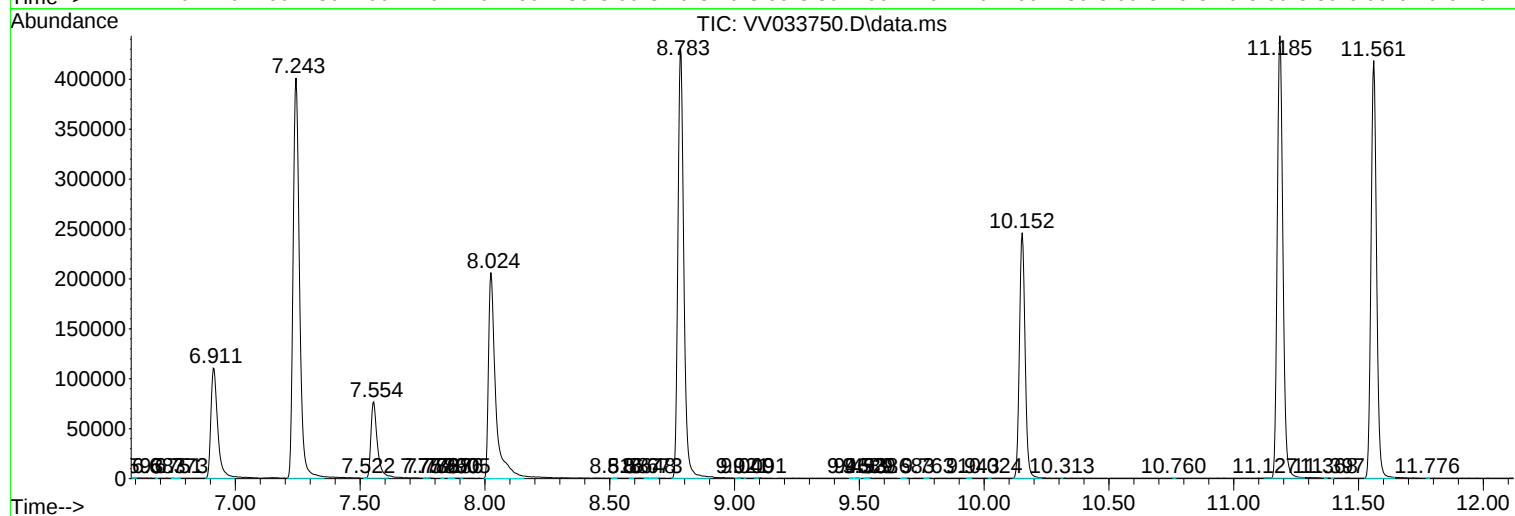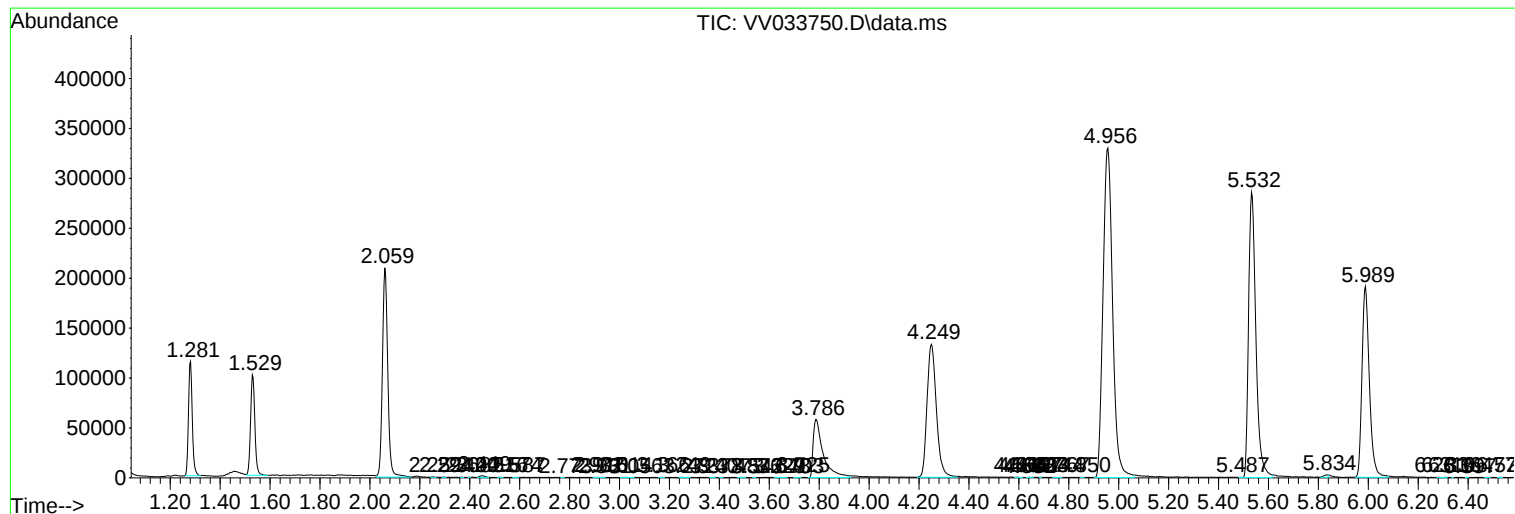

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033750.D
Acq On : 19 Jan 2024 13:39
Operator : SY/MD
Sample : P1190-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033750.D
Acq On : 19 Jan 2024 13:39
Operator : SY/MD
Sample : P1190-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc