

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033752.D
 Acq On : 19 Jan 2024 14:26
 Operator : SY/MD
 Sample : P1190-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	12793	15646	1.83%	0.233%
2	1.281	68	75	90	rBV	116092	118469	13.83%	1.762%
3	1.532	145	153	165	rBV	95097	114472	13.36%	1.702%
4	2.059	308	317	332	rBV	194417	284892	33.25%	4.237%
5	2.359	406	410	416	rBV2	435	258	0.03%	0.004%
6	2.564	463	474	480	rBV2	1245	2639	0.31%	0.039%
7	2.641	497	498	500	rVB2	107	21	0.00%	0.000%
8	2.722	520	523	526	rBV2	94	67	0.01%	0.001%
9	2.751	529	532	533	rBV2	77	50	0.01%	0.001%
10	2.780	539	541	546	rBV	128	83	0.01%	0.001%
11	2.838	557	559	561	rBV	42	25	0.00%	0.000%
12	2.867	566	568	572	rVB2	256	94	0.01%	0.001%
13	2.892	572	576	579	rBV	151	100	0.01%	0.001%
14	2.953	592	595	600	rVB2	201	160	0.02%	0.002%
15	3.027	616	618	619	rBV2	112	47	0.01%	0.001%
16	3.104	637	642	647	rVB2	279	279	0.03%	0.004%
17	3.130	647	650	651	rBV	96	55	0.01%	0.001%
18	3.169	657	662	664	rBV	168	133	0.02%	0.002%
19	3.304	701	704	706	rBV	98	71	0.01%	0.001%
20	3.349	713	718	721	rBV2	144	155	0.02%	0.002%
21	3.407	733	736	738	rBV	131	71	0.01%	0.001%
22	3.477	756	758	761	rVB	121	39	0.00%	0.001%
23	3.516	767	770	774	rVB2	94	55	0.01%	0.001%
24	3.564	782	785	789	rBV2	76	52	0.01%	0.001%
25	3.587	789	792	795	rVB	180	113	0.01%	0.002%
26	3.603	795	797	800	rBV	119	75	0.01%	0.001%
27	3.674	816	819	822	rBV2	77	46	0.01%	0.001%
28	3.715	828	832	835	rVB	108	79	0.01%	0.001%
29	3.738	835	839	841	rBV	128	99	0.01%	0.001%
30	3.783	845	853	884	rBV	54530	145110	16.94%	2.158%
31	4.249	982	998	1031	rBV	129499	335363	39.14%	4.988%
32	4.526	1083	1084	1085	rBV	122	46	0.01%	0.001%
33	4.600	1105	1107	1111	rBV2	190	158	0.02%	0.002%
34	4.619	1111	1113	1116	rBV3	131	83	0.01%	0.001%
35	4.664	1124	1127	1128	rBV	86	44	0.01%	0.001%
36	4.757	1152	1156	1159	rVB	248	153	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033752.D
 Acq On : 19 Jan 2024 14:26
 Operator : SY/MD
 Sample : P1190-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	4.776	1159	1162	1165	rBV2	147	143	0.02%	0.002%
38	4.847	1181	1184	1185	rBV	134	60	0.01%	0.001%
39	4.956	1202	1218	1255	rBV2	320405	856855	100.00%	12.744%
40	5.532	1386	1397	1426	rBV	290762	592479	69.15%	8.812%
41	5.834	1484	1491	1505	rVB3	2112	3760	0.44%	0.056%
42	5.989	1526	1539	1569	rBV	187081	388515	45.34%	5.778%
43	6.281	1625	1630	1632	rBV3	277	169	0.02%	0.003%
44	6.323	1640	1643	1644	rBV	214	97	0.01%	0.001%
45	6.342	1648	1649	1651	rVV	138	34	0.00%	0.001%
46	6.355	1651	1653	1657	rVB	102	62	0.01%	0.001%
47	6.390	1661	1664	1668	rBV2	132	92	0.01%	0.001%
48	6.529	1699	1707	1711	rBV2	152	193	0.02%	0.003%
49	6.593	1724	1727	1730	rBV2	330	217	0.03%	0.003%
50	6.645	1741	1743	1745	rBV2	167	115	0.01%	0.002%
51	6.706	1760	1762	1764	rBV2	79	40	0.00%	0.001%
52	6.735	1769	1771	1774	rVB	157	52	0.01%	0.001%
53	6.911	1816	1826	1857	rBV	108052	205488	23.98%	3.056%
54	7.243	1915	1929	1961	rBV	391688	691708	80.73%	10.287%
55	7.554	2016	2026	2055	rBV	73382	135113	15.77%	2.009%
56	7.799	2099	2102	2110	rBV2	146	123	0.01%	0.002%
57	7.882	2120	2128	2138	rVB3	488	968	0.11%	0.014%
58	7.931	2139	2143	2146	rBV2	113	113	0.01%	0.002%
59	8.024	2163	2172	2217	rBV	185929	375902	43.87%	5.591%
60	8.374	2280	2281	2282	rBV	91	33	0.00%	0.000%
61	8.400	2285	2289	2291	rBV2	171	168	0.02%	0.002%
62	8.516	2323	2325	2329	rVB	261	127	0.01%	0.002%
63	8.532	2329	2330	2335	rBV	122	44	0.01%	0.001%
64	8.564	2337	2340	2341	rBV	167	74	0.01%	0.001%
65	8.625	2352	2359	2362	rBV2	116	144	0.02%	0.002%
66	8.654	2367	2368	2369	rBV	157	33	0.00%	0.000%
67	8.702	2381	2383	2386	rVB2	80	42	0.00%	0.001%
68	8.725	2388	2390	2393	rBV2	170	55	0.01%	0.001%
69	8.783	2397	2408	2441	rBV	439697	728229	84.99%	10.831%
70	9.005	2472	2477	2479	rBV2	334	282	0.03%	0.004%
71	9.056	2490	2493	2496	rBV3	193	144	0.02%	0.002%
72	9.088	2499	2503	2505	rBV3	210	191	0.02%	0.003%
73	9.439	2609	2612	2617	rVB2	209	131	0.02%	0.002%
74	9.464	2617	2620	2622	rBV	74	50	0.01%	0.001%
75	9.490	2622	2628	2633	rVV3	229	305	0.04%	0.005%
76	9.615	2663	2667	2672	rBV	126	114	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033752.D
 Acq On : 19 Jan 2024 14:26
 Operator : SY/MD
 Sample : P1190-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	9.644	2672	2676	2678	rBV	157	119	0.01%	0.002%
78	9.831	2731	2734	2736	rBV	129	81	0.01%	0.001%
79	9.969	2775	2777	2780	rBV	110	65	0.01%	0.001%
80	10.152	2822	2834	2857	rBV	240188	376235	43.91%	5.596%
81	10.268	2866	2870	2872	rBV	151	111	0.01%	0.002%
82	10.416	2913	2916	2918	rBV	88	59	0.01%	0.001%
83	10.712	3005	3008	3011	rBV2	187	140	0.02%	0.002%
84	11.130	3135	3138	3144	rVB2	610	473	0.06%	0.007%
85	11.185	3144	3155	3181	rBV	456574	713310	83.25%	10.609%
86	11.493	3250	3251	3252	rBV	192	45	0.01%	0.001%
87	11.561	3261	3272	3296	rBV	396088	625655	73.02%	9.305%
88	11.757	3331	3333	3337	rVB2	235	123	0.01%	0.002%
89	11.821	3351	3353	3359	rVB2	142	85	0.01%	0.001%
90	11.853	3359	3363	3368	rBV2	156	189	0.02%	0.003%
91	11.914	3379	3382	3386	rBV2	139	145	0.02%	0.002%
92	12.156	3455	3457	3460	rVB	180	56	0.01%	0.001%
93	12.641	3605	3608	3614	rBV2	165	208	0.02%	0.003%
94	13.178	3774	3775	3776	rBV	211	46	0.01%	0.001%
95	13.213	3781	3786	3790	rVV3	471	591	0.07%	0.009%
96	13.377	3834	3837	3839	rBV2	194	126	0.01%	0.002%
97	13.451	3855	3860	3872	rVB3	3047	3982	0.46%	0.059%
98	13.647	3919	3921	3924	rBV2	202	79	0.01%	0.001%
99	13.770	3956	3959	3964	rBV2	197	154	0.02%	0.002%




Sum of corrected areas: 6723843

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033752.D
Acq On : 19 Jan 2024 14:26
Operator : SY/MD
Sample : P1190-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

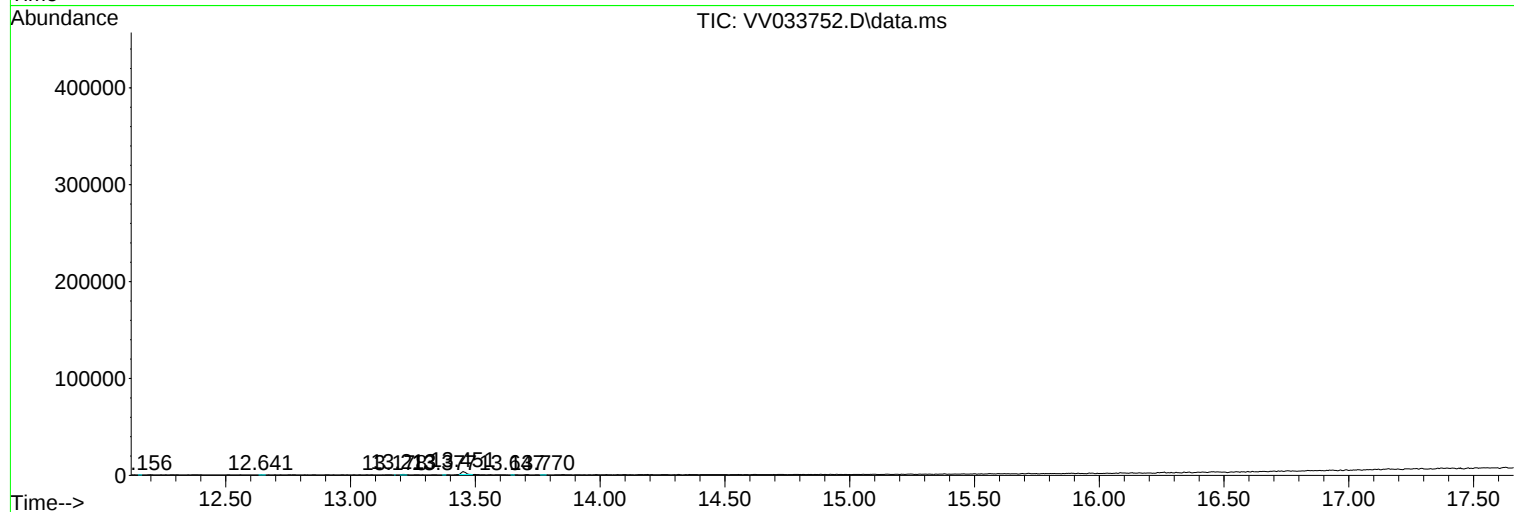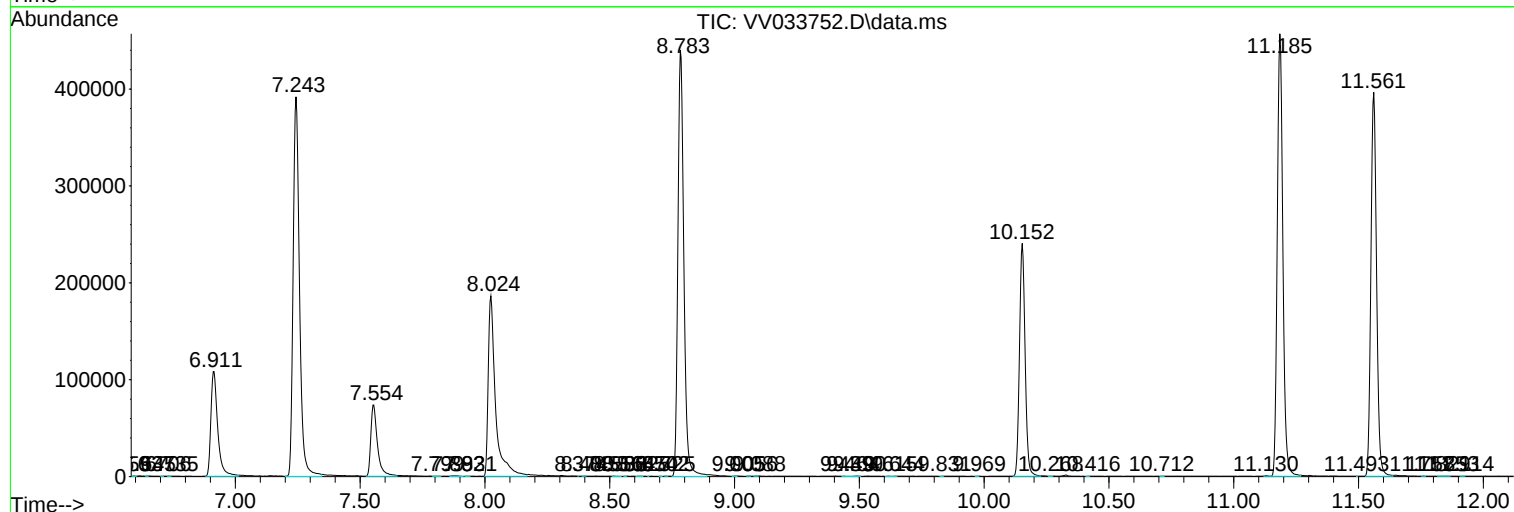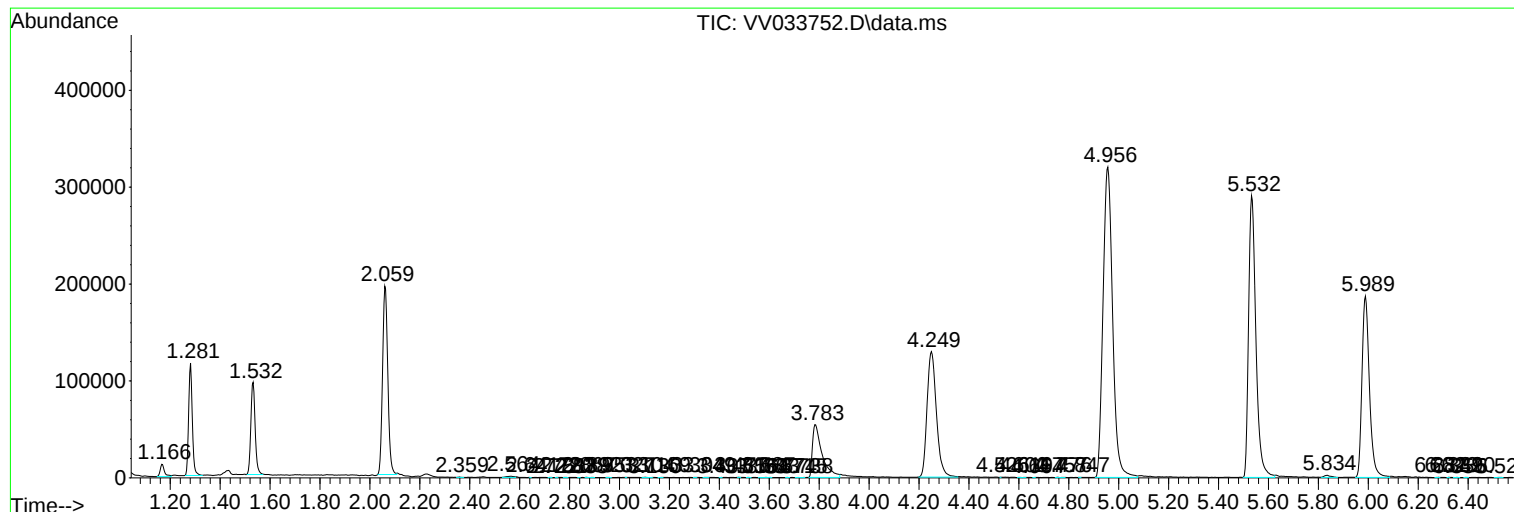

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033752.D
Acq On : 19 Jan 2024 14:26
Operator : SY/MD
Sample : P1190-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033752.D
Acq On : 19 Jan 2024 14:26
Operator : SY/MD
Sample : P1190-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
