

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033753.D
 Acq On : 19 Jan 2024 14:50
 Operator : SY/MD
 Sample : P1190-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	51	rBV	15412	18331	2.14%	0.271%
2	1.282	68	75	90	rBV	112902	119518	13.93%	1.765%
3	1.532	146	153	169	rVB	97503	116961	13.63%	1.727%
4	2.060	308	317	331	rBV	198215	286216	33.36%	4.227%
5	2.410	423	426	428	rBV	336	194	0.02%	0.003%
6	2.423	428	430	433	rVB2	393	208	0.02%	0.003%
7	2.526	460	462	466	rBV	154	102	0.01%	0.002%
8	2.555	466	471	473	rBV2	391	458	0.05%	0.007%
9	2.809	549	550	552	rBB	170	34	0.00%	0.001%
10	3.137	649	652	656	rVB	279	188	0.02%	0.003%
11	3.163	656	660	665	rBV	209	204	0.02%	0.003%
12	3.462	750	753	755	rBV	111	65	0.01%	0.001%
13	3.471	755	756	760	rVB2	207	82	0.01%	0.001%
14	3.503	760	766	769	rBV	144	130	0.02%	0.002%
15	3.564	782	785	787	rBV	106	48	0.01%	0.001%
16	3.603	792	797	799	rBV	122	123	0.01%	0.002%
17	3.751	839	843	845	rBV	187	132	0.02%	0.002%
18	3.783	845	853	885	rBV	55809	148142	17.27%	2.188%
19	4.249	982	998	1029	rBV	132171	338842	39.50%	5.004%
20	4.568	1095	1097	1099	rBV2	202	134	0.02%	0.002%
21	4.603	1107	1108	1109	rBV	282	79	0.01%	0.001%
22	4.658	1122	1125	1126	rBV	243	105	0.01%	0.002%
23	4.683	1132	1133	1136	rVB2	204	68	0.01%	0.001%
24	4.854	1185	1186	1187	rVB2	102	20	0.00%	0.000%
25	4.873	1187	1192	1194	rVB2	178	101	0.01%	0.001%
26	4.902	1195	1201	1202	rBV2	135	112	0.01%	0.002%
27	4.957	1202	1218	1254	rBV2	324042	857900	100.00%	12.670%
28	5.394	1351	1354	1357	rBV3	297	225	0.03%	0.003%
29	5.494	1382	1385	1386	rBV2	213	140	0.02%	0.002%
30	5.532	1386	1397	1436	rVV	291852	602541	70.23%	8.899%
31	5.838	1482	1492	1508	rVB6	2193	4822	0.56%	0.071%
32	5.896	1508	1510	1513	rBV3	246	204	0.02%	0.003%
33	5.989	1526	1539	1573	rBV	186667	390512	45.52%	5.768%
34	6.246	1617	1619	1622	rVB2	173	80	0.01%	0.001%
35	6.269	1623	1626	1628	rBV	224	113	0.01%	0.002%
36	6.307	1636	1638	1644	rVB3	252	198	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033753.D
 Acq On : 19 Jan 2024 14:50
 Operator : SY/MD
 Sample : P1190-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.336	1644	1647	1650	rBV2	188	128	0.01%	0.002%
38	6.349	1650	1651	1652	rVB	178	34	0.00%	0.001%
39	6.365	1652	1656	1658	rBV2	144	119	0.01%	0.002%
40	6.449	1679	1682	1685	rBV	147	105	0.01%	0.002%
41	6.487	1691	1694	1697	rBV	172	104	0.01%	0.002%
42	6.590	1725	1726	1727	rBV	222	68	0.01%	0.001%
43	6.654	1743	1746	1751	rVB	257	227	0.03%	0.003%
44	6.680	1752	1754	1757	rVV2	125	62	0.01%	0.001%
45	6.741	1771	1773	1778	rVB2	145	99	0.01%	0.001%
46	6.912	1816	1826	1850	rBV	109083	204828	23.88%	3.025%
47	7.243	1917	1929	1961	rBV	394493	692255	80.69%	10.224%
48	7.551	2016	2025	2047	rBV	74708	133665	15.58%	1.974%
49	7.780	2094	2096	2098	rBV	121	63	0.01%	0.001%
50	7.873	2121	2125	2138	rVB3	1073	1722	0.20%	0.025%
51	8.024	2163	2172	2223	rBV	193749	386871	45.10%	5.714%
52	8.333	2266	2268	2269	rBV	359	85	0.01%	0.001%
53	8.432	2297	2299	2301	rBV	203	105	0.01%	0.002%
54	8.465	2306	2309	2311	rBV	174	80	0.01%	0.001%
55	8.503	2320	2321	2322	rVB	138	27	0.00%	0.000%
56	8.519	2323	2326	2330	rBV2	226	212	0.02%	0.003%
57	8.670	2368	2373	2376	rBV2	151	148	0.02%	0.002%
58	8.783	2397	2408	2437	rBV	436468	730309	85.13%	10.786%
59	8.998	2472	2475	2476	rBV	326	183	0.02%	0.003%
60	9.024	2481	2483	2484	rBV	149	63	0.01%	0.001%
61	9.034	2484	2486	2487	rBV	109	28	0.00%	0.000%
62	9.175	2527	2530	2536	rBV2	157	171	0.02%	0.003%
63	9.239	2547	2550	2552	rBV	144	90	0.01%	0.001%
64	9.330	2572	2578	2581	rBV2	141	161	0.02%	0.002%
65	9.683	2685	2688	2691	rBV	83	80	0.01%	0.001%
66	10.153	2822	2834	2865	rBV	241725	380801	44.39%	5.624%
67	10.288	2873	2876	2879	rBV	119	91	0.01%	0.001%
68	10.326	2879	2888	2900	rVV4	1680	2622	0.31%	0.039%
69	10.368	2900	2901	2903	rVB	157	58	0.01%	0.001%
70	10.802	3031	3036	3039	rBV2	184	171	0.02%	0.003%
71	10.821	3039	3042	3044	rBV2	132	93	0.01%	0.001%
72	10.966	3084	3087	3090	rBV2	115	83	0.01%	0.001%
73	11.185	3144	3155	3176	rBV	456536	715098	83.35%	10.561%
74	11.397	3218	3221	3223	rBV2	176	106	0.01%	0.002%
75	11.461	3239	3241	3243	rBV	188	60	0.01%	0.001%
76	11.561	3260	3272	3296	rBV	398843	629119	73.33%	9.292%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033753.D
Acq On : 19 Jan 2024 14:50
Operator : SY/MD
Sample : P1190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

77	12.278	3492	3495	3496	rBV	207	127	0.01%	0.002%
78	12.882	3679	3683	3686	rBV2	152	128	0.01%	0.002%
79	13.175	3771	3774	3778	rBV	301	252	0.03%	0.004%
80	13.452	3856	3860	3872	rVB6	1792	2501	0.29%	0.037%
81	13.606	3907	3908	3909	rBV	225	52	0.01%	0.001%
82	14.062	4047	4050	4052	rBV3	190	111	0.01%	0.002%




Sum of corrected areas: 6770897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033753.D
Acq On : 19 Jan 2024 14:50
Operator : SY/MD
Sample : P1190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

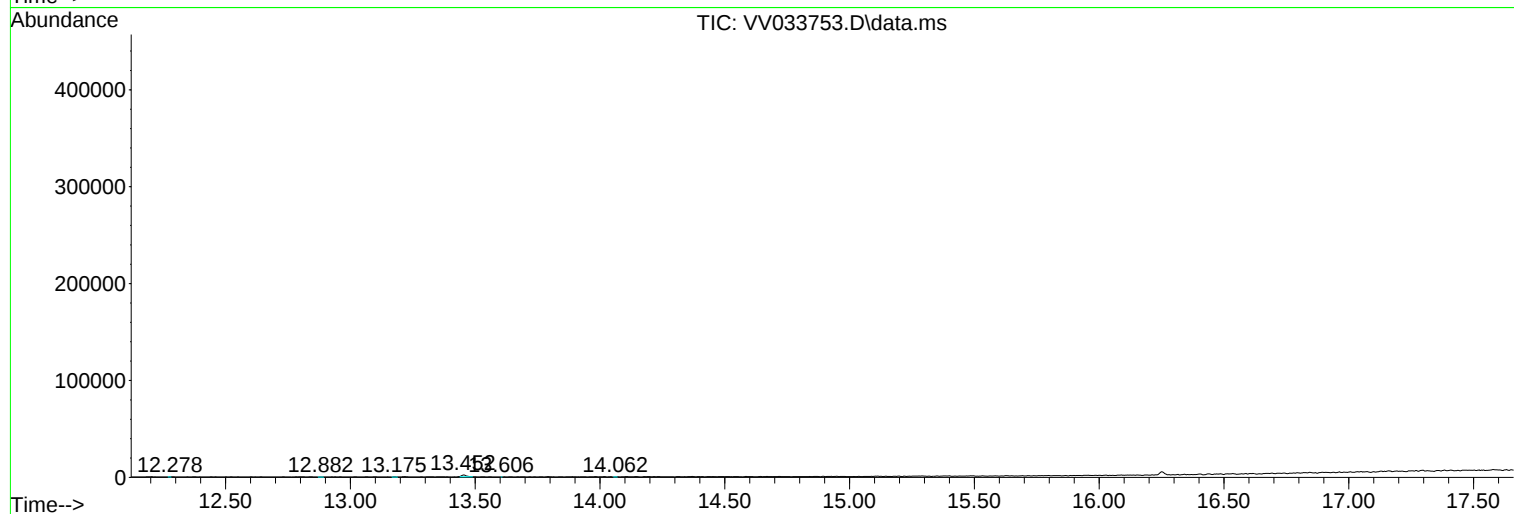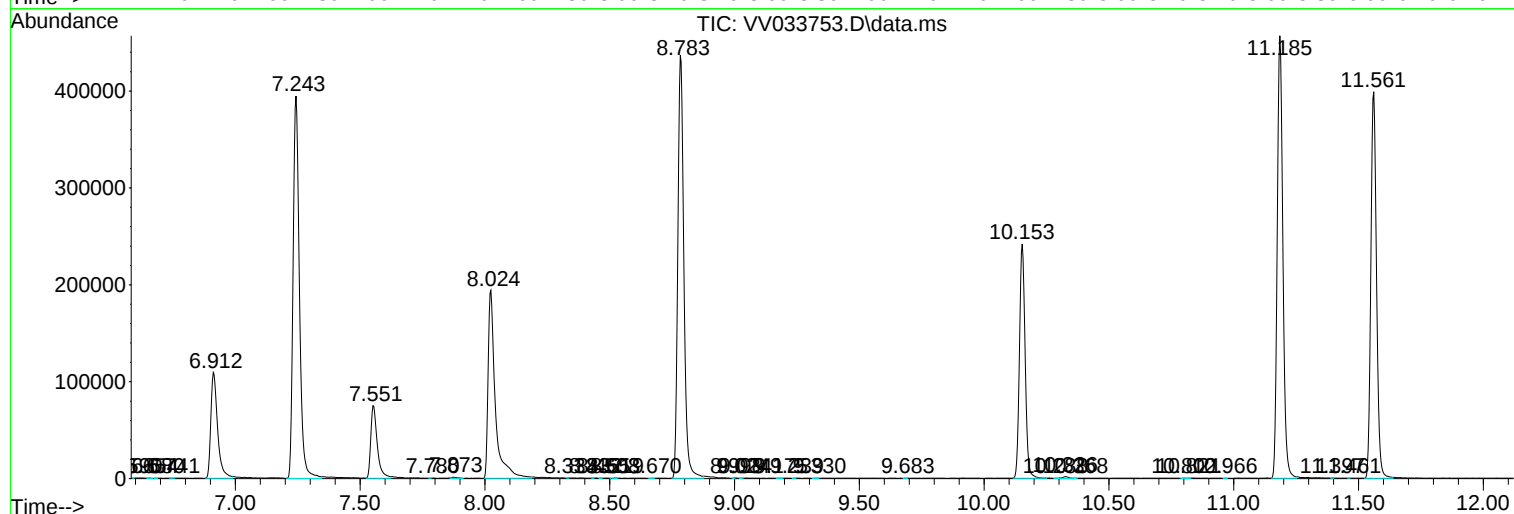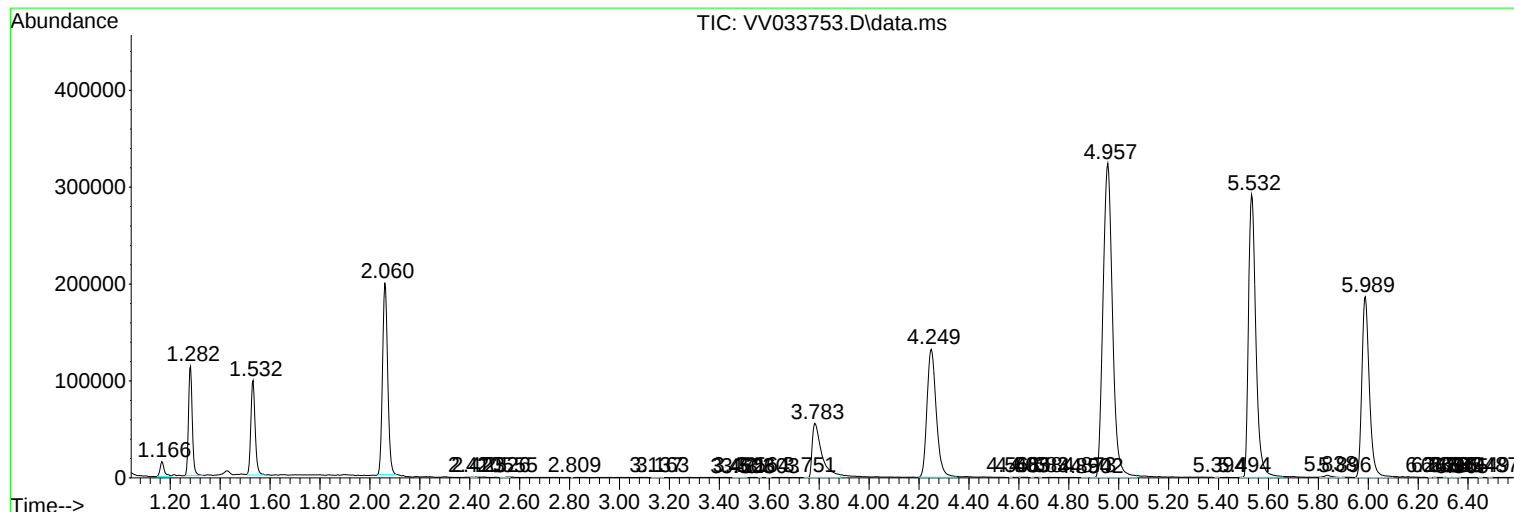

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033753.D
Acq On : 19 Jan 2024 14:50
Operator : SY/MD
Sample : P1190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033753.D
Acq On : 19 Jan 2024 14:50
Operator : SY/MD
Sample : P1190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc