

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033774.D
 Acq On : 19 Jan 2024 23:58
 Operator : SY/MD
 Sample : P1189-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	31	39	62	rBV	153538	185528	24.38%	2.824%
2	1.278	65	74	106	rBV2	181867	326933	42.97%	4.976%
3	1.532	147	153	171	rVB	88879	111762	14.69%	1.701%
4	2.059	308	317	351	rVB	180838	284527	37.39%	4.331%
5	2.178	352	354	356	rBV2	423	192	0.03%	0.003%
6	2.564	471	474	479	rVB2	323	307	0.04%	0.005%
7	2.677	504	509	511	rBV	272	241	0.03%	0.004%
8	2.703	515	517	522	rVB3	237	173	0.02%	0.003%
9	2.760	531	535	539	rBV2	209	242	0.03%	0.004%
10	2.873	565	570	572	rBV	282	170	0.02%	0.003%
11	2.944	589	592	595	rBV	182	141	0.02%	0.002%
12	3.323	704	710	714	rVV2	159	188	0.02%	0.003%
13	3.375	722	726	730	rVB2	147	133	0.02%	0.002%
14	3.397	730	733	740	rBV2	126	163	0.02%	0.002%
15	3.564	781	785	789	rBV2	125	112	0.01%	0.002%
16	3.783	845	853	898	rBV	46675	135268	17.78%	2.059%
17	4.175	973	975	979	rVB	318	138	0.02%	0.002%
18	4.249	982	998	1030	rVV	118959	303117	39.84%	4.614%
19	4.522	1080	1083	1086	rVB3	190	126	0.02%	0.002%
20	4.571	1095	1098	1100	rBV	294	171	0.02%	0.003%
21	4.770	1157	1160	1164	rBV2	120	109	0.01%	0.002%
22	4.956	1201	1218	1246	rBV2	286566	760912	100.00%	11.581%
23	5.133	1270	1273	1280	rVB2	397	283	0.04%	0.004%
24	5.374	1347	1348	1352	rVB2	256	152	0.02%	0.002%
25	5.407	1352	1358	1360	rBV	379	290	0.04%	0.004%
26	5.445	1368	1370	1373	rVB2	182	105	0.01%	0.002%
27	5.532	1386	1397	1424	rBV	275185	564326	74.16%	8.589%
28	5.751	1463	1465	1468	rBV2	184	126	0.02%	0.002%
29	5.844	1485	1494	1505	rVB7	1484	2824	0.37%	0.043%
30	5.989	1526	1539	1571	rBV	169104	348908	45.85%	5.310%
31	6.133	1583	1584	1586	rBV2	271	125	0.02%	0.002%
32	6.217	1609	1610	1613	rVB2	276	119	0.02%	0.002%
33	6.310	1636	1639	1643	rBV2	219	141	0.02%	0.002%
34	6.358	1647	1654	1658	rBV	252	377	0.05%	0.006%
35	6.535	1704	1709	1712	rBV2	213	214	0.03%	0.003%
36	6.580	1718	1723	1724	rBV2	126	106	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033774.D
 Acq On : 19 Jan 2024 23:58
 Operator : SY/MD
 Sample : P1189-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.590	1724	1726	1729	rVV	160	116	0.02%	0.002%
38	6.606	1729	1731	1734	rVB2	197	112	0.01%	0.002%
39	6.628	1734	1738	1739	rBV	172	118	0.02%	0.002%
40	6.677	1748	1753	1755	rBV2	201	179	0.02%	0.003%
41	6.760	1776	1779	1782	rBV	135	105	0.01%	0.002%
42	6.915	1814	1827	1856	rBV	90071	168291	22.12%	2.561%
43	7.127	1890	1893	1895	rBV	156	121	0.02%	0.002%
44	7.149	1898	1900	1902	rBV2	316	159	0.02%	0.002%
45	7.162	1902	1904	1907	rVB3	385	207	0.03%	0.003%
46	7.181	1907	1910	1918	rVB2	547	546	0.07%	0.008%
47	7.243	1918	1929	1959	rBV	350248	617924	81.21%	9.405%
48	7.519	2012	2015	2017	rBV2	330	224	0.03%	0.003%
49	7.554	2017	2026	2051	rVV	60130	107792	14.17%	1.641%
50	7.760	2087	2090	2092	rBV	161	117	0.02%	0.002%
51	7.805	2098	2104	2106	rBV2	115	106	0.01%	0.002%
52	7.866	2120	2123	2124	rBV2	226	152	0.02%	0.002%
53	7.911	2130	2137	2147	rVB2	2254	3338	0.44%	0.051%
54	8.024	2163	2172	2217	rBV	176818	338938	44.54%	5.159%
55	8.374	2277	2281	2283	rBV2	169	143	0.02%	0.002%
56	8.783	2397	2408	2441	rBV	418333	687284	90.32%	10.461%
57	9.066	2491	2496	2498	rVB2	211	200	0.03%	0.003%
58	9.271	2557	2560	2564	rVB	142	105	0.01%	0.002%
59	9.374	2589	2592	2598	rVB2	147	107	0.01%	0.002%
60	9.763	2707	2713	2714	rBV	99	115	0.02%	0.002%
61	10.152	2823	2834	2863	rVV	220041	345307	45.38%	5.256%
62	10.394	2906	2909	2915	rVB2	104	129	0.02%	0.002%
63	10.654	2985	2990	2993	rBV2	231	306	0.04%	0.005%
64	10.934	3074	3077	3082	rVB2	138	131	0.02%	0.002%
65	10.963	3082	3086	3091	rBV2	162	224	0.03%	0.003%
66	11.033	3104	3108	3111	rBV	156	131	0.02%	0.002%
67	11.185	3144	3155	3176	rBV	436345	677846	89.08%	10.317%
68	11.445	3230	3236	3239	rBV	193	206	0.03%	0.003%
69	11.561	3260	3272	3294	rVV	360015	574366	75.48%	8.742%
70	11.766	3334	3336	3339	rBV	141	99	0.01%	0.002%
71	12.027	3414	3417	3420	rBV2	131	100	0.01%	0.002%
72	12.191	3465	3468	3471	rBV2	190	163	0.02%	0.002%
73	12.210	3471	3474	3480	rVB	161	136	0.02%	0.002%
74	12.326	3507	3510	3513	rVB	223	143	0.02%	0.002%
75	12.557	3578	3582	3587	rVB	154	128	0.02%	0.002%
76	12.586	3588	3591	3595	rBV	155	124	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
 Data File : VV033774.D
 Acq On : 19 Jan 2024 23:58
 Operator : SY/MD
 Sample : P1189-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.963	3705	3708	3712	rVB2	159	100	0.01%	0.002%
78	12.985	3712	3715	3717	rBV	129	98	0.01%	0.001%
79	13.098	3748	3750	3752	rBV	354	203	0.03%	0.003%
80	13.120	3755	3757	3759	rVB	478	181	0.02%	0.003%
81	13.345	3825	3827	3829	rVB	212	110	0.01%	0.002%
82	13.377	3835	3837	3838	rBV	292	141	0.02%	0.002%
83	13.406	3844	3846	3848	rVB	254	99	0.01%	0.002%
84	13.869	3985	3990	3995	rBV3	208	208	0.03%	0.003%
85	13.988	4024	4027	4032	rBV2	336	338	0.04%	0.005%
86	14.014	4032	4035	4038	rBV2	170	135	0.02%	0.002%
87	14.082	4047	4056	4069	rBV7	4157	10621	1.40%	0.162%
88	14.242	4104	4106	4108	rVB2	336	109	0.01%	0.002%
89	14.297	4119	4123	4127	rBV5	516	538	0.07%	0.008%
90	14.329	4131	4133	4135	rBV2	149	101	0.01%	0.002%
91	14.435	4163	4166	4169	rVB2	413	226	0.03%	0.003%
92	14.464	4171	4175	4178	rBV2	251	252	0.03%	0.004%
93	14.516	4185	4191	4194	rBV2	423	460	0.06%	0.007%
94	14.651	4231	4233	4235	rBV2	188	114	0.01%	0.002%
95	14.667	4235	4238	4241	rVB3	257	170	0.02%	0.003%
96	14.815	4282	4284	4288	rVB2	294	152	0.02%	0.002%
97	14.985	4334	4337	4342	rBV2	266	248	0.03%	0.004%
98	15.178	4395	4397	4398	rBV	289	102	0.01%	0.002%
99	15.323	4439	4442	4447	rBV4	547	493	0.06%	0.008%
100	15.371	4455	4457	4460	rBV3	314	210	0.03%	0.003%




Sum of corrected areas: 6570196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033774.D
Acq On : 19 Jan 2024 23:58
Operator : SY/MD
Sample : P1189-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

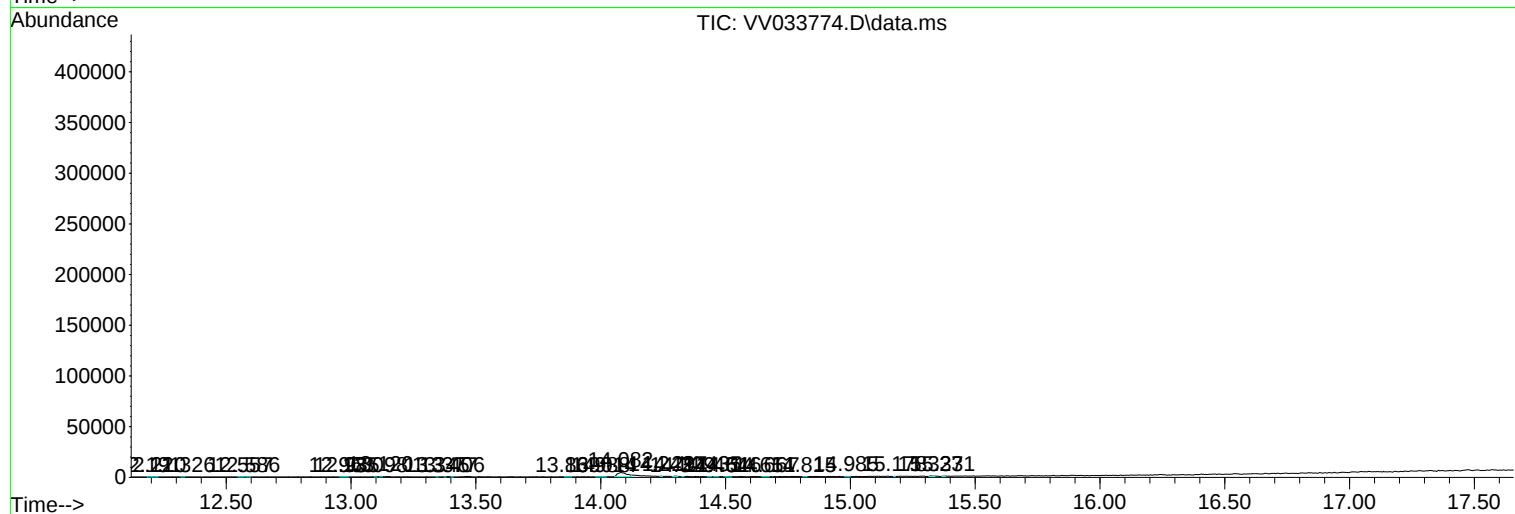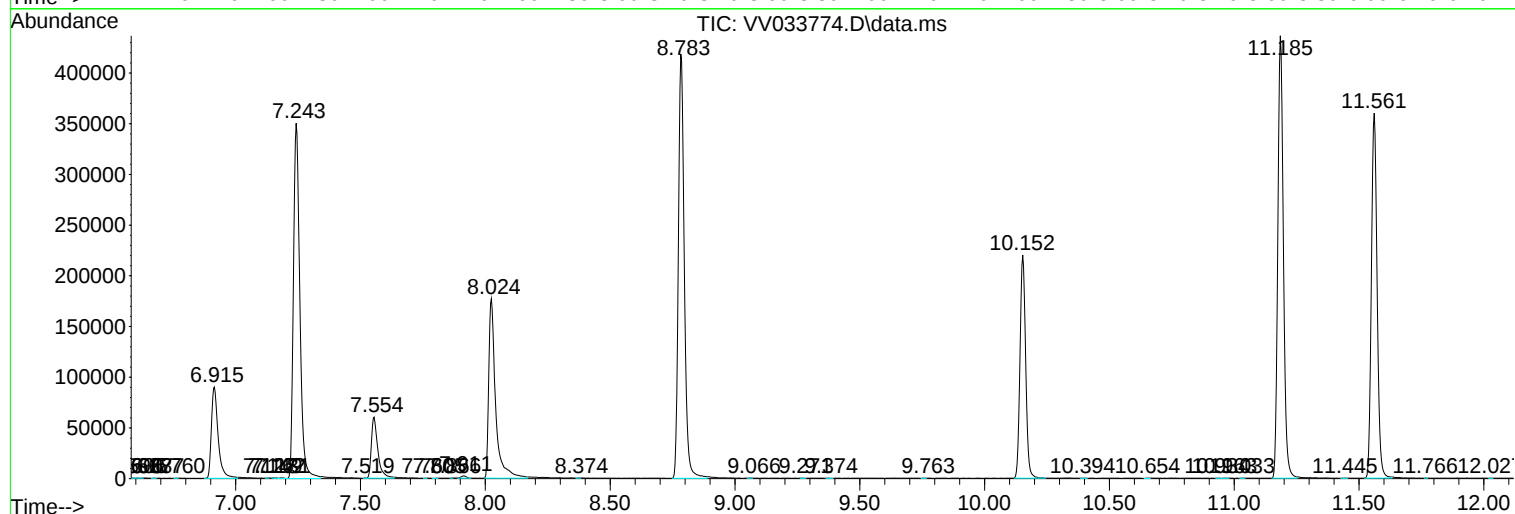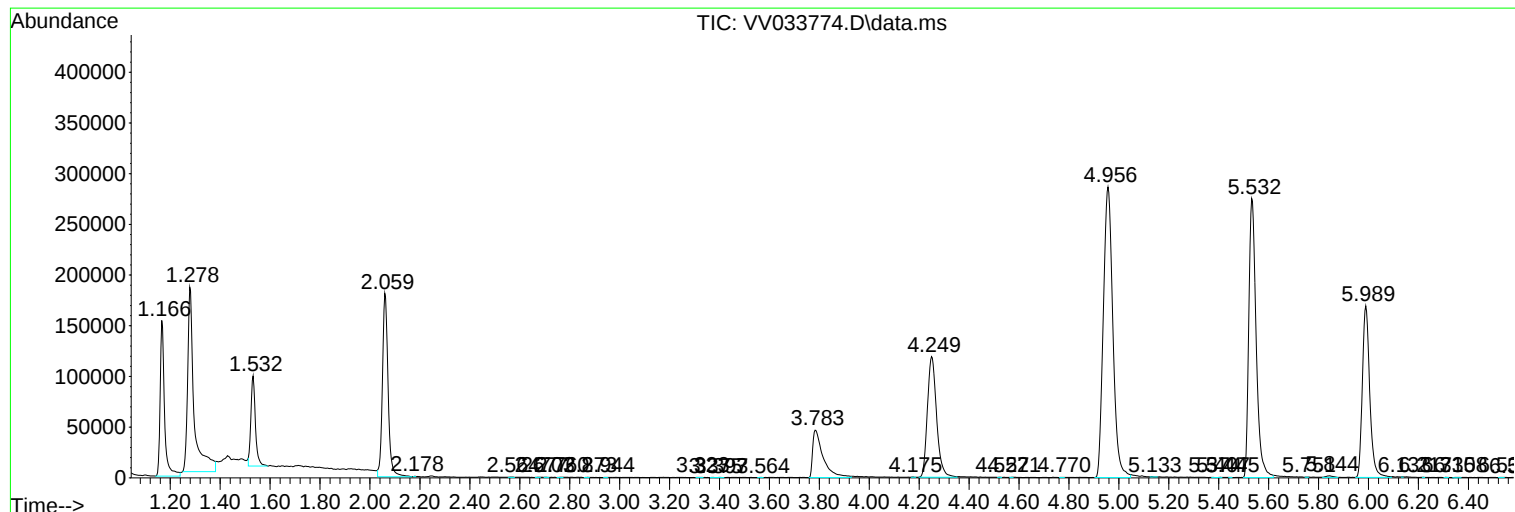

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033774.D
Acq On : 19 Jan 2024 23:58
Operator : SY/MD
Sample : P1189-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033774.D
Acq On : 19 Jan 2024 23:58
Operator : SY/MD
Sample : P1189-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc