
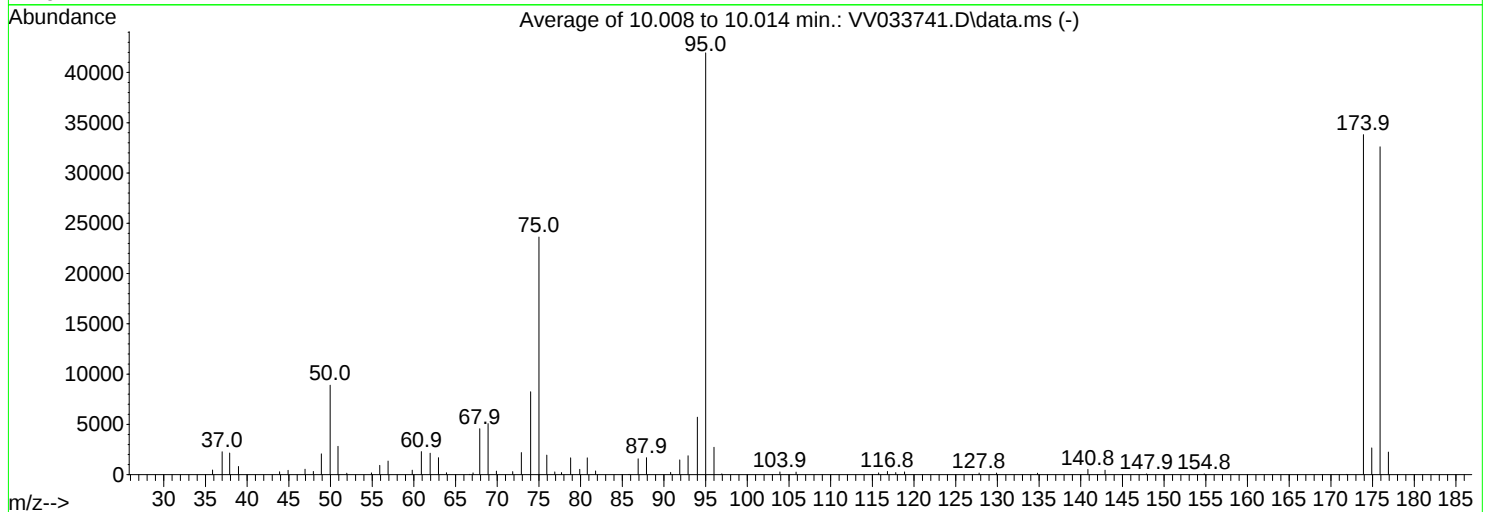


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011924\
Data File : VV033741.D
Acq On : 19 Jan 2024 08:24
Operator : SY/MD
Sample : BFB254
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB254

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Wed Jan 24 02:00:55 2024

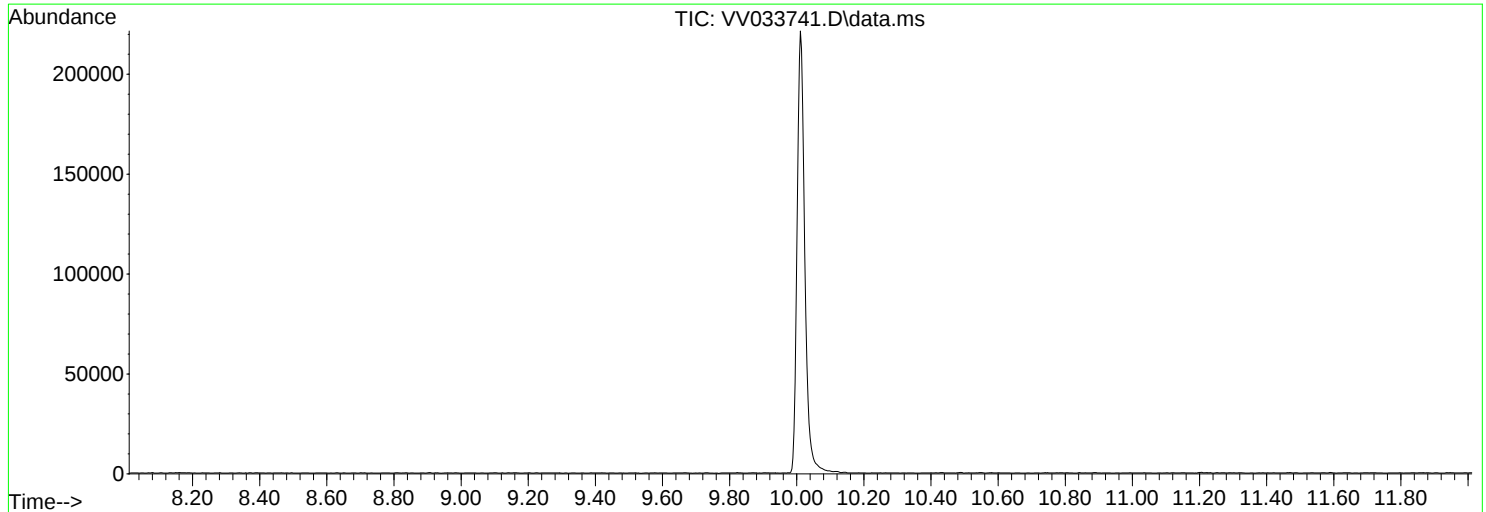

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	8891	PASS
75	95	30	80	56.3	23637	PASS
95	95	100	100	100.0	41949	PASS
96	95	5	9	6.5	2726	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.6	33811	PASS
175	174	5	9	7.9	2660	PASS
176	174	95	105	96.4	32608	PASS
177	176	5	10	6.9	2241	PASS

m/z	Abundance
39.90	280.0
41.00	132.0
43.80	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.90	476.0
37.00	2236.0
37.90	2154.0
39.00	752.0
40.00	214.0
43.90	460.0
44.90	465.0
46.90	584.0
47.90	342.0
48.90	2071.0
49.90	8811.0
50.90	2841.0
51.90	138.0
54.90	162.0
55.90	898.0
56.90	1295.0
59.80	456.0
60.90	2239.0
61.90	2075.0
63.00	1692.0
63.90	204.0
67.10	174.0
67.90	4518.0
68.90	4930.0
69.90	321.0
71.80	281.0
72.90	2236.0
74.00	7984.0
75.00	23240.0
75.90	1907.0
76.90	237.0
77.80	184.0
78.80	1647.0
79.90	526.0
80.80	1660.0
81.80	369.0
85.80	101.0
86.90	1671.0
87.90	1604.0
90.80	226.0
91.90	1359.0
92.90	1841.0
94.00	5449.0
95.00	40552.0
96.00	2748.0
97.00	134.0
103.90	259.0
105.90	267.0
115.80	129.0
116.80	339.0
117.80	195.0
118.80	278.0
127.80	149.0
129.80	133.0
134.80	129.0
140.80	458.0
142.90	425.0
147.90	126.0
154.80	134.0
173.90	32224.0
174.90	2665.0
175.90	30872.0
176.90	2155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.90	468.0
37.00	2359.0
37.90	2211.0
39.00	840.0
39.80	244.0
44.00	477.0
44.90	455.0
47.00	554.0
47.90	331.0
48.90	2166.0
50.00	9140.0
50.90	2901.0
52.00	150.0
54.90	174.0
55.90	983.0
56.90	1389.0
59.80	453.0
60.90	2386.0
62.00	2202.0
63.00	1747.0
63.90	207.0
67.10	168.0
67.90	4672.0
68.90	5273.0
69.90	382.0
71.80	312.0
72.90	2304.0
74.00	8566.0
75.00	24576.0
76.00	2026.0
76.90	287.0
77.70	199.0
78.80	1732.0
79.90	527.0
80.80	1715.0
81.80	398.0
86.90	1588.0
87.90	1772.0
90.80	233.0
91.90	1502.0
92.90	1937.0
94.00	5976.0
95.00	43584.0
96.00	2837.0
96.90	127.0
103.90	304.0
105.80	273.0
115.70	178.0
116.80	312.0
117.80	226.0
118.80	279.0
127.80	157.0
129.90	160.0
134.80	146.0
140.90	542.0
142.90	453.0
147.90	125.0
154.80	124.0
173.90	34960.0
174.90	2739.0
175.90	33816.0
176.90	2309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.80	438.0
37.00	2242.0
37.90	2088.0
38.90	845.0
39.80	252.0
44.00	466.0
44.90	391.0
47.00	500.0
48.00	282.0
48.90	1959.0
50.00	8723.0
50.90	2694.0
52.00	144.0
54.90	180.0
55.90	905.0
56.90	1384.0
59.80	430.0
60.90	2272.0
62.00	2112.0
62.90	1626.0
63.90	177.0
66.70	114.0
67.10	162.0
67.90	4519.0
68.90	5034.0
69.90	357.0
71.90	294.0
72.90	2033.0
74.00	8186.0
75.00	23096.0
76.00	1894.0
76.90	306.0
77.60	218.0
78.80	1627.0
79.90	508.0
80.80	1642.0
81.80	358.0
86.90	1476.0
87.90	1679.0
90.80	209.0
91.90	1523.0
92.90	1851.0
94.00	5709.0
95.00	41712.0
96.00	2594.0
103.90	267.0
105.80	226.0
115.70	219.0
116.80	300.0
117.80	206.0
118.90	271.0
127.80	157.0
130.00	170.0
134.80	134.0
140.90	565.0
142.90	458.0
171.90	122.0
173.90	34248.0
174.90	2576.0
175.90	33136.0
176.90	2258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254