

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020082.D
 Acq On : 20 Jan 2021 17:46
 Operator : SY/MD
 Sample : VIBLK61
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK61

Quant Time: Jan 20 23:41:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 20 23:39:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	374195	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.858	117	363018	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	187828	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	111228	47.38	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.76%
7) Chloroethane-d5	1.569	69	84786	46.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.70%
11) 1,1-Dichloroethene-d2	2.110	63	167597	35.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.48%
21) 2-Butanone-d5	3.891	46	159004	97.19	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.19%
24) Chloroform-d	4.354	84	240440	45.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.72%
26) 1,2-Dichloroethane-d4	5.039	65	166431	47.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.82%
32) Benzene-d6	5.055	84	468281	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.58%
36) 1,2-Dichloropropane-d6	6.074	67	136351	48.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.22%
41) Toluene-d8	7.318	98	429537	47.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.10%
43) trans-1,3-Dichloroprop...	7.627	79	71671	45.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.28%
47) 2-Hexanone-d5	8.093	63	100110	86.43	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.43%
57) 1,1,2,2-Tetrachloroeth...	10.222	84	175090	44.38	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.76%
64) 1,2-Dichlorobenzene-d4	11.633	152	190744	51.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.78%
Target Compounds						
48) 2-Hexanone	8.148	43	8886	3.38	ug/L	Qvalue # 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020082.D
Acq On : 20 Jan 2021 17:46
Operator : SY/MD
Sample : VIBLK61
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK61

Quant Time: Jan 20 23:41:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 20 23:39:20 2021
Response via : Initial Calibration

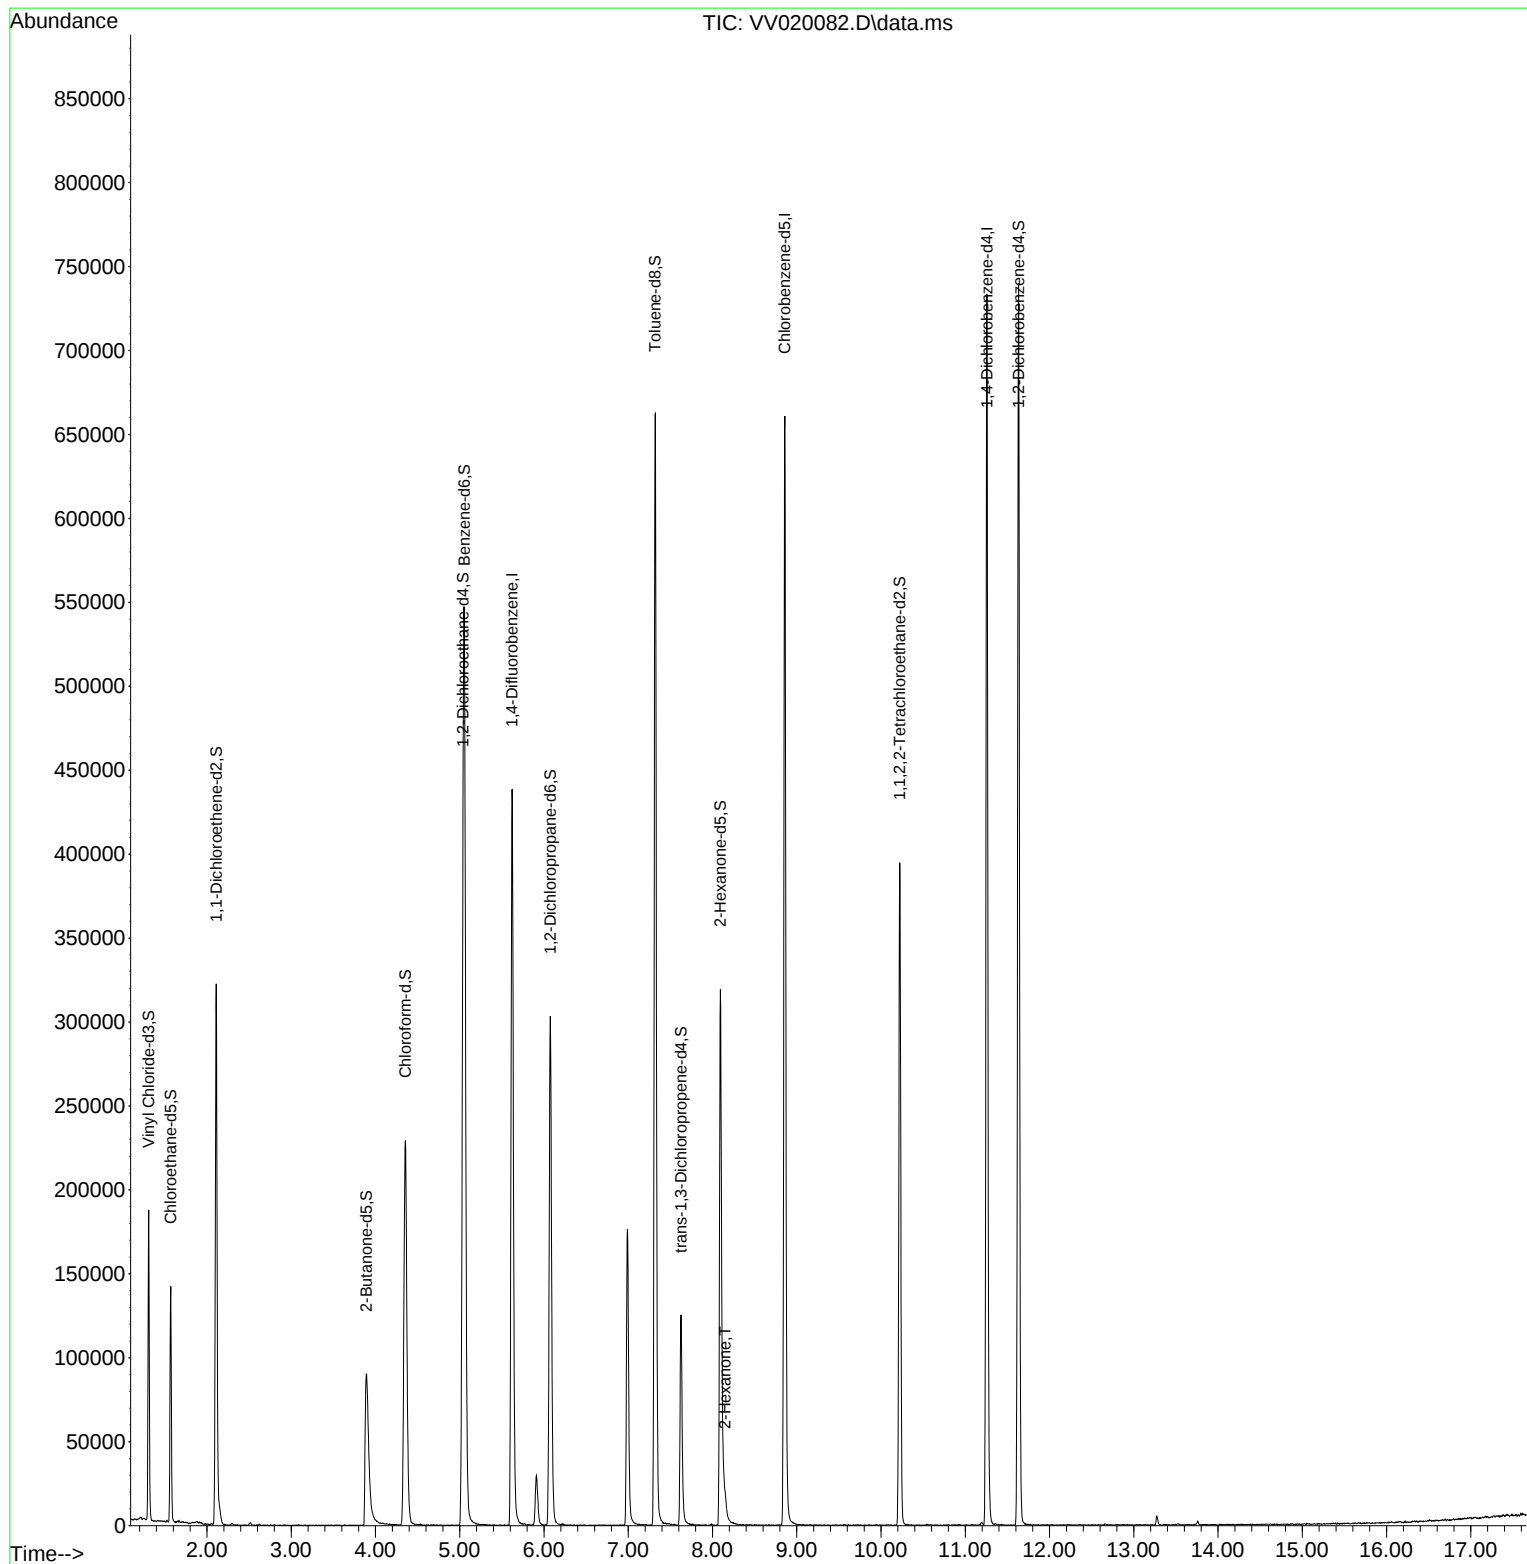

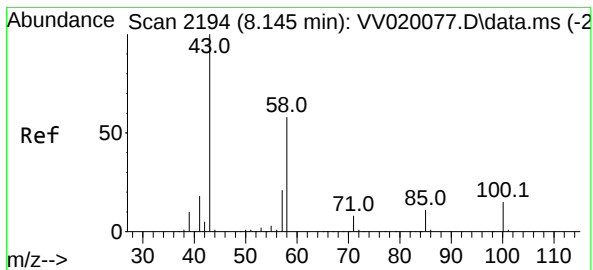

#48
 2-Hexanone
 Concen: 3.38 ug/L
 RT: 8.148 min Scan# 2195
 Delta R.T. 0.003 min
 Lab File: VV020082.D
 Acq: 20 Jan 2021 17:46

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK61

Tgt Ion: 43	Resp: 8886
Ion Ratio	Lower Upper
43	100
58	0.0 41.8 62.6#
57	9.2 15.0 22.4#
100	3.5 8.9 13.3#

