

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020078.D
 Acq On : 20 Jan 2021 16:08
 Operator : SY/MD
 Sample : VV0120MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

Signal : TIC: VV020078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	188274	185067	13.71%	1.747%
2	1.569	142	149	160	rVB	144841	157804	11.69%	1.489%
3	2.110	306	317	346	rVB	312414	468104	34.68%	4.418%
4	2.296	367	375	384	rBV2	2553	3835	0.28%	0.036%
5	2.396	403	406	407	rBV	199	141	0.01%	0.001%
6	2.659	486	488	492	rBV	180	83	0.01%	0.001%
7	2.769	515	522	526	rBV3	958	1268	0.09%	0.012%
8	2.917	565	568	570	rBV	188	119	0.01%	0.001%
9	3.151	638	641	647	rVB	231	149	0.01%	0.001%
10	3.193	648	654	658	rBV	380	409	0.03%	0.004%
11	3.261	673	675	679	rBV2	264	182	0.01%	0.002%
12	3.303	685	688	689	rBV	210	122	0.01%	0.001%
13	3.396	712	717	720	rVB	252	236	0.02%	0.002%
14	3.460	735	737	738	rBV	178	76	0.01%	0.001%
15	3.589	774	777	780	rBV2	204	118	0.01%	0.001%
16	3.621	784	787	792	rVB	272	245	0.02%	0.002%
17	3.643	792	794	796	rBV	208	116	0.01%	0.001%
18	3.708	809	814	817	rBV	314	406	0.03%	0.004%
19	3.798	840	842	845	rVB	297	152	0.01%	0.001%
20	3.814	845	847	848	rBV	258	123	0.01%	0.001%
21	3.833	850	853	855	rVV	196	120	0.01%	0.001%
22	3.897	861	873	906	rBV	85236	259334	19.22%	2.448%
23	4.354	999	1015	1043	rBV	225205	549566	40.72%	5.187%
24	4.724	1127	1130	1133	rBV2	153	93	0.01%	0.001%
25	4.823	1159	1161	1164	rBV2	257	210	0.02%	0.002%
26	4.901	1183	1185	1192	rVB2	324	295	0.02%	0.003%
27	4.936	1192	1196	1200	rBV	270	258	0.02%	0.002%
28	5.052	1215	1232	1266	rBV2	528071	1349587	100.00%	12.737%
29	5.409	1340	1343	1346	rBV2	496	343	0.03%	0.003%
30	5.454	1356	1357	1358	rBV2	117	29	0.00%	0.000%
31	5.527	1375	1380	1382	rBV2	280	263	0.02%	0.002%
32	5.576	1392	1395	1397	rBV	228	119	0.01%	0.001%
33	5.621	1397	1409	1437	rBV	427036	846817	62.75%	7.992%
34	5.910	1488	1499	1517	rBV2	26584	55327	4.10%	0.522%
35	6.019	1529	1533	1537	rBV2	308	331	0.02%	0.003%
36	6.074	1537	1550	1577	rVV	291976	598328	44.33%	5.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020078.D
 Acq On : 20 Jan 2021 16:08
 Operator : SY/MD
 Sample : VV0120MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	6.318	1624	1626	1627	rBV	132	54	0.00%	0.001%
38	6.425	1657	1659	1662	rBV2	225	162	0.01%	0.002%
39	6.479	1674	1676	1678	rBV	213	118	0.01%	0.001%
40	6.515	1685	1687	1690	rBV	195	125	0.01%	0.001%
41	6.527	1690	1691	1693	rBV	205	75	0.01%	0.001%
42	6.614	1716	1718	1720	rVB	205	85	0.01%	0.001%
43	6.711	1745	1748	1749	rBV	175	109	0.01%	0.001%
44	6.759	1759	1763	1765	rBV2	190	158	0.01%	0.001%
45	6.772	1765	1767	1771	rBV2	394	257	0.02%	0.002%
46	6.865	1794	1796	1797	rBV	151	41	0.00%	0.000%
47	6.881	1799	1801	1804	rVB	246	148	0.01%	0.001%
48	6.904	1807	1808	1809	rBB	62	28	0.00%	0.000%
49	6.990	1823	1835	1855	rBV	170297	307598	22.79%	2.903%
50	7.142	1879	1882	1887	rBV3	571	483	0.04%	0.005%
51	7.322	1925	1938	1964	rBV	637642	1106398	81.98%	10.442%
52	7.624	2022	2032	2063	rBV	117586	209826	15.55%	1.980%
53	7.817	2089	2092	2094	rBV	347	273	0.02%	0.003%
54	7.981	2138	2143	2152	rVB5	1716	2236	0.17%	0.021%
55	8.093	2168	2178	2220	rBV2	306834	606879	44.97%	5.728%
56	8.367	2260	2263	2266	rBV2	336	233	0.02%	0.002%
57	8.408	2271	2276	2278	rBV2	328	371	0.03%	0.004%
58	8.653	2349	2352	2353	rBV	166	96	0.01%	0.001%
59	8.859	2404	2416	2438	rBV	632816	1041000	77.13%	9.825%
60	9.344	2564	2567	2571	rVB	227	151	0.01%	0.001%
61	9.466	2604	2605	2606	rBV	217	69	0.01%	0.001%
62	9.556	2629	2633	2636	rBV2	912	790	0.06%	0.007%
63	9.720	2676	2684	2687	rBV	283	491	0.04%	0.005%
64	9.810	2709	2712	2713	rBV2	205	120	0.01%	0.001%
65	10.000	2767	2771	2773	rBV2	347	303	0.02%	0.003%
66	10.071	2790	2793	2796	rBV	291	194	0.01%	0.002%
67	10.119	2805	2808	2811	rBV2	266	162	0.01%	0.002%
68	10.222	2828	2840	2866	rVB	388702	613777	45.48%	5.793%
69	10.447	2907	2910	2911	rBV	232	118	0.01%	0.001%
70	10.643	2967	2971	2972	rBV	219	136	0.01%	0.001%
71	10.807	3020	3022	3025	rBV	247	160	0.01%	0.002%
72	10.836	3029	3031	3032	rVB	258	103	0.01%	0.001%
73	11.029	3089	3091	3097	rBV	254	188	0.01%	0.002%
74	11.196	3135	3143	3150	rVB3	2148	3169	0.23%	0.030%
75	11.257	3150	3162	3187	rBV	699633	1080935	80.09%	10.202%
76	11.630	3266	3278	3299	rBV	713769	1114245	82.56%	10.516%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020078.D
 Acq On : 20 Jan 2021 16:08
 Operator : SY/MD
 Sample : VV0120MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.823	3334	3338	3340	rBV2	347	310	0.02%	0.003%
78	12.141	3435	3437	3439	rBV	276	171	0.01%	0.002%
79	12.656	3590	3597	3610	rVB5	3593	5465	0.40%	0.052%
80	12.710	3610	3614	3616	rBV2	313	296	0.02%	0.003%
81	13.276	3782	3790	3801	rVB7	4166	6502	0.48%	0.061%
82	13.518	3860	3865	3882	rVB3	3593	5908	0.44%	0.056%
83	13.755	3933	3939	3950	rVB5	3560	5281	0.39%	0.050%




Sum of corrected areas: 10595572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020078.D
Acq On : 20 Jan 2021 16:08
Operator : SY/MD
Sample : VV0120MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

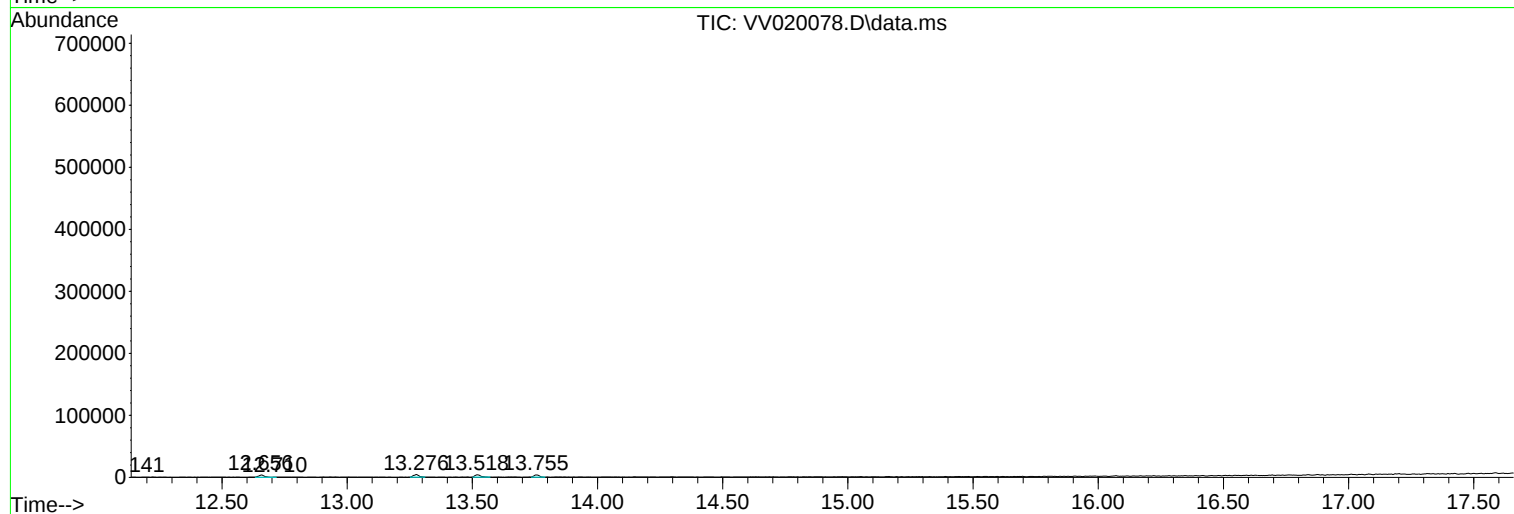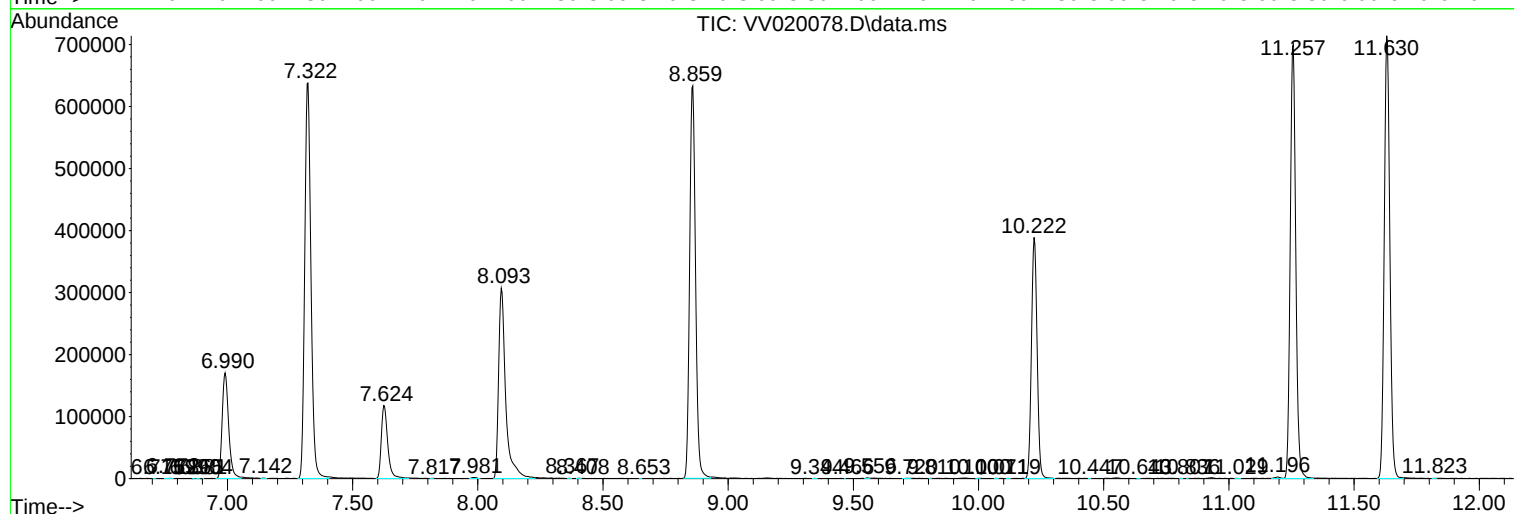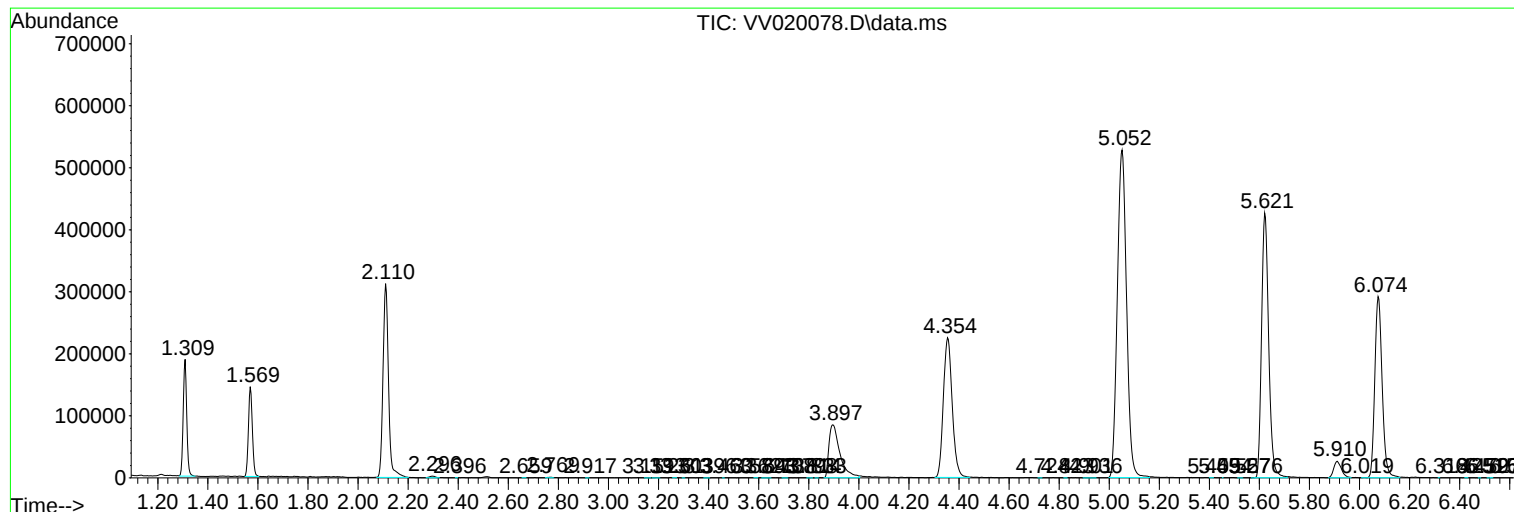

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020078.D
Acq On : 20 Jan 2021 16:08
Operator : SY/MD
Sample : VV0120MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020078.D
Acq On : 20 Jan 2021 16:08
Operator : SY/MD
Sample : VV0120MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
